

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018483.D
 Acq On : 01 Dec 2023 19:03
 Operator : MA/JU
 Sample : 05332-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCGA5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018483.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	38	rVB	79975	95643	0.99%	0.110%
2	3.563	78	81	85	rBV2	10119	14416	0.15%	0.017%
3	3.693	100	103	116	rBV	328644	492668	5.10%	0.568%
4	3.934	139	144	148	rBV	17718	21902	0.23%	0.025%
5	4.028	156	160	165	rBV	23939	31981	0.33%	0.037%
6	4.093	168	171	176	rBV3	5685	9845	0.10%	0.011%
7	4.505	237	241	246	rBV5	7209	10690	0.11%	0.012%
8	5.569	415	422	424	rBV6	8117	12981	0.13%	0.015%
9	7.028	663	670	681	rVB	330240	524339	5.43%	0.605%
10	7.199	693	699	708	rVB	1180649	1839657	19.06%	2.121%
11	7.393	725	732	741	rBV	1106457	1696937	17.58%	1.956%
12	7.475	741	746	752	rBV4	18600	36763	0.38%	0.042%
13	7.863	805	812	820	rBV	1335042	2072399	21.47%	2.389%
14	7.934	820	824	830	rVB3	10284	18241	0.19%	0.021%
15	8.575	926	933	943	rBV	991805	1555611	16.12%	1.794%
16	9.022	1002	1009	1021	rBV	1347936	2221959	23.02%	2.562%
17	9.451	1075	1082	1089	rVB2	30133	57397	0.59%	0.066%
18	9.745	1123	1132	1143	rBV	1060672	1681782	17.42%	1.939%
19	10.281	1215	1223	1231	rBV	1713892	2728720	28.27%	3.146%
20	10.663	1280	1288	1296	rVB	1902811	3159457	32.74%	3.643%
21	10.798	1302	1311	1324	rBV	1273558	2150885	22.29%	2.480%
22	11.322	1394	1400	1403	rBV4	6181	14432	0.15%	0.017%
23	11.945	1500	1506	1512	rBV2	27747	47500	0.49%	0.055%
24	12.251	1553	1558	1562	rBV2	30668	51309	0.53%	0.059%
25	12.857	1659	1661	1667	rBV3	9855	13392	0.14%	0.015%
26	12.957	1674	1678	1682	rBV3	6359	11037	0.11%	0.013%
27	13.116	1700	1705	1708	rBV6	12398	20849	0.22%	0.024%
28	13.334	1737	1742	1747	rVB4	17321	29014	0.30%	0.033%
29	13.398	1747	1753	1761	rBV	84200	143993	1.49%	0.166%
30	13.728	1805	1809	1812	rVB4	8528	10907	0.11%	0.013%
31	13.910	1833	1840	1847	rBV	3761860	5159128	53.45%	5.948%
32	14.186	1880	1887	1895	rVB	3963556	5690464	58.96%	6.561%
33	14.398	1920	1923	1929	rVB5	8104	11693	0.12%	0.013%
34	14.492	1932	1939	1950	rVV	3154933	4687540	48.57%	5.404%
35	14.575	1951	1953	1958	rVB6	9921	11107	0.12%	0.013%
36	14.686	1966	1972	1984	rBV	325289	483829	5.01%	0.558%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018483.D
 Acq On : 01 Dec 2023 19:03
 Operator : MA/JU
 Sample : 05332-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCGA5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	14.910	2006	2010	2017	rVB7	20733	31964	0.33%	0.037%
38	15.298	2071	2076	2077	rBV2	8432	9705	0.10%	0.011%
39	15.486	2101	2108	2116	rBV	5180378	7539121	78.11%	8.692%
40	15.598	2120	2127	2136	rBV	1582354	2134424	22.11%	2.461%
41	15.722	2144	2148	2153	rVB2	25818	40666	0.42%	0.047%
42	16.269	2238	2241	2248	rVB3	14497	23082	0.24%	0.027%
43	16.639	2301	2304	2310	rBV2	17116	23866	0.25%	0.028%
44	16.916	2348	2351	2356	rVB3	9973	15700	0.16%	0.018%
45	17.169	2391	2394	2397	rBV4	18488	19635	0.20%	0.023%
46	17.239	2399	2406	2413	rVV	3990988	5520025	57.19%	6.364%
47	17.339	2416	2423	2434	rVV	6195018	8912767	92.35%	10.276%
48	17.416	2434	2436	2442	rVB5	14933	21044	0.22%	0.024%
49	17.622	2467	2471	2473	rBV3	9085	14939	0.15%	0.017%
50	17.916	2518	2521	2527	rVB	55170	70656	0.73%	0.081%
51	18.004	2534	2536	2542	rVB6	10748	14127	0.15%	0.016%
52	18.133	2553	2558	2566	rBV	323605	479197	4.96%	0.552%
53	18.545	2626	2628	2633	rBV4	12620	15812	0.16%	0.018%
54	19.051	2711	2714	2718	rVB2	65745	68647	0.71%	0.079%
55	19.151	2727	2731	2735	rBV2	90800	120052	1.24%	0.138%
56	19.221	2739	2743	2745	rBV	86412	111591	1.16%	0.129%
57	19.363	2763	2767	2776	rBV2	170277	267369	2.77%	0.308%
58	19.574	2797	2803	2809	rBV	7313640	9651566	100.00%	11.128%
59	21.045	3049	3053	3059	rBV2	193714	294035	3.05%	0.339%
60	21.321	3095	3100	3107	rBV	3515835	4320207	44.76%	4.981%
61	23.545	3471	3478	3486	rBV2	3323262	6432209	66.64%	7.416%
62	23.698	3498	3504	3515	rVB	1959648	3762936	38.99%	4.338%




Sum of corrected areas: 86735809

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018483.D
Acq On : 01 Dec 2023 19:03
Operator : MA/JU
Sample : 05332-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCGA5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

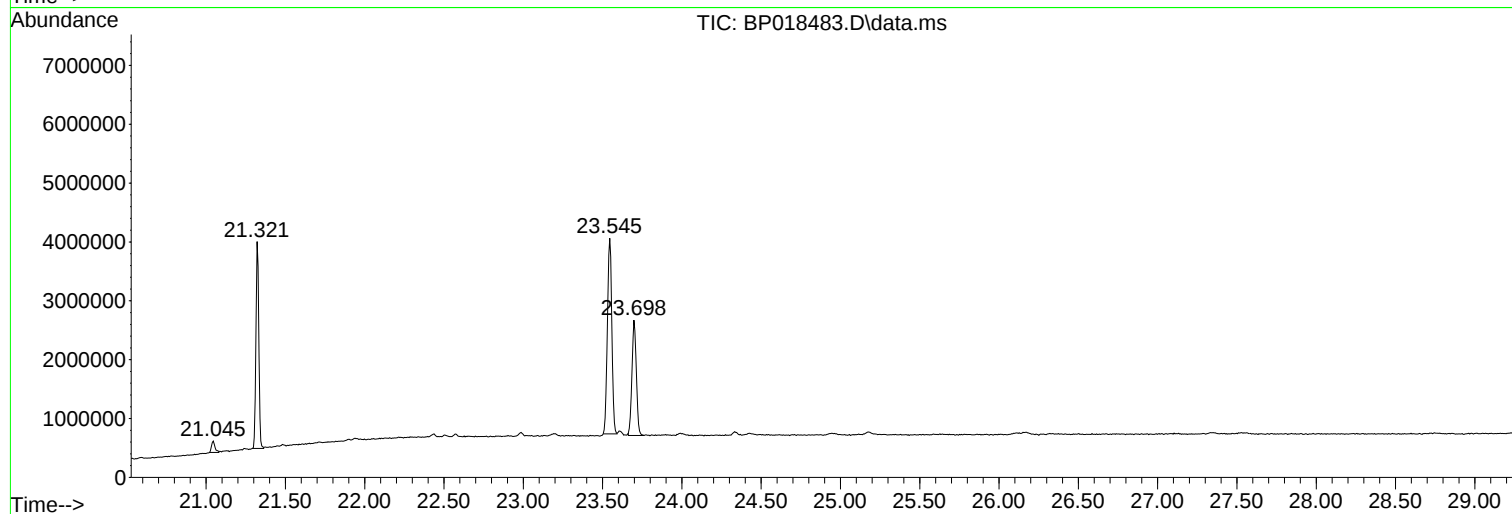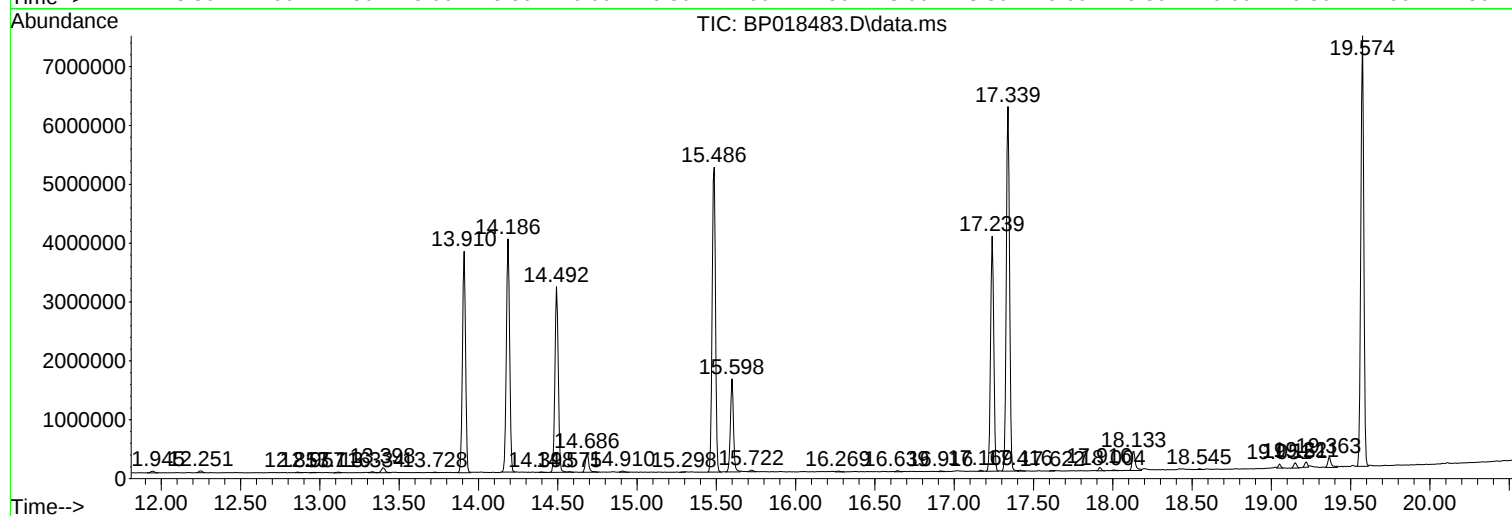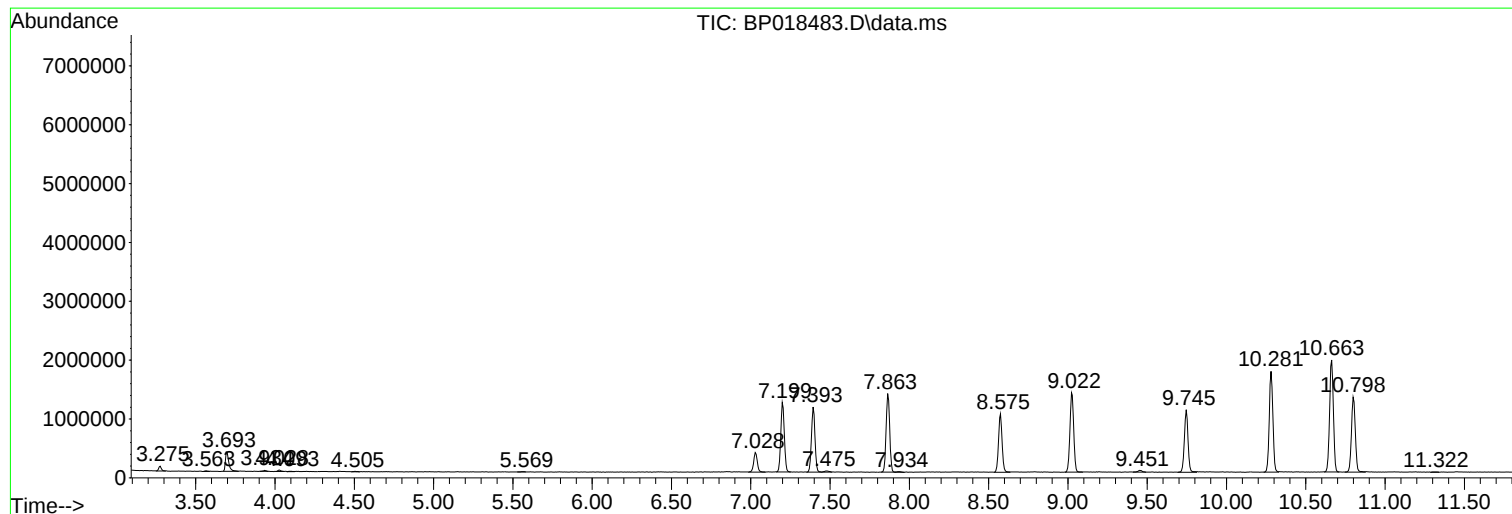

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018483.D
Acq On : 01 Dec 2023 19:03
Operator : MA/JU
Sample : 05332-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCGA5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018483.D
Acq On : 01 Dec 2023 19:03
Operator : MA/JU
Sample : 05332-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCGA5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc