

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018484.D
 Acq On : 01 Dec 2023 19:37
 Operator : MA/JU
 Sample : 05332-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCGA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018484.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.276	28	32	37	rVB	65626	77109	0.96%	0.093%
2	3.693	100	103	115	rBV	406127	591619	7.34%	0.713%
3	3.940	140	145	147	rBV2	16324	22372	0.28%	0.027%
4	4.028	156	160	165	rVB2	22418	31628	0.39%	0.038%
5	4.564	246	251	258	rVB2	29831	51243	0.64%	0.062%
6	5.570	416	422	423	rBV2	5744	9170	0.11%	0.011%
7	6.846	636	639	645	rBV2	6355	10041	0.12%	0.012%
8	7.028	663	670	679	rVB	311266	481825	5.98%	0.580%
9	7.199	692	699	710	rVB	1309298	1981865	24.60%	2.387%
10	7.393	725	732	739	rBV	1129999	1753888	21.77%	2.112%
11	7.487	744	748	753	rBV2	10919	19655	0.24%	0.024%
12	7.864	804	812	820	rBV	1293320	2002728	24.86%	2.412%
13	8.575	925	933	942	rBV	920320	1458682	18.11%	1.757%
14	9.022	1002	1009	1020	rBV	1470169	2373468	29.46%	2.859%
15	9.452	1078	1082	1087	rVB3	24609	39856	0.49%	0.048%
16	9.746	1123	1132	1143	rBV	1098727	1745909	21.67%	2.103%
17	9.975	1167	1171	1176	rVB4	7734	14789	0.18%	0.018%
18	10.281	1215	1223	1232	rBV	1772368	2914986	36.19%	3.511%
19	10.663	1278	1288	1295	rBV	1781862	2945677	36.57%	3.548%
20	10.799	1304	1311	1320	rBV	1391775	2305778	28.62%	2.777%
21	11.946	1499	1506	1510	rBV2	12483	24193	0.30%	0.029%
22	12.246	1552	1557	1564	rVB3	32721	57042	0.71%	0.069%
23	12.457	1589	1593	1597	rBV4	5116	8245	0.10%	0.010%
24	12.857	1656	1661	1665	rBV3	8759	15914	0.20%	0.019%
25	13.116	1701	1705	1709	rVB6	8831	15362	0.19%	0.019%
26	13.399	1747	1753	1759	rBV3	45140	77718	0.96%	0.094%
27	13.457	1759	1763	1771	rVV4	9573	18737	0.23%	0.023%
28	13.910	1831	1840	1847	rBV	3835509	5399442	67.03%	6.503%
29	14.187	1879	1887	1896	rBV	4014013	5996290	74.44%	7.222%
30	14.493	1931	1939	1949	rBV	2844789	4202799	52.17%	5.062%
31	14.575	1951	1953	1958	rVB2	12913	14000	0.17%	0.017%
32	14.687	1964	1972	1982	rBV	232413	371042	4.61%	0.447%
33	14.904	2005	2009	2014	rBV3	17562	29335	0.36%	0.035%
34	15.487	2101	2108	2114	rBV	5355988	7840516	97.33%	9.443%
35	15.598	2120	2127	2137	rBV	1388548	1881261	23.35%	2.266%
36	15.722	2144	2148	2156	rVB3	27220	45373	0.56%	0.055%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018484.D
 Acq On : 01 Dec 2023 19:37
 Operator : MA/JU
 Sample : 05332-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCGA7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	16.051	2199	2204	2209	rBV4	8739	18035	0.22%	0.022%
38	16.269	2237	2241	2245	rVB4	10676	18493	0.23%	0.022%
39	16.645	2301	2305	2310	rBV5	11277	15445	0.19%	0.019%
40	16.916	2349	2351	2356	rVB4	11081	13335	0.17%	0.016%
41	17.240	2399	2406	2412	rBV	3197659	4479557	55.61%	5.395%
42	17.340	2416	2423	2432	rBV	5498688	8018380	99.54%	9.658%
43	18.128	2553	2557	2563	rBV	222568	283897	3.52%	0.342%
44	19.151	2727	2731	2737	rVB2	75568	97997	1.22%	0.118%
45	19.216	2738	2742	2746	rBV	76800	108813	1.35%	0.131%
46	19.363	2763	2767	2771	rBV3	113021	132262	1.64%	0.159%
47	19.575	2797	2803	2809	rBV	6085032	8055363	100.00%	9.702%
48	21.045	3049	3053	3060	rBV3	110551	177243	2.20%	0.213%
49	21.322	3095	3100	3106	rBV	2882388	3598748	44.68%	4.334%
50	23.545	3471	3478	3486	rBV2	3900659	7239159	89.87%	8.719%
51	23.698	3497	3504	3515	rVB	1927030	3940900	48.92%	4.747%




Sum of corrected areas: 83027184

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018484.D
Acq On : 01 Dec 2023 19:37
Operator : MA/JU
Sample : 05332-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCGA7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

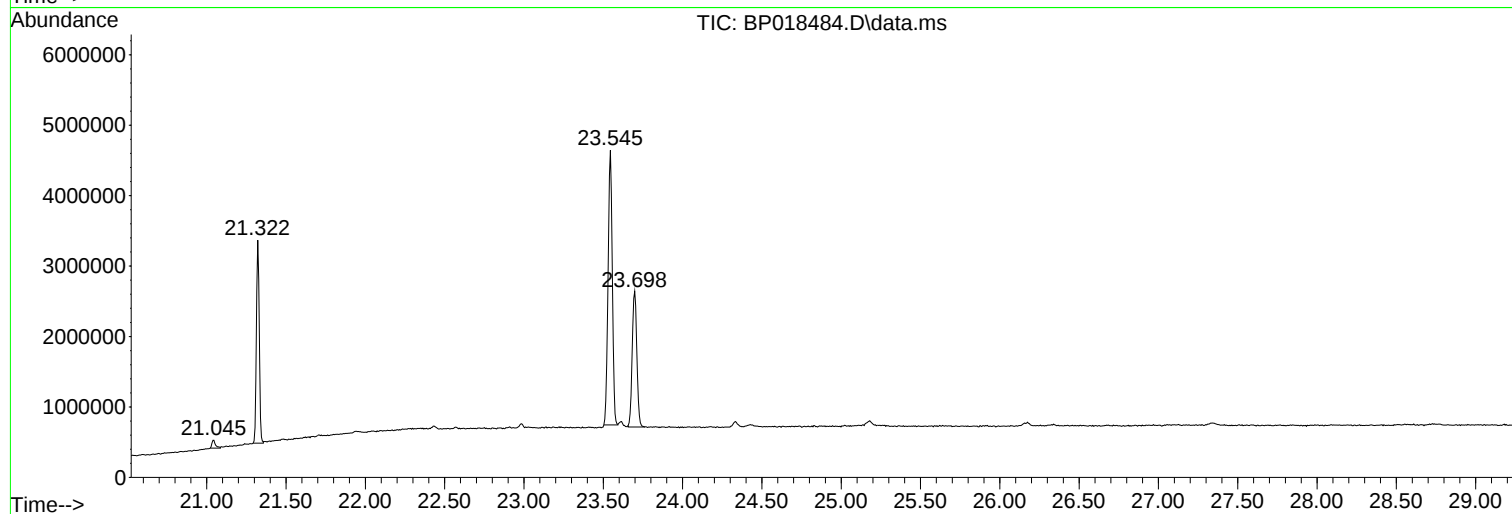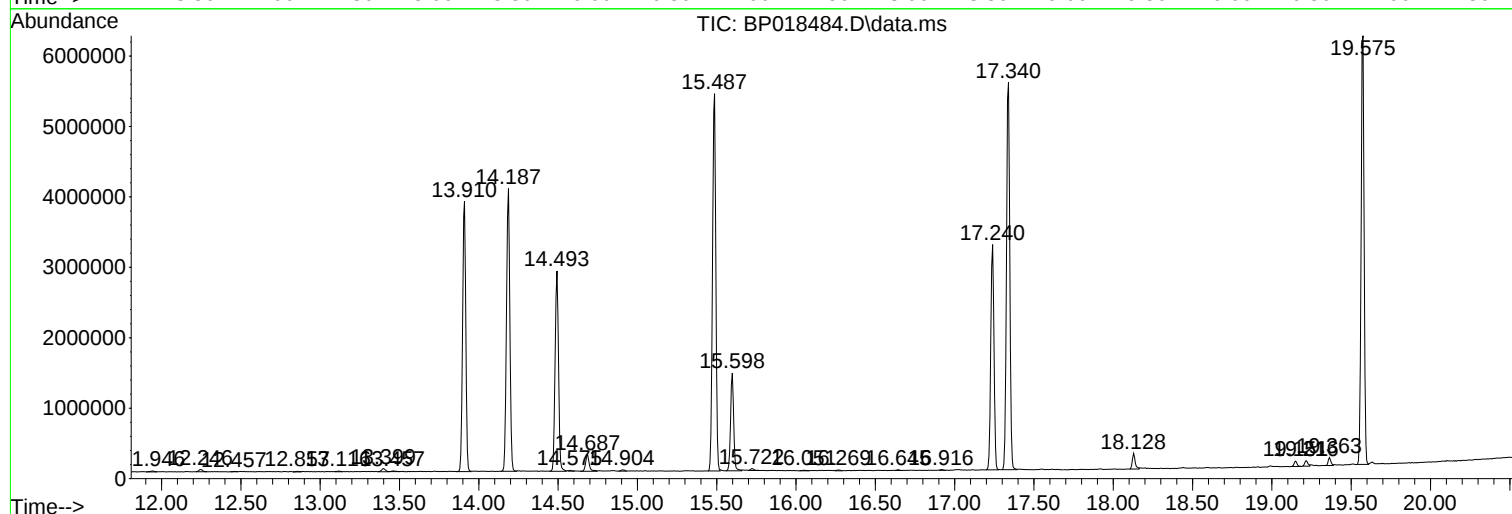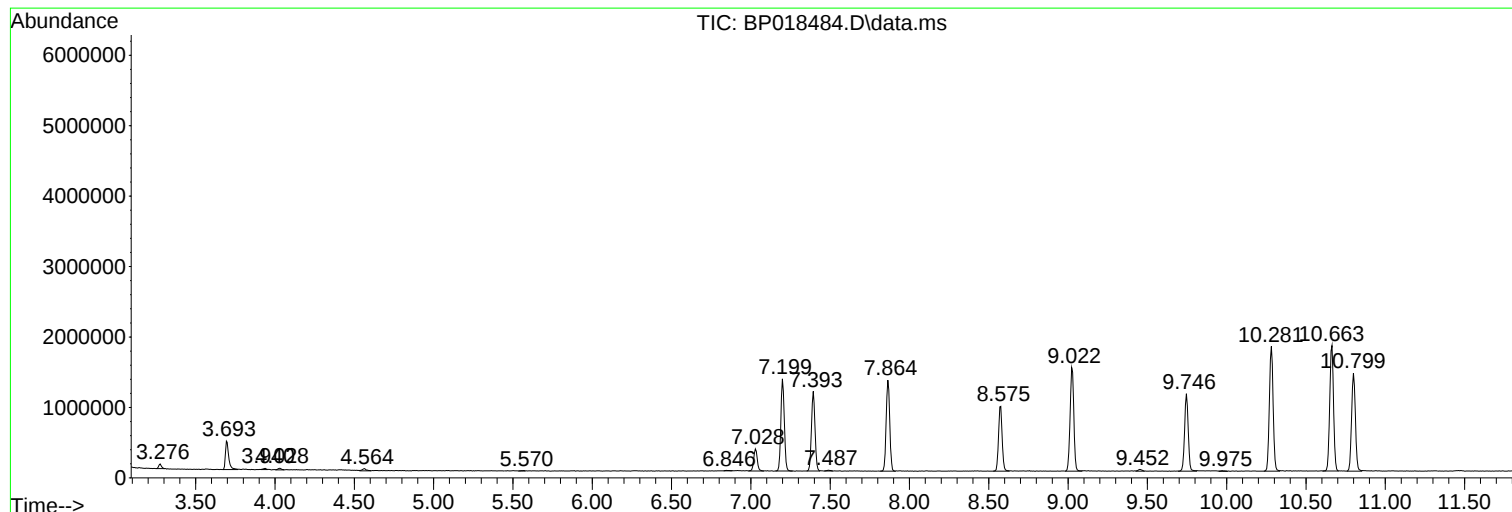

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018484.D
Acq On : 01 Dec 2023 19:37
Operator : MA/JU
Sample : 05332-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCGA7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018484.D
Acq On : 01 Dec 2023 19:37
Operator : MA/JU
Sample : 05332-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCGA7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc