

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018486.D
 Acq On : 01 Dec 2023 20:45
 Operator : MA/JU
 Sample : 05332-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCG41

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018486.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	38	rVB	63096	80135	0.73%	0.087%
2	3.693	100	103	115	rBV	366842	542674	4.95%	0.589%
3	3.934	140	144	148	rVB	21949	26502	0.24%	0.029%
4	4.022	156	159	164	rBV2	19795	28154	0.26%	0.031%
5	5.569	413	422	425	rBV4	8781	18802	0.17%	0.020%
6	7.028	663	670	679	rVB	300755	479135	4.37%	0.520%
7	7.199	692	699	711	rVB	1214278	1877508	17.14%	2.037%
8	7.393	724	732	745	rBV	1107663	1701743	15.53%	1.847%
9	7.487	745	748	752	rVV4	8003	11472	0.10%	0.012%
10	7.863	804	812	820	rBV	1240854	1913661	17.47%	2.077%
11	8.575	926	933	945	rBV	910189	1446688	13.20%	1.570%
12	9.022	1001	1009	1017	rBV	1369197	2232456	20.38%	2.423%
13	9.452	1077	1082	1088	rVB2	41480	71174	0.65%	0.077%
14	9.746	1124	1132	1141	rBV	1055604	1676232	15.30%	1.819%
15	10.281	1215	1223	1234	rBV	1695493	2751697	25.12%	2.986%
16	10.616	1274	1280	1281	rBV4	7357	13083	0.12%	0.014%
17	10.663	1281	1288	1296	rVB	1757029	2907811	26.54%	3.155%
18	10.799	1304	1311	1320	rBV	1583626	2622447	23.94%	2.846%
19	10.928	1328	1333	1339	rVB4	14751	31650	0.29%	0.034%
20	11.451	1418	1422	1425	rBV6	7576	13071	0.12%	0.014%
21	11.940	1501	1505	1510	rBV3	16786	27388	0.25%	0.030%
22	12.246	1552	1557	1564	rBV3	31010	56865	0.52%	0.062%
23	13.340	1738	1743	1748	rVB4	8801	15921	0.15%	0.017%
24	13.398	1748	1753	1759	rBV	58901	91118	0.83%	0.099%
25	13.469	1761	1765	1769	rVB5	6733	12115	0.11%	0.013%
26	13.910	1833	1840	1848	rBV	3758539	5244849	47.87%	5.692%
27	14.187	1880	1887	1896	rBV	3956661	5851699	53.41%	6.350%
28	14.492	1932	1939	1949	rBV	3054674	4479901	40.89%	4.861%
29	14.687	1966	1972	1981	rBV	345172	498290	4.55%	0.541%
30	14.910	2007	2010	2015	rVV6	15116	19482	0.18%	0.021%
31	15.116	2041	2045	2050	rBV6	10390	16802	0.15%	0.018%
32	15.292	2072	2075	2078	rBV4	10262	12617	0.12%	0.014%
33	15.481	2101	2107	2118	rVB	5331754	7810026	71.29%	8.475%
34	15.598	2121	2127	2138	rBV	1696491	2266499	20.69%	2.460%
35	15.722	2144	2148	2155	rVB4	26774	46070	0.42%	0.050%
36	16.051	2201	2204	2209	rBV6	8780	12549	0.11%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018486.D
 Acq On : 01 Dec 2023 20:45
 Operator : MA/JU
 Sample : 05332-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCG41

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	16.263	2238	2240	2247	rVB6	11684	17324	0.16%	0.019%
38	16.345	2247	2254	2259	rBV8	8955	20914	0.19%	0.023%
39	16.639	2302	2304	2308	rBV4	11127	13237	0.12%	0.014%
40	17.239	2399	2406	2413	rBV	3917691	5466966	49.90%	5.933%
41	17.339	2416	2423	2434	rBV	6548565	9382488	85.64%	10.182%
42	18.128	2552	2557	2565	rBV2	219399	329304	3.01%	0.357%
43	19.151	2727	2731	2736	rVB2	94637	118825	1.08%	0.129%
44	19.216	2738	2742	2746	rBV	101945	131006	1.20%	0.142%
45	19.363	2763	2767	2773	rBV	138974	187980	1.72%	0.204%
46	19.575	2797	2803	2809	rBV	8278336	10955777	100.00%	11.889%
47	21.322	3095	3100	3106	rBV	4107840	5266786	48.07%	5.715%
48	23.545	3471	3478	3486	rBV2	4463180	8659829	79.04%	9.397%
49	23.698	3498	3504	3515	rVB	2316242	4692656	42.83%	5.092%




Sum of corrected areas: 92151378

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018486.D
Acq On : 01 Dec 2023 20:45
Operator : MA/JU
Sample : 05332-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCG41

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

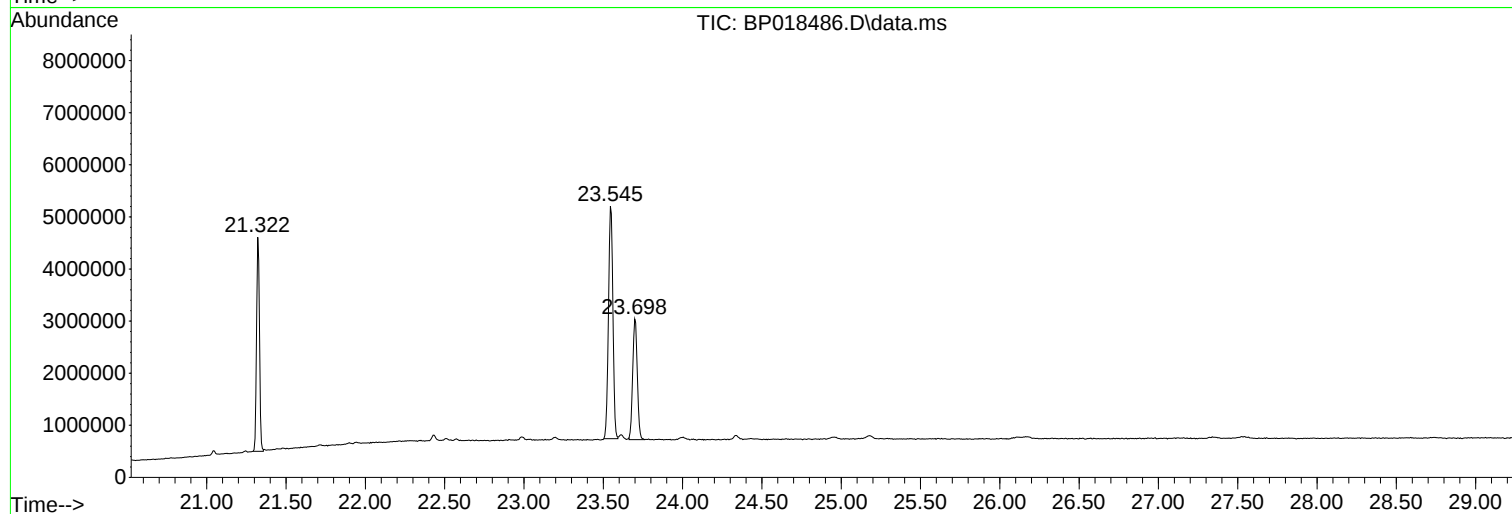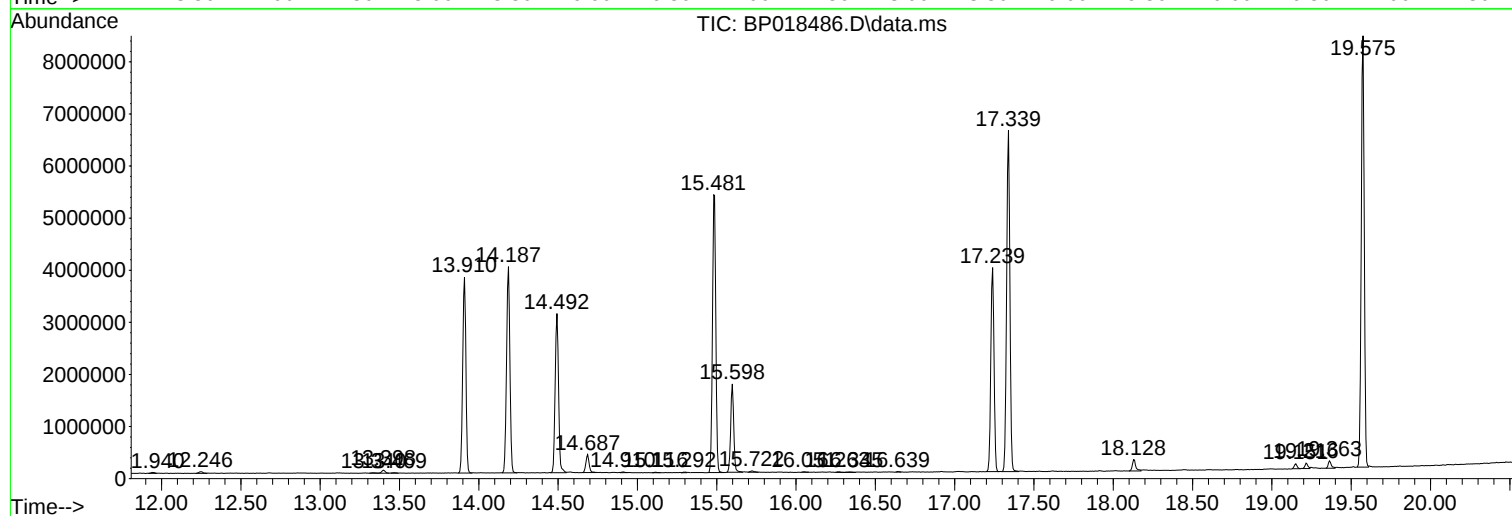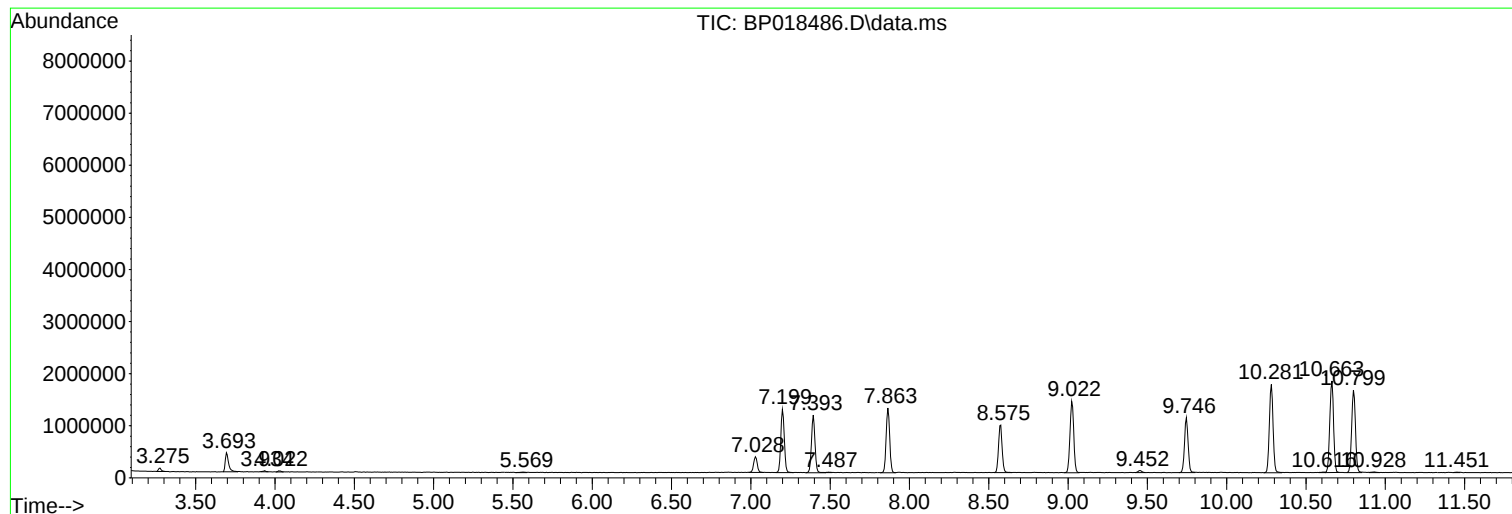

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018486.D
Acq On : 01 Dec 2023 20:45
Operator : MA/JU
Sample : 05332-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCG41

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018486.D
Acq On : 01 Dec 2023 20:45
Operator : MA/JU
Sample : 05332-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCG41

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------