

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018487.D
 Acq On : 01 Dec 2023 21:19
 Operator : MA/JU
 Sample : 05332-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCG62

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018487.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	28	32	38	rVB	63605	85296	1.13%	0.118%
2	3.693	99	103	115	rBV	385335	547339	7.24%	0.760%
3	3.934	140	144	148	rVB2	16892	23993	0.32%	0.033%
4	4.022	156	159	166	rBV2	20703	28804	0.38%	0.040%
5	6.728	612	619	622	rBV2	4060	8720	0.12%	0.012%
6	7.028	664	670	680	rVB	268025	415449	5.49%	0.577%
7	7.199	688	699	707	rBV	1189754	1811331	23.95%	2.514%
8	7.393	724	732	739	rBV	1038024	1579473	20.88%	2.192%
9	7.493	746	749	754	rVB6	8981	11787	0.16%	0.016%
10	7.863	805	812	820	rVV	1083819	1681520	22.23%	2.333%
11	7.928	820	823	827	rVB4	5564	7600	0.10%	0.011%
12	8.575	925	933	942	rBV	777695	1256069	16.61%	1.743%
13	9.022	1002	1009	1019	rBV	1326879	2101314	27.78%	2.916%
14	9.452	1078	1082	1088	rVB3	19895	30416	0.40%	0.042%
15	9.746	1122	1132	1141	rBV	957205	1526176	20.18%	2.118%
16	9.899	1156	1158	1163	rVB2	5802	8010	0.11%	0.011%
17	9.969	1165	1170	1172	rBV5	6000	10814	0.14%	0.015%
18	10.281	1216	1223	1236	rVB	1503635	2428411	32.11%	3.370%
19	10.663	1279	1288	1296	rBV	1446507	2432401	32.16%	3.375%
20	10.799	1302	1311	1320	rBV	1340629	2284075	30.20%	3.170%
21	11.222	1377	1383	1385	rBV2	3875	7616	0.10%	0.011%
22	11.946	1500	1506	1510	rBV2	6278	11670	0.15%	0.016%
23	12.246	1550	1557	1562	rBV2	29770	51865	0.69%	0.072%
24	13.104	1702	1703	1706	rBV3	6459	7951	0.11%	0.011%
25	13.328	1738	1741	1744	rVB2	8684	9357	0.12%	0.013%
26	13.398	1749	1753	1759	rVB3	40830	66885	0.88%	0.093%
27	13.463	1759	1764	1767	rBV3	9055	14319	0.19%	0.020%
28	13.910	1833	1840	1846	rBV	3280498	4313008	57.03%	5.985%
29	14.187	1876	1887	1894	rBV	3488872	4947736	65.42%	6.866%
30	14.492	1932	1939	1949	rBV	2253189	3334782	44.09%	4.628%
31	14.687	1965	1972	1983	rBV	206497	335133	4.43%	0.465%
32	14.904	2007	2009	2014	rVB4	13006	18334	0.24%	0.025%
33	15.487	2098	2108	2114	rBV	4568887	6548782	86.59%	9.088%
34	15.598	2120	2127	2137	rBV	1200148	1614271	21.34%	2.240%
35	15.722	2144	2148	2155	rVB4	25504	40606	0.54%	0.056%
36	16.263	2238	2240	2244	rVV4	7987	10758	0.14%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018487.D
 Acq On : 01 Dec 2023 21:19
 Operator : MA/JU
 Sample : 05332-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCG62

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	17.116	2379	2385	2388	rBV4	7658	17746	0.23%	0.025%
38	17.239	2400	2406	2412	rBV	2501311	3601899	47.63%	4.998%
39	17.339	2416	2423	2433	rVV2	4870269	7192852	95.11%	9.981%
40	17.922	2518	2522	2527	rBV6	9214	14784	0.20%	0.021%
41	18.128	2553	2557	2564	rBV2	108774	159337	2.11%	0.221%
42	19.151	2727	2731	2736	rVB2	63762	81995	1.08%	0.114%
43	19.216	2738	2742	2746	rBV	66178	86389	1.14%	0.120%
44	19.363	2763	2767	2772	rBV4	65465	81160	1.07%	0.113%
45	19.575	2797	2803	2809	rBV	5596349	7562769	100.00%	10.495%
46	21.322	3095	3100	3107	rBV	2502015	3103008	41.03%	4.306%
47	23.545	3471	3478	3486	rBV2	3720161	7173477	94.85%	9.955%
48	23.698	3498	3504	3516	rVB	1666886	3374783	44.62%	4.683%




Sum of corrected areas: 72062270

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018487.D
Acq On : 01 Dec 2023 21:19
Operator : MA/JU
Sample : 05332-11
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCG62

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

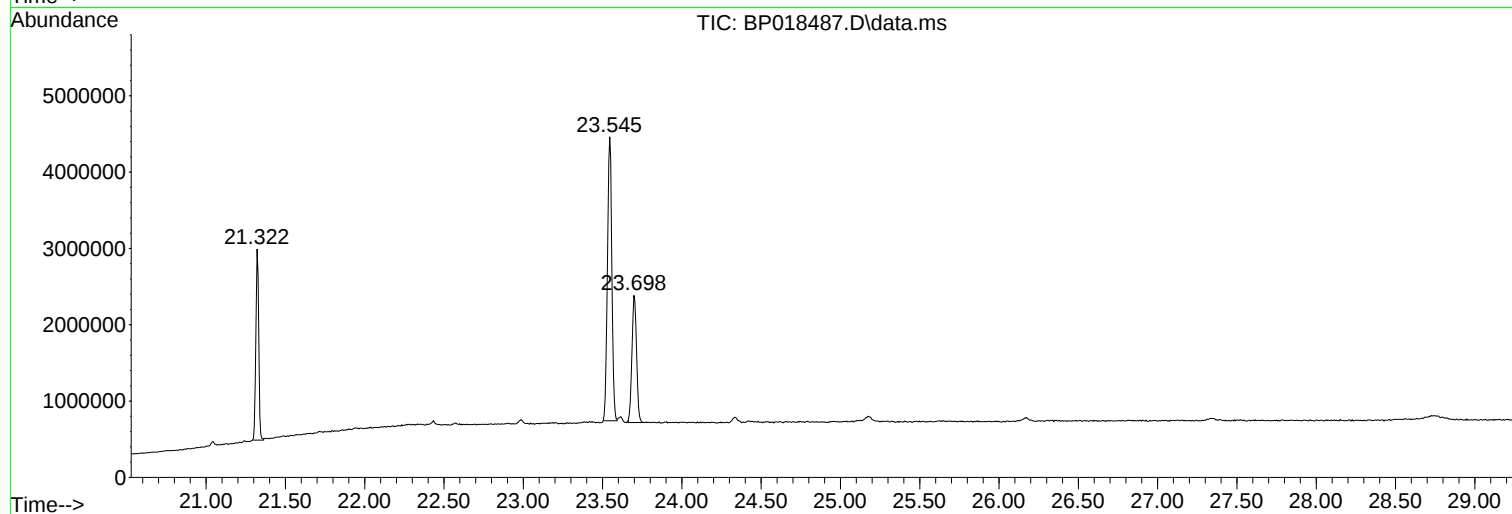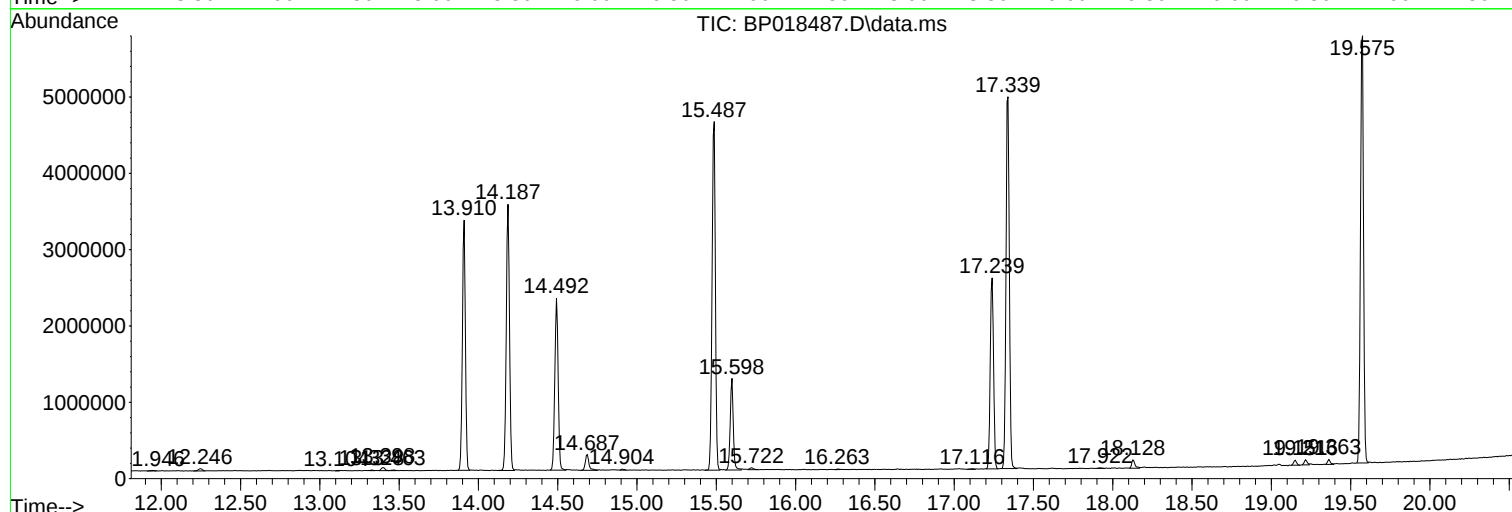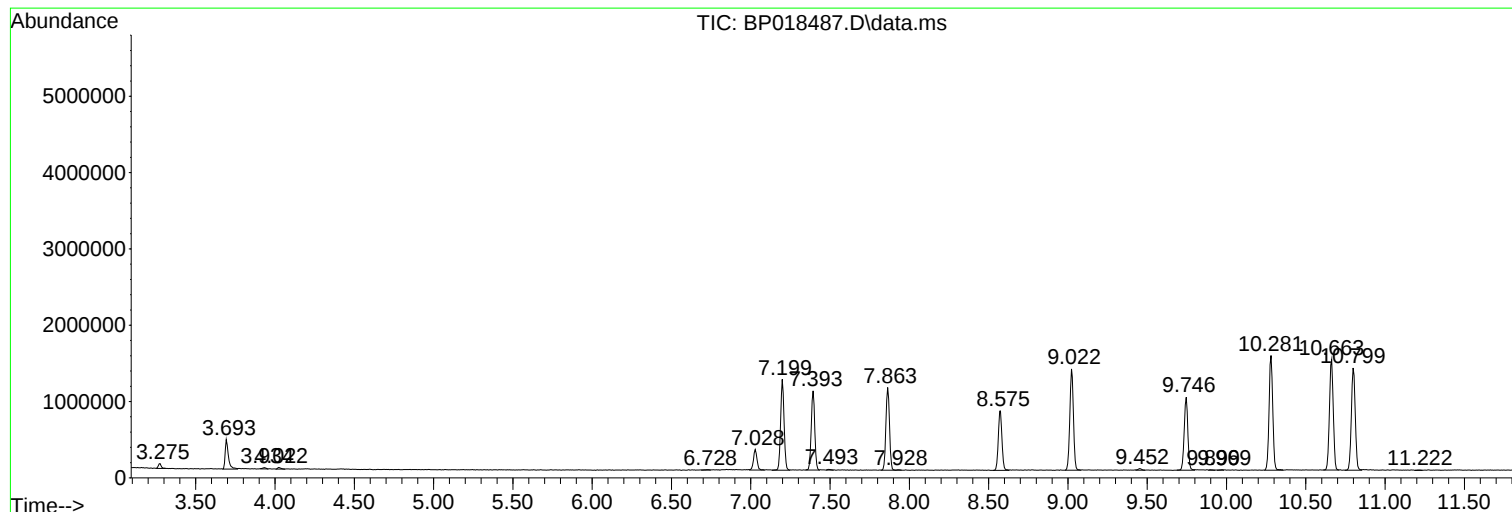

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018487.D
Acq On : 01 Dec 2023 21:19
Operator : MA/JU
Sample : 05332-11
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCG62

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018487.D
Acq On : 01 Dec 2023 21:19
Operator : MA/JU
Sample : 05332-11
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCG62

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------