

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018490.D
 Acq On : 01 Dec 2023 23:02
 Operator : MA/JU
 Sample : 05332-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCG52

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018490.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	28	31	38	rVB	74229	96923	1.21%	0.129%
2	3.693	99	103	114	rBV	439003	607854	7.61%	0.809%
3	3.934	139	144	148	rBV2	21138	31923	0.40%	0.043%
4	4.028	155	160	165	rBV2	21365	35681	0.45%	0.048%
5	6.834	634	637	639	rBV	6088	8709	0.11%	0.012%
6	7.028	663	670	679	rVB	276990	419425	5.25%	0.559%
7	7.199	692	699	706	rBV	1216393	1843521	23.09%	2.455%
8	7.393	725	732	742	rVV	1041732	1607492	20.14%	2.141%
9	7.493	746	749	754	rVB2	8379	10663	0.13%	0.014%
10	7.863	806	812	819	rVB	1081027	1662554	20.83%	2.214%
11	8.569	924	932	941	rBV	839122	1301983	16.31%	1.734%
12	9.022	1001	1009	1017	rBV	1367307	2198803	27.54%	2.928%
13	9.452	1078	1082	1086	rVB2	13766	17693	0.22%	0.024%
14	9.746	1125	1132	1139	rBV	961034	1531969	19.19%	2.040%
15	10.281	1214	1223	1231	rBV	1541563	2493833	31.24%	3.321%
16	10.663	1279	1288	1298	rVB	1456365	2485838	31.14%	3.310%
17	10.799	1300	1311	1319	rBV	1445957	2426009	30.39%	3.231%
18	11.946	1500	1506	1512	rVB5	12694	24955	0.31%	0.033%
19	12.187	1543	1547	1551	rVB2	13470	17886	0.22%	0.024%
20	12.246	1551	1557	1565	rBV2	32353	54101	0.68%	0.072%
21	13.116	1702	1705	1711	rVB3	12947	20558	0.26%	0.027%
22	13.398	1747	1753	1757	rBV3	25551	43749	0.55%	0.058%
23	13.463	1761	1764	1770	rVB4	8381	10633	0.13%	0.014%
24	13.816	1822	1824	1829	rVB	5485	8412	0.11%	0.011%
25	13.910	1833	1840	1847	rVV	3419329	4696433	58.83%	6.254%
26	14.187	1878	1887	1895	rBV	3717891	5400167	67.65%	7.191%
27	14.493	1932	1939	1948	rBV	2360402	3510776	43.98%	4.675%
28	14.687	1966	1972	1981	rBV	216196	329207	4.12%	0.438%
29	14.851	1996	2000	2005	rVB4	5954	9205	0.12%	0.012%
30	14.910	2005	2010	2016	rVB5	12243	19863	0.25%	0.026%
31	15.481	2099	2107	2118	rBV	4947661	7165625	89.76%	9.543%
32	15.598	2120	2127	2137	rBV	1196714	1653905	20.72%	2.203%
33	15.722	2143	2148	2154	rVB3	23186	40950	0.51%	0.055%
34	16.269	2235	2241	2246	rBV8	8150	16402	0.21%	0.022%
35	16.916	2347	2351	2354	rBV3	9798	12609	0.16%	0.017%
36	17.028	2366	2370	2373	rBV4	8343	13634	0.17%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018490.D
 Acq On : 01 Dec 2023 23:02
 Operator : MA/JU
 Sample : 05332-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCG52

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	17.239	2399	2406	2412	rBV	2839569	4010860	50.24%	5.341%
38	17.339	2416	2423	2436	rBV	5363134	7656656	95.91%	10.196%
39	18.128	2553	2557	2562	rBV4	47305	69509	0.87%	0.093%
40	19.151	2727	2731	2738	rVB2	66188	86688	1.09%	0.115%
41	19.216	2738	2742	2749	rBV	70833	109280	1.37%	0.146%
42	19.363	2764	2767	2771	rBV6	40781	50780	0.64%	0.068%
43	19.575	2797	2803	2810	rBV	5984368	7982944	100.00%	10.631%
44	21.322	3095	3100	3108	rBV	2657002	3354238	42.02%	4.467%
45	23.545	3471	3478	3486	rBV2	3528901	6650246	83.31%	8.856%
46	23.698	3498	3504	3513	rVB	1685445	3290348	41.22%	4.382%




Sum of corrected areas: 75091492

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018490.D
Acq On : 01 Dec 2023 23:02
Operator : MA/JU
Sample : 05332-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCG52

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

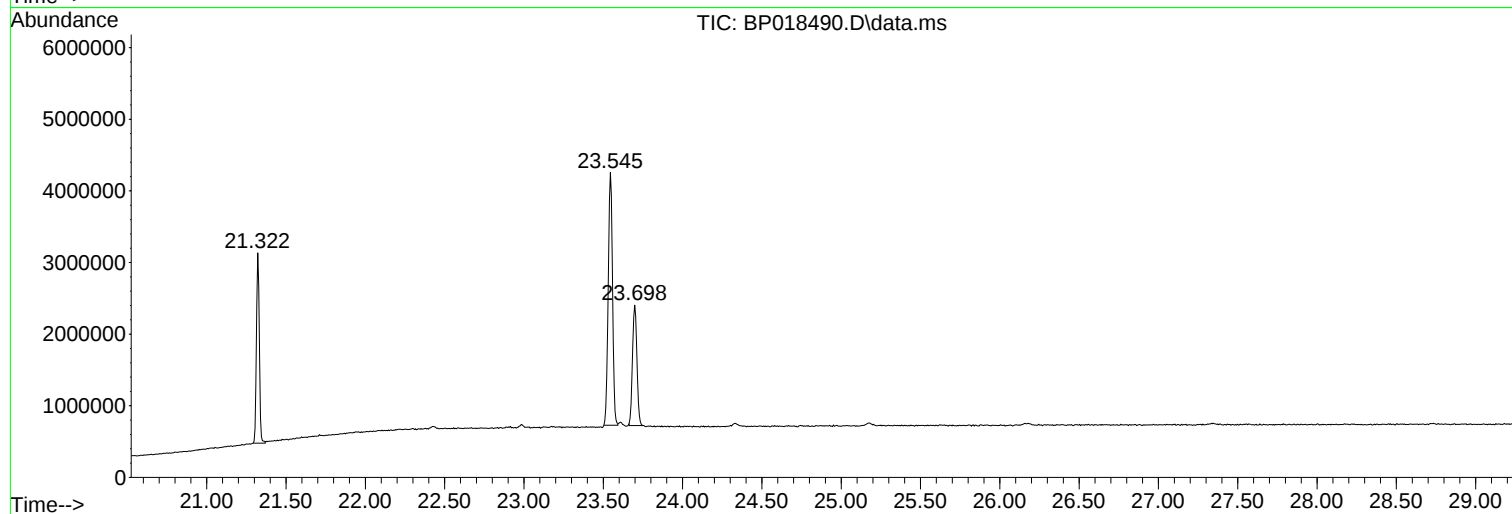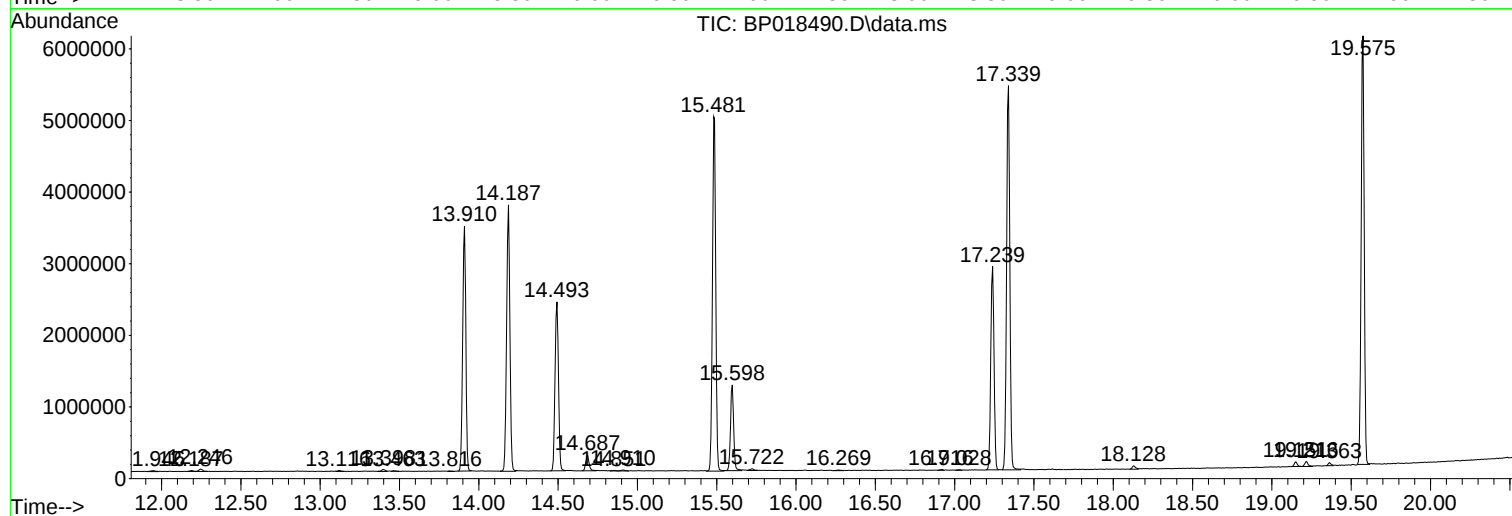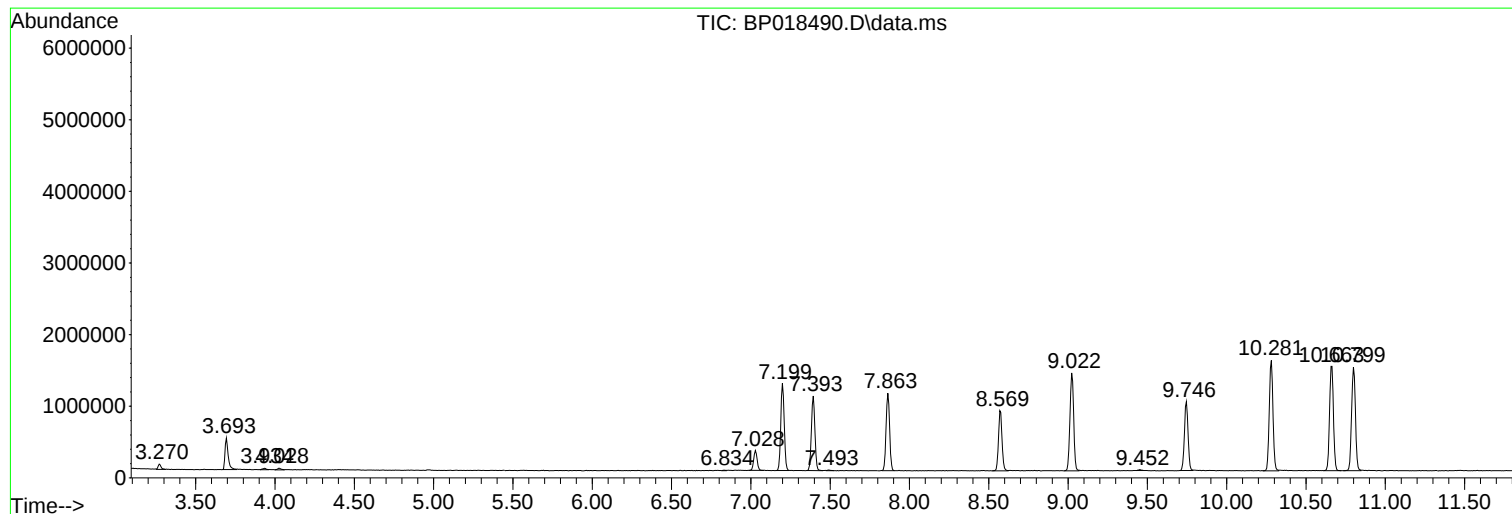

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018490.D
Acq On : 01 Dec 2023 23:02
Operator : MA/JU
Sample : 05332-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCG52

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018490.D
Acq On : 01 Dec 2023 23:02
Operator : MA/JU
Sample : 05332-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCG52

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------