

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018491.D
 Acq On : 01 Dec 2023 23:36
 Operator : MA/JU
 Sample : 05332-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCG73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018491.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	37	rVB	62874	81987	1.17%	0.133%
2	3.528	72	75	78	rBV3	5252	8127	0.12%	0.013%
3	3.693	100	103	112	rBV	211242	296620	4.22%	0.481%
4	3.934	138	144	149	rBV2	18389	26495	0.38%	0.043%
5	4.028	155	160	164	rBV	20358	25245	0.36%	0.041%
6	4.881	300	305	308	rBV5	10583	14693	0.21%	0.024%
7	4.969	316	320	325	rVB4	8476	15249	0.22%	0.025%
8	5.964	483	489	492	rVB3	4772	11513	0.16%	0.019%
9	7.028	664	670	676	rBV	234925	355657	5.06%	0.577%
10	7.199	691	699	709	rBV	1050942	1601257	22.80%	2.597%
11	7.393	723	732	741	rBV	878783	1392753	19.83%	2.258%
12	7.487	744	748	755	rVB3	10598	22715	0.32%	0.037%
13	7.863	804	812	820	rBV	1018020	1570811	22.36%	2.547%
14	7.934	820	824	827	rBV4	7867	12185	0.17%	0.020%
15	8.181	864	866	870	rVB	6498	7624	0.11%	0.012%
16	8.569	926	932	943	rBV	671779	1067584	15.20%	1.731%
17	9.022	1001	1009	1017	rBV	1163682	1799197	25.61%	2.918%
18	9.369	1062	1068	1075	rVV5	19726	49918	0.71%	0.081%
19	9.452	1079	1082	1087	rVB3	21970	34700	0.49%	0.056%
20	9.746	1125	1132	1139	rBV	754765	1231760	17.54%	1.997%
21	10.281	1215	1223	1236	rBV	1265106	2042211	29.07%	3.312%
22	10.663	1279	1288	1297	rVB	1303371	2180061	31.04%	3.535%
23	10.799	1304	1311	1321	rBV	1077313	1766078	25.14%	2.864%
24	11.210	1380	1381	1387	rVB3	5334	8076	0.11%	0.013%
25	11.463	1419	1424	1427	rVB5	4633	8411	0.12%	0.014%
26	11.946	1501	1506	1510	rBV2	28664	44031	0.63%	0.071%
27	12.081	1527	1529	1534	rBV2	4873	7934	0.11%	0.013%
28	12.246	1552	1557	1563	rVB3	26627	46246	0.66%	0.075%
29	12.763	1641	1645	1646	rBV3	6060	7453	0.11%	0.012%
30	13.122	1702	1706	1710	rVB4	10900	17404	0.25%	0.028%
31	13.322	1737	1740	1746	rVB4	8299	14642	0.21%	0.024%
32	13.398	1746	1753	1757	rBV	27942	43214	0.62%	0.070%
33	13.469	1760	1765	1768	rVV5	6335	10329	0.15%	0.017%
34	13.569	1777	1782	1785	rBV4	6356	13203	0.19%	0.021%
35	13.904	1833	1839	1847	rBV	2370307	3266978	46.51%	5.298%
36	14.187	1880	1887	1893	rVV	2621212	3893866	55.44%	6.314%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018491.D
 Acq On : 01 Dec 2023 23:36
 Operator : MA/JU
 Sample : 05332-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCG73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	14.328	1909	1911	1915	rBV5	5828	7525	0.11%	0.012%
38	14.492	1931	1939	1948	rBV	1838882	2768813	39.42%	4.490%
39	14.575	1950	1953	1959	rVB3	8055	15948	0.23%	0.026%
40	14.687	1963	1972	1982	rVV	155709	267104	3.80%	0.433%
41	14.781	1986	1988	1991	rVV3	6077	7930	0.11%	0.013%
42	14.845	1995	1999	2005	rVV4	11558	23814	0.34%	0.039%
43	14.904	2007	2009	2014	rVB4	11385	17113	0.24%	0.028%
44	15.222	2058	2063	2069	rBV7	5200	11967	0.17%	0.019%
45	15.481	2100	2107	2114	rBV	3502196	4964857	70.68%	8.051%
46	15.598	2121	2127	2132	rBV	807109	1132649	16.13%	1.837%
47	15.722	2144	2148	2152	rVB4	14366	19591	0.28%	0.032%
48	16.263	2238	2240	2244	rVB3	7480	8157	0.12%	0.013%
49	16.316	2247	2249	2253	rBV	6696	8850	0.13%	0.014%
50	17.010	2363	2367	2368	rBV4	7780	8315	0.12%	0.013%
51	17.239	2399	2406	2412	rBV	2029583	2950000	42.00%	4.784%
52	17.333	2416	2422	2434	rVV2	3887775	5564240	79.22%	9.023%
53	18.128	2552	2557	2563	rBV2	182095	247930	3.53%	0.402%
54	19.151	2726	2731	2736	rBV3	50915	74074	1.05%	0.120%
55	19.216	2738	2742	2746	rBV	56352	79827	1.14%	0.129%
56	19.363	2764	2767	2773	rBV2	69351	83332	1.19%	0.135%
57	19.575	2797	2803	2810	rBV	4751372	6508041	92.65%	10.553%
58	21.039	3049	3052	3058	rBV2	155566	219347	3.12%	0.356%
59	21.322	3095	3100	3109	rBV	2494202	3172170	45.16%	5.144%
60	23.545	3471	3478	3486	rBV2	3716380	7024001	100.00%	11.390%
61	23.698	3498	3504	3514	rVB	1755569	3485883	49.63%	5.653%




Sum of corrected areas: 61667705

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018491.D
Acq On : 01 Dec 2023 23:36
Operator : MA/JU
Sample : 05332-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCG73

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

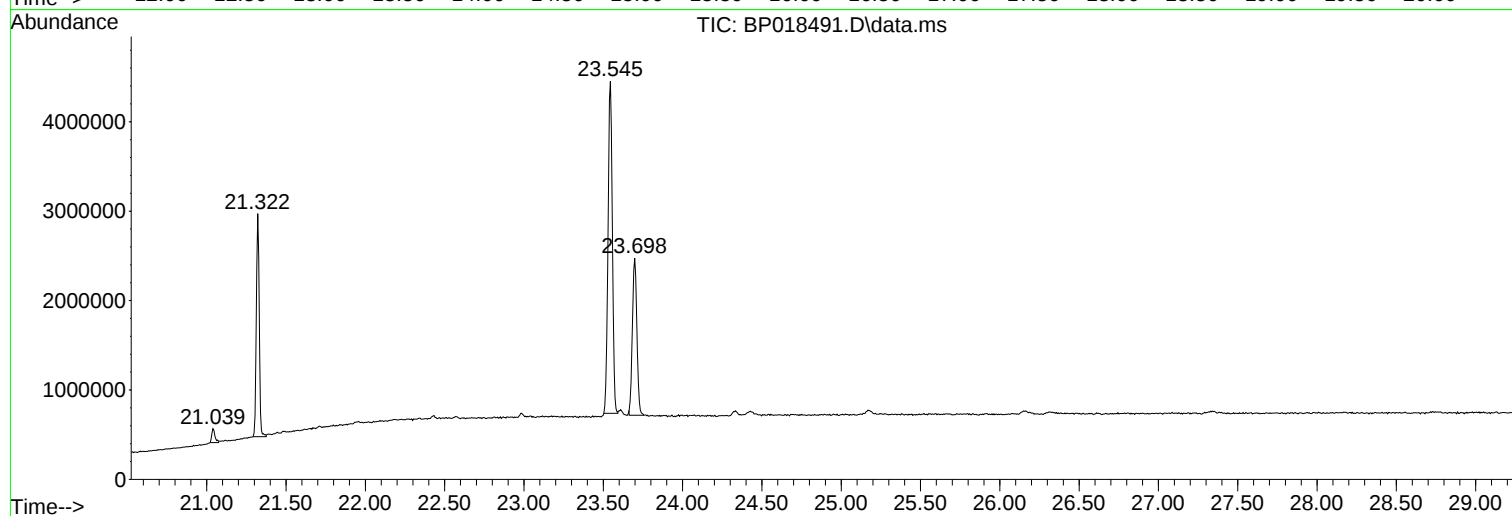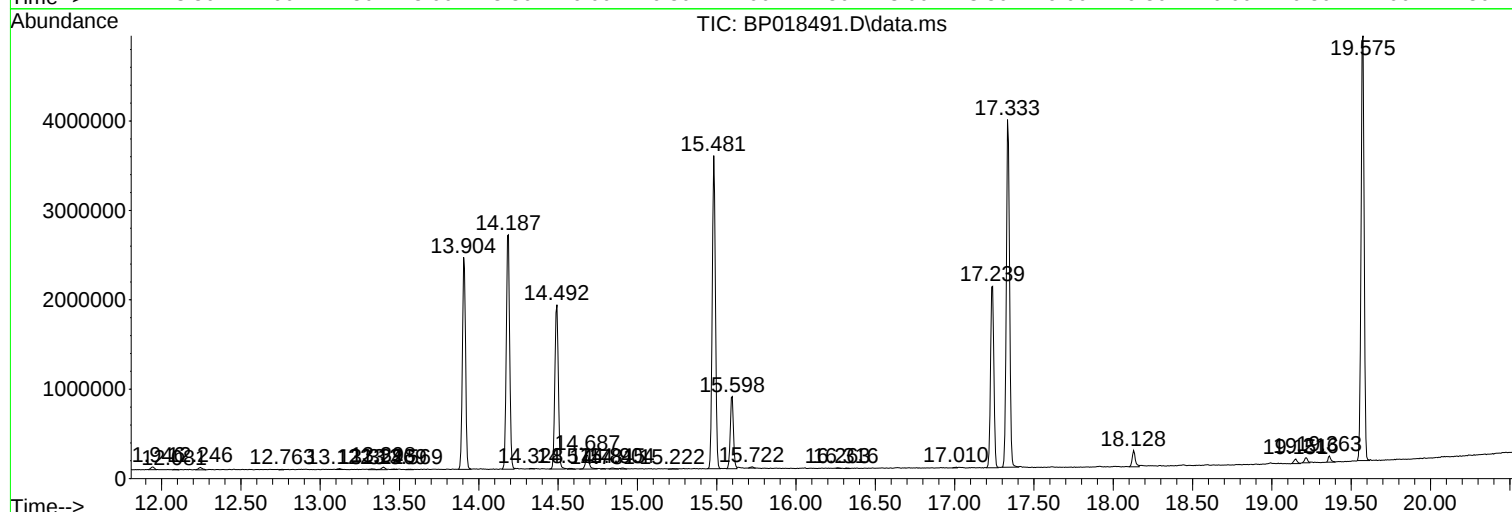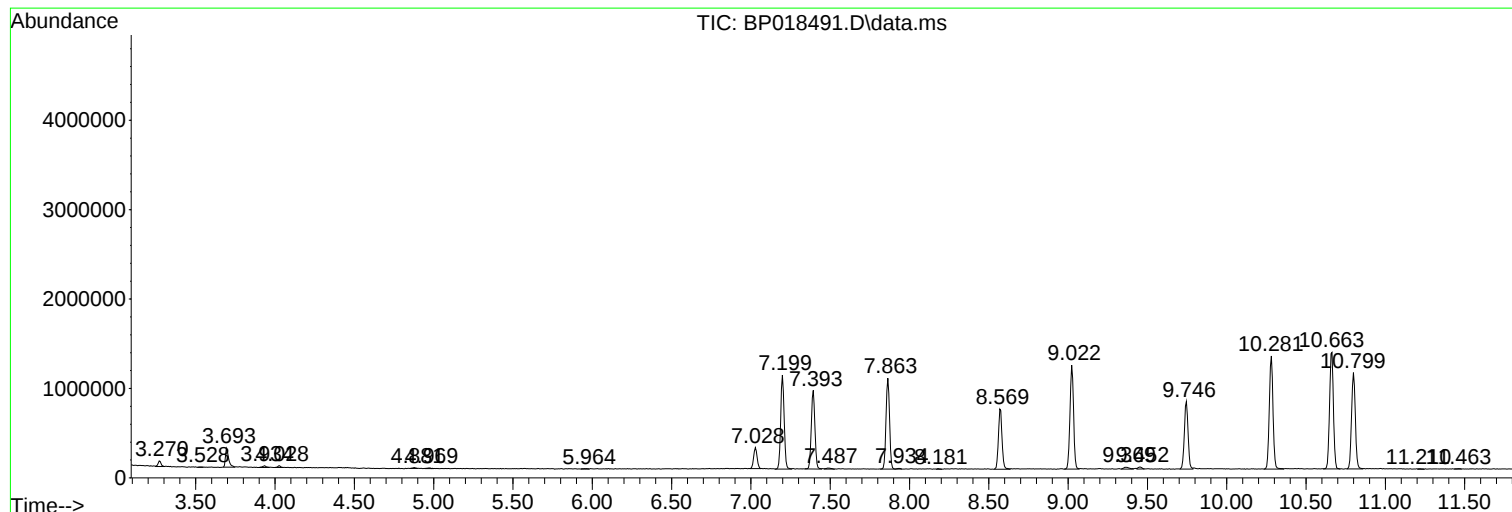

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018491.D
Acq On : 01 Dec 2023 23:36
Operator : MA/JU
Sample : 05332-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCG73

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018491.D
Acq On : 01 Dec 2023 23:36
Operator : MA/JU
Sample : 05332-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCG73

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------