

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018494.D
 Acq On : 02 Dec 2023 01:18
 Operator : MA/JU
 Sample : 05332-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCG99

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018494.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	28	31	37	rVB	67446	81528	1.11%	0.110%
2	3.693	99	103	116	rBV	371904	527130	7.18%	0.711%
3	3.858	128	131	135	rBV	5296	7546	0.10%	0.010%
4	3.928	139	143	150	rVB3	17966	31694	0.43%	0.043%
5	4.028	155	160	166	rBV2	18429	29538	0.40%	0.040%
6	4.499	239	240	248	rVB7	4655	8479	0.12%	0.011%
7	4.658	264	267	271	rBV5	9670	14674	0.20%	0.020%
8	6.428	564	568	572	rBV2	5160	10602	0.14%	0.014%
9	6.775	624	627	630	rBV3	5862	8428	0.11%	0.011%
10	6.846	636	639	640	rBV2	7662	8265	0.11%	0.011%
11	7.028	663	670	676	rBV	281468	419327	5.71%	0.565%
12	7.199	691	699	709	rBV	1254612	1909497	26.02%	2.574%
13	7.393	725	732	739	rBV	1078019	1651772	22.51%	2.226%
14	7.493	744	749	752	rBV4	9798	16647	0.23%	0.022%
15	7.681	779	781	786	rVB	6575	9051	0.12%	0.012%
16	7.863	805	812	821	rBV	1091099	1696739	23.12%	2.287%
17	8.575	926	933	941	rBV	833449	1317421	17.95%	1.776%
18	9.022	1002	1009	1017	rVB	1417411	2219919	30.25%	2.992%
19	9.451	1077	1082	1088	rVB2	40914	66874	0.91%	0.090%
20	9.746	1124	1132	1145	rBV	997462	1620060	22.08%	2.184%
21	10.081	1185	1189	1196	rVB4	5652	11704	0.16%	0.016%
22	10.281	1215	1223	1233	rBV	1581127	2550960	34.76%	3.438%
23	10.663	1280	1288	1295	rBV	1482747	2494222	33.99%	3.362%
24	10.798	1302	1311	1321	rBV	1339481	2173302	29.62%	2.929%
25	11.310	1392	1398	1402	rBV3	16699	29871	0.41%	0.040%
26	11.940	1501	1505	1511	rBV4	18130	30696	0.42%	0.041%
27	12.163	1538	1543	1549	rBV4	17822	35992	0.49%	0.049%
28	12.245	1549	1557	1564	rVB2	35094	65609	0.89%	0.088%
29	12.857	1656	1661	1666	rBV2	35775	54825	0.75%	0.074%
30	12.910	1666	1670	1674	rVB4	11282	16966	0.23%	0.023%
31	13.110	1700	1704	1712	rVB5	18818	38316	0.52%	0.052%
32	13.334	1739	1742	1743	rBV2	6409	7640	0.10%	0.010%
33	13.398	1747	1753	1760	rBV	42929	73715	1.00%	0.099%
34	13.463	1761	1764	1768	rVB5	7369	7482	0.10%	0.010%
35	13.798	1817	1821	1827	rVB4	10420	18707	0.25%	0.025%
36	13.904	1833	1839	1847	rBV	3285155	4618956	62.95%	6.226%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018494.D
 Acq On : 02 Dec 2023 01:18
 Operator : MA/JU
 Sample : 05332-06
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCG99

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	14.187	1876	1887	1895	rBV	3660202	5452924	74.31%	7.350%
38	14.492	1932	1939	1949	rVB	2378746	3458192	47.13%	4.661%
39	14.686	1966	1972	1982	rBV	194992	306933	4.18%	0.414%
40	14.851	1995	2000	2003	rBV4	6778	12339	0.17%	0.017%
41	14.904	2005	2009	2013	rBV5	13525	19575	0.27%	0.026%
42	15.239	2061	2066	2070	rVB2	7471	12680	0.17%	0.017%
43	15.298	2070	2076	2083	rBV2	89764	150531	2.05%	0.203%
44	15.481	2097	2107	2114	rBV	4923364	6959154	94.84%	9.380%
45	15.598	2120	2127	2139	rBV	1101926	1514975	20.65%	2.042%
46	15.722	2145	2148	2155	rVB3	24783	43072	0.59%	0.058%
47	15.851	2166	2170	2175	rVB6	9635	13158	0.18%	0.018%
48	16.110	2210	2214	2218	rVB2	13057	16996	0.23%	0.023%
49	16.910	2344	2350	2351	rBV4	9215	14996	0.20%	0.020%
50	17.028	2364	2370	2377	rBV6	9249	26826	0.37%	0.036%
51	17.116	2380	2385	2387	rVB	6445	10165	0.14%	0.014%
52	17.239	2399	2406	2415	rBV	2660558	3792034	51.68%	5.111%
53	17.339	2416	2423	2434	rVV	4883303	7144832	97.37%	9.630%
54	17.416	2434	2436	2446	rVB10	12150	23649	0.32%	0.032%
55	17.910	2516	2520	2525	rBV7	18179	26571	0.36%	0.036%
56	18.127	2552	2557	2563	rBV2	192867	263538	3.59%	0.355%
57	19.151	2727	2731	2735	rVB2	58467	80760	1.10%	0.109%
58	19.216	2738	2742	2745	rBV	68833	93787	1.28%	0.126%
59	19.363	2763	2767	2772	rBV3	79760	112453	1.53%	0.152%
60	19.569	2797	2802	2809	rBV	5504827	7337751	100.00%	9.890%
61	21.039	3049	3052	3057	rBV2	141115	194856	2.66%	0.263%
62	21.321	3095	3100	3107	rBV	2682992	3246928	44.25%	4.377%
63	23.545	3471	3478	3487	rBV2	3481623	6630291	90.36%	8.937%
64	23.698	3497	3504	3512	rBV	1663651	3345843	45.60%	4.510%




Sum of corrected areas: 74189963

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018494.D
Acq On : 02 Dec 2023 01:18
Operator : MA/JU
Sample : 05332-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCG99

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

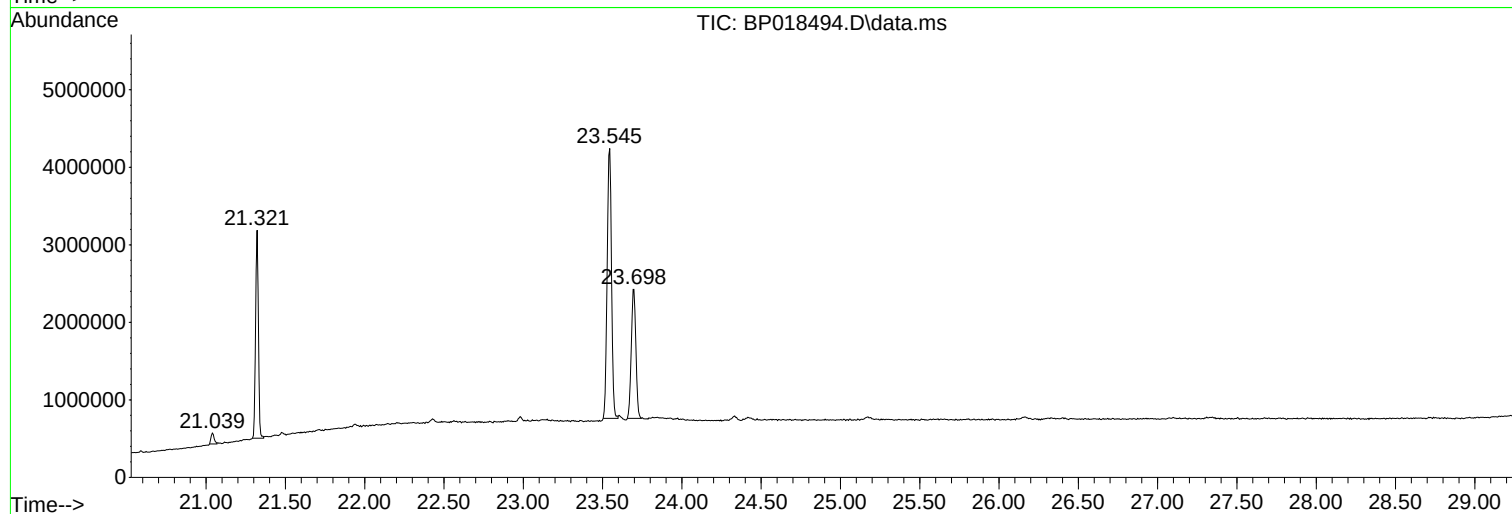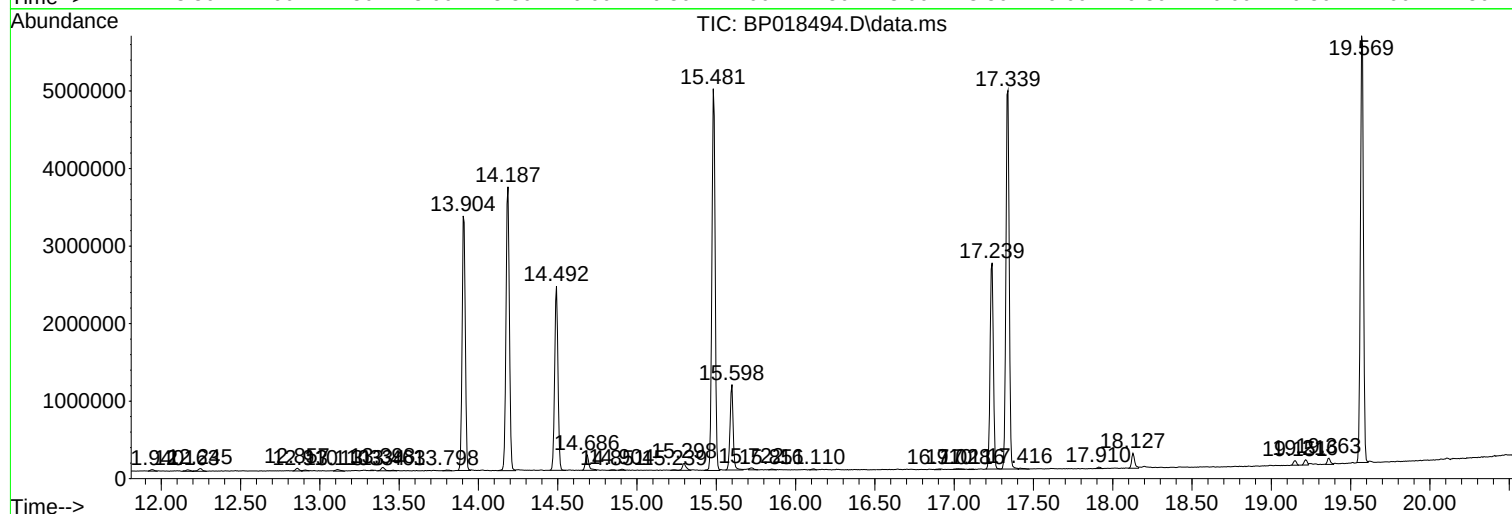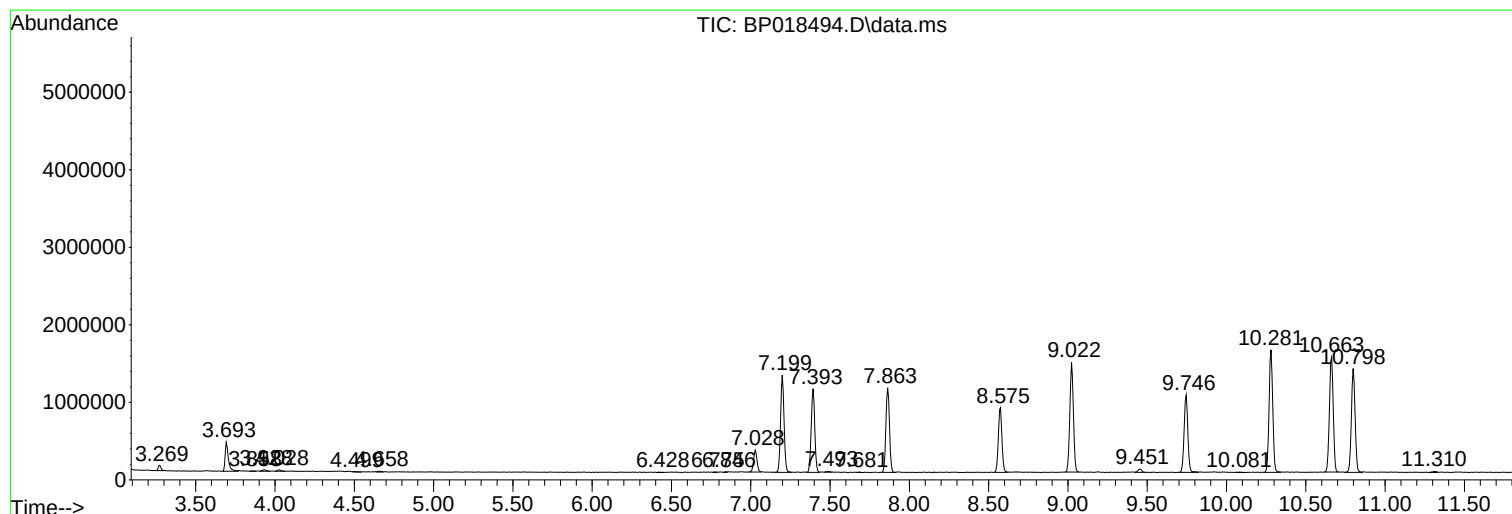

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018494.D
Acq On : 02 Dec 2023 01:18
Operator : MA/JU
Sample : 05332-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCG99

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018494.D
Acq On : 02 Dec 2023 01:18
Operator : MA/JU
Sample : 05332-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCG99

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------