

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018507.D
 Acq On : 02 Dec 2023 09:49
 Operator : MA/JU
 Sample : 05328-02
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A49P9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018507.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	28	31	36	rBV	99851	128617	1.02%	0.116%
2	3.693	100	103	114	rBV	336562	481944	3.83%	0.433%
3	3.934	140	144	149	rVB	23238	32051	0.25%	0.029%
4	4.028	156	160	165	rVB	31385	43501	0.35%	0.039%
5	7.028	662	670	681	rVB	342565	548135	4.35%	0.492%
6	7.199	692	699	712	rVB	1525113	2353662	18.69%	2.114%
7	7.393	724	732	742	rBV	1317681	2064580	16.40%	1.855%
8	7.487	744	748	754	rVB5	12003	22725	0.18%	0.020%
9	7.863	804	812	820	rBV	1881324	2952983	23.45%	2.653%
10	7.934	820	824	828	rVB3	11605	18652	0.15%	0.017%
11	8.569	925	932	941	rBV	1004795	1570430	12.47%	1.411%
12	9.022	1002	1009	1018	rBV	1681675	2703511	21.47%	2.429%
13	9.451	1076	1082	1087	rBV4	16968	30753	0.24%	0.028%
14	9.746	1122	1132	1139	rBV	1184667	1947042	15.46%	1.749%
15	10.281	1214	1223	1234	rBV	1959560	3239804	25.73%	2.910%
16	10.657	1279	1287	1295	rBV	2545603	4268254	33.90%	3.834%
17	10.798	1301	1311	1323	rBV	1438398	2398388	19.05%	2.154%
18	11.445	1416	1421	1426	rBV2	8338	16597	0.13%	0.015%
19	12.245	1550	1557	1563	rBV4	42139	78579	0.62%	0.071%
20	13.322	1736	1740	1744	rBV2	16635	21331	0.17%	0.019%
21	13.398	1748	1753	1760	rBV2	36023	61768	0.49%	0.055%
22	13.904	1833	1839	1847	rBV	3873459	5332820	42.35%	4.790%
23	14.181	1878	1886	1896	rBV	4309136	6324390	50.23%	5.681%
24	14.492	1931	1939	1948	rVV	3687723	5601140	44.48%	5.031%
25	14.569	1950	1952	1957	rVB3	10160	15377	0.12%	0.014%
26	14.681	1965	1971	1977	rBV	288798	438412	3.48%	0.394%
27	14.845	1991	1999	2003	rBV5	28123	55781	0.44%	0.050%
28	14.910	2005	2010	2015	rVB6	21280	36932	0.29%	0.033%
29	15.481	2100	2107	2116	rBV	5677231	8160801	64.81%	7.331%
30	15.598	2121	2127	2138	rBV	1460562	2034742	16.16%	1.828%
31	15.722	2144	2148	2158	rVB2	32388	56151	0.45%	0.050%
32	16.269	2238	2241	2244	rVB4	11090	15053	0.12%	0.014%
33	16.639	2300	2304	2308	rBV2	13923	20960	0.17%	0.019%
34	17.022	2361	2369	2377	rBV4	19541	72520	0.58%	0.065%
35	17.110	2381	2384	2387	rVV3	9956	15210	0.12%	0.014%
36	17.233	2399	2405	2412	rBV	4447917	6411444	50.92%	5.759%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018507.D
 Acq On : 02 Dec 2023 09:49
 Operator : MA/JU
 Sample : 05328-02
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A49P9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	17.333	2416	2422	2432	rBV	6052533	8599477	68.30%	7.725%
38	17.616	2466	2470	2473	rBV4	10177	15221	0.12%	0.014%
39	17.998	2533	2535	2542	rBV7	10504	18327	0.15%	0.016%
40	18.127	2553	2557	2562	rBV	337634	431665	3.43%	0.388%
41	18.439	2606	2610	2619	rVB3	67165	97851	0.78%	0.088%
42	18.586	2632	2635	2643	rVB4	41619	61768	0.49%	0.055%
43	19.145	2726	2730	2736	rBV	91495	122435	0.97%	0.110%
44	19.210	2737	2741	2745	rBV2	147147	224383	1.78%	0.202%
45	19.363	2763	2767	2773	rBV	155456	191503	1.52%	0.172%
46	19.569	2796	2802	2809	rBV	8372675	11250705	89.35%	10.106%
47	21.039	3049	3052	3062	rBV	243293	321707	2.55%	0.289%
48	21.321	3094	3100	3106	rBV	5958747	7592885	60.30%	6.821%
49	22.980	3379	3382	3388	rVB	265346	373611	2.97%	0.336%
50	23.545	3470	3478	3484	rBV2	6289827	12591490	100.00%	11.311%
51	23.604	3485	3488	3494	rVB	383531	618357	4.91%	0.555%
52	23.698	3496	3504	3515	rVB	4209639	8557112	67.96%	7.687%
53	24.327	3607	3611	3619	rVB	352262	680081	5.40%	0.611%




Sum of corrected areas: 111323618

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018507.D
Acq On : 02 Dec 2023 09:49
Operator : MA/JU
Sample : 05328-02
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A49P9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

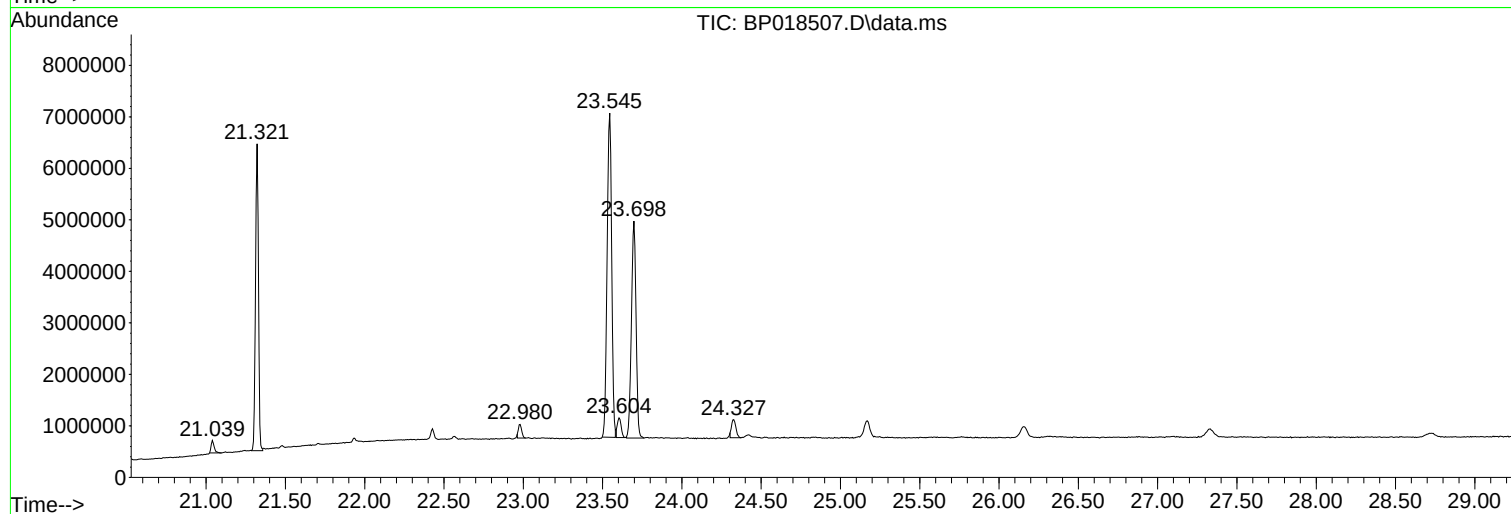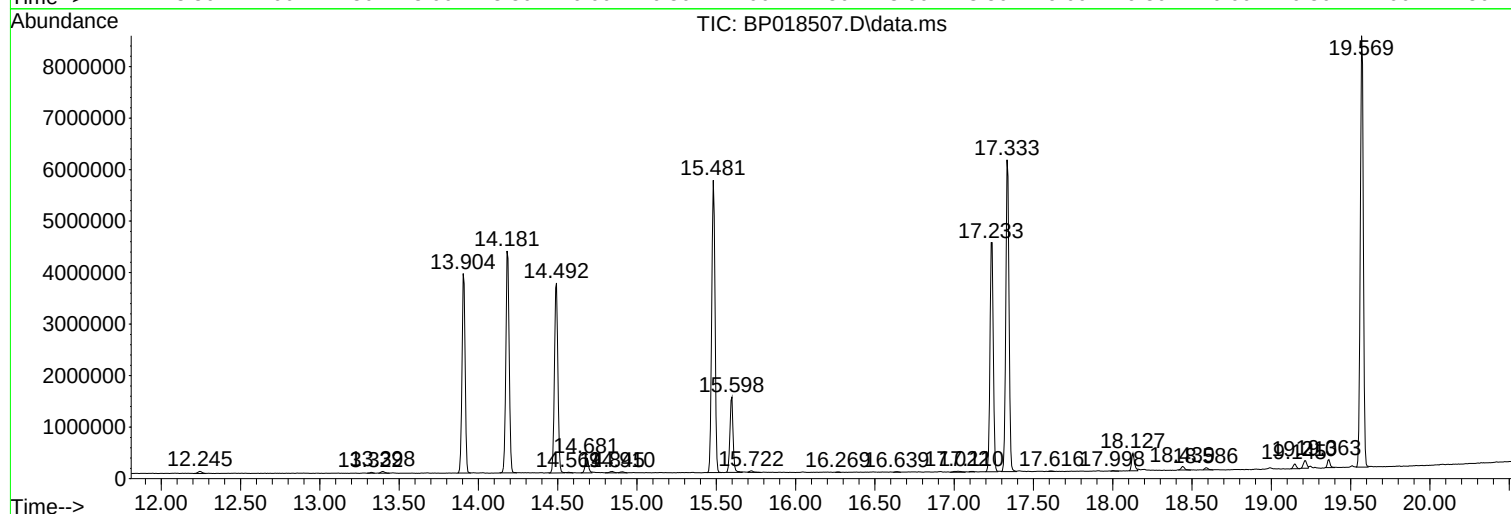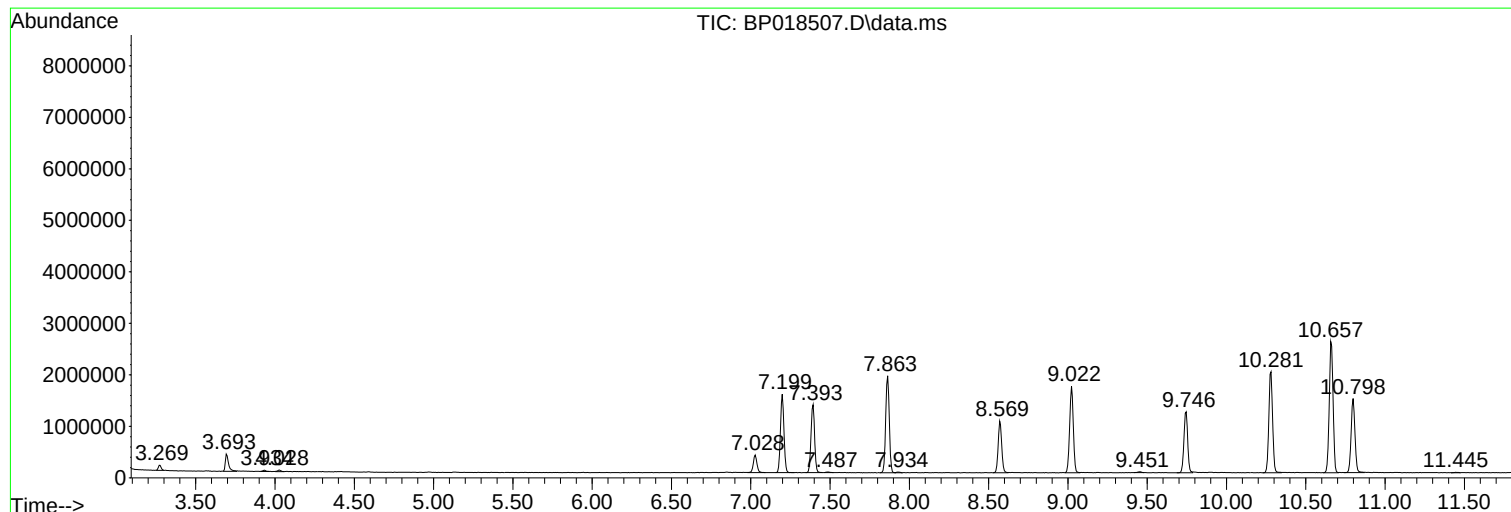

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018507.D
Acq On : 02 Dec 2023 09:49
Operator : MA/JU
Sample : 05328-02
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A49P9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018507.D
Acq On : 02 Dec 2023 09:49
Operator : MA/JU
Sample : 05328-02
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A49P9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------