

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018510.D
 Acq On : 02 Dec 2023 11:31
 Operator : MA/JU
 Sample : 05328-07
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A49W7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018510.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	37	rBV	98029	125349	1.20%	0.126%
2	3.693	100	103	112	rBV	296803	426567	4.08%	0.430%
3	3.805	120	122	127	rVB4	12494	13033	0.12%	0.013%
4	3.934	138	144	151	rVB2	20031	33432	0.32%	0.034%
5	4.028	156	160	165	rVB	21561	28460	0.27%	0.029%
6	4.964	316	319	325	rVB5	7278	12825	0.12%	0.013%
7	5.140	346	349	355	rVB3	7154	12367	0.12%	0.012%
8	6.846	633	639	644	rBV3	8061	17605	0.17%	0.018%
9	7.028	660	670	679	rVB	359390	569251	5.45%	0.573%
10	7.199	689	699	707	rBV	1433189	2226859	21.33%	2.243%
11	7.393	725	732	741	rVB	1248142	1948917	18.66%	1.963%
12	7.487	744	748	755	rVB6	10358	14975	0.14%	0.015%
13	7.864	803	812	818	rBV	1502482	2381020	22.80%	2.398%
14	7.928	818	823	828	rVB4	11437	18358	0.18%	0.018%
15	8.569	926	932	942	rBV	1008495	1584827	15.18%	1.596%
16	9.022	1001	1009	1020	rBV	1680728	2662437	25.50%	2.681%
17	9.193	1034	1038	1042	rBV2	14506	19725	0.19%	0.020%
18	9.452	1074	1082	1086	rBV2	64512	104053	1.00%	0.105%
19	9.740	1125	1131	1139	rBV	1167617	1917864	18.37%	1.931%
20	10.281	1212	1223	1231	rBV	1928502	3234229	30.97%	3.257%
21	10.657	1278	1287	1296	rVB	2221926	3744180	35.86%	3.771%
22	10.799	1302	1311	1325	rBV	1431085	2435335	23.32%	2.453%
23	11.446	1417	1421	1422	rBV	10204	12825	0.12%	0.013%
24	11.940	1497	1505	1510	rBV	40475	60698	0.58%	0.061%
25	12.246	1549	1557	1563	rBV2	41072	72813	0.70%	0.073%
26	13.322	1736	1740	1746	rBV2	17679	24309	0.23%	0.024%
27	13.393	1748	1752	1757	rBV2	35729	54876	0.53%	0.055%
28	13.675	1795	1800	1804	rVB4	7902	15018	0.14%	0.015%
29	13.904	1833	1839	1850	rBV	4373515	5904781	56.55%	5.946%
30	14.010	1854	1857	1861	rBV3	6625	10476	0.10%	0.011%
31	14.181	1876	1886	1896	rBV	4322507	6584681	63.06%	6.631%
32	14.487	1930	1938	1948	rBV	3604734	5449790	52.19%	5.488%
33	14.563	1949	1951	1958	rVB3	11357	17734	0.17%	0.018%
34	14.681	1966	1971	1984	rBV	322247	475906	4.56%	0.479%
35	14.840	1993	1998	2003	rBV2	34605	53729	0.51%	0.054%
36	14.904	2005	2009	2014	rVB6	24701	34217	0.33%	0.034%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018510.D
 Acq On : 02 Dec 2023 11:31
 Operator : MA/JU
 Sample : 05328-07
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A49W7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	15.293	2072	2075	2080	rBV6	8453	16264	0.16%	0.016%
38	15.481	2100	2107	2115	rBV	6220021	8802300	84.29%	8.864%
39	15.593	2120	2126	2142	rVV	1577775	2256315	21.61%	2.272%
40	15.722	2144	2148	2152	rVB3	31006	44686	0.43%	0.045%
41	16.640	2300	2304	2309	rBV2	17971	25946	0.25%	0.026%
42	16.775	2325	2327	2333	rVB7	11704	18361	0.18%	0.018%
43	16.904	2346	2349	2351	rBV3	9920	13210	0.13%	0.013%
44	16.998	2363	2365	2369	rBV2	13113	18874	0.18%	0.019%
45	17.110	2381	2384	2390	rBV7	15318	22661	0.22%	0.023%
46	17.234	2399	2405	2411	rBV	4300832	6153865	58.93%	6.197%
47	17.334	2416	2422	2432	rVV2	6312531	9025811	86.43%	9.090%
48	17.998	2532	2535	2539	rBV5	13284	18159	0.17%	0.018%
49	18.128	2552	2557	2566	rBV	375061	548207	5.25%	0.552%
50	18.439	2606	2610	2617	rVB3	63391	99359	0.95%	0.100%
51	18.586	2631	2635	2640	rBV4	42031	64735	0.62%	0.065%
52	18.986	2700	2703	2711	rBV4	48260	82934	0.79%	0.084%
53	19.145	2726	2730	2734	rVB	90923	115916	1.11%	0.117%
54	19.210	2736	2741	2745	rBV2	148965	225068	2.16%	0.227%
55	19.357	2763	2766	2776	rBV2	149681	208435	2.00%	0.210%
56	19.510	2789	2792	2795	rBV4	28706	30460	0.29%	0.031%
57	19.569	2796	2802	2809	rVV	7900940	10442332	100.00%	10.516%
58	21.039	3048	3052	3060	rBV3	220240	333194	3.19%	0.336%
59	21.316	3094	3099	3108	rBV	4068211	5043963	48.30%	5.080%
60	23.539	3470	3477	3484	rBV2	4485417	8373138	80.18%	8.432%
61	23.692	3497	3503	3513	rVB	2637642	5011547	47.99%	5.047%




Sum of corrected areas: 99299261

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018510.D
Acq On : 02 Dec 2023 11:31
Operator : MA/JU
Sample : 05328-07
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A49W7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

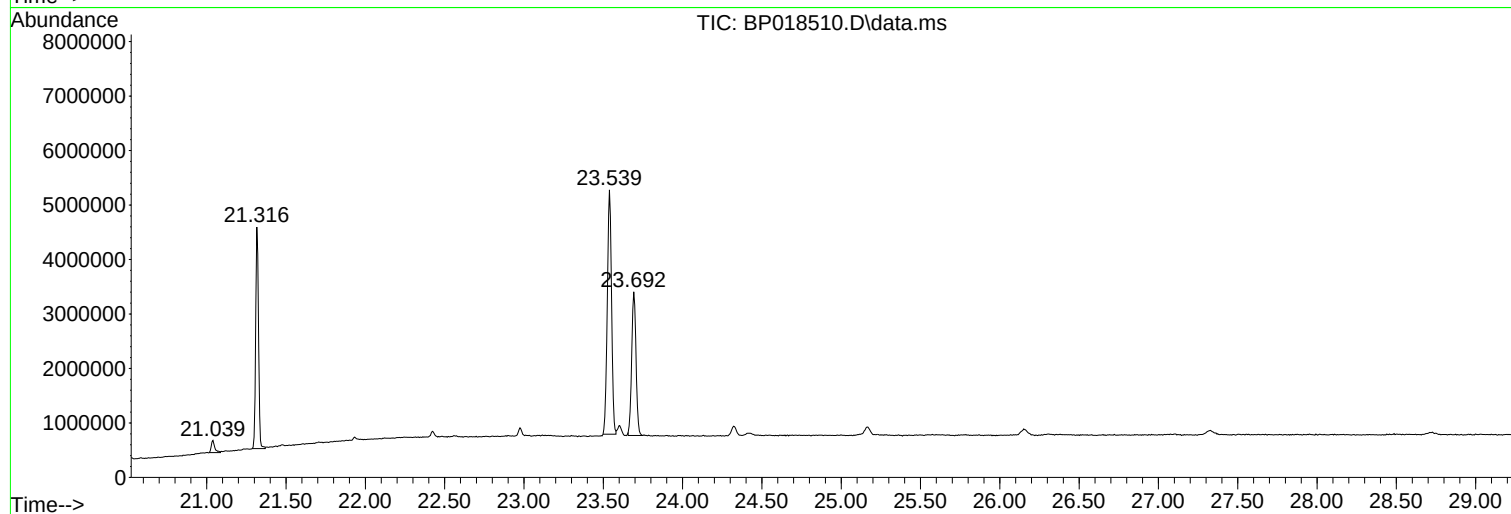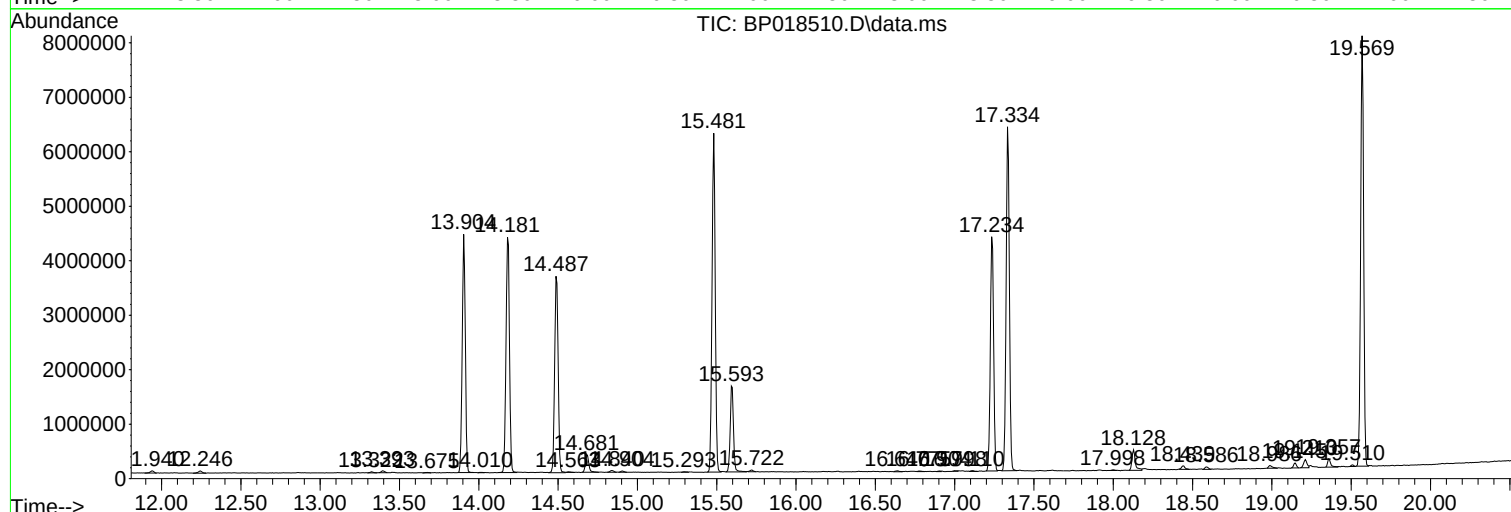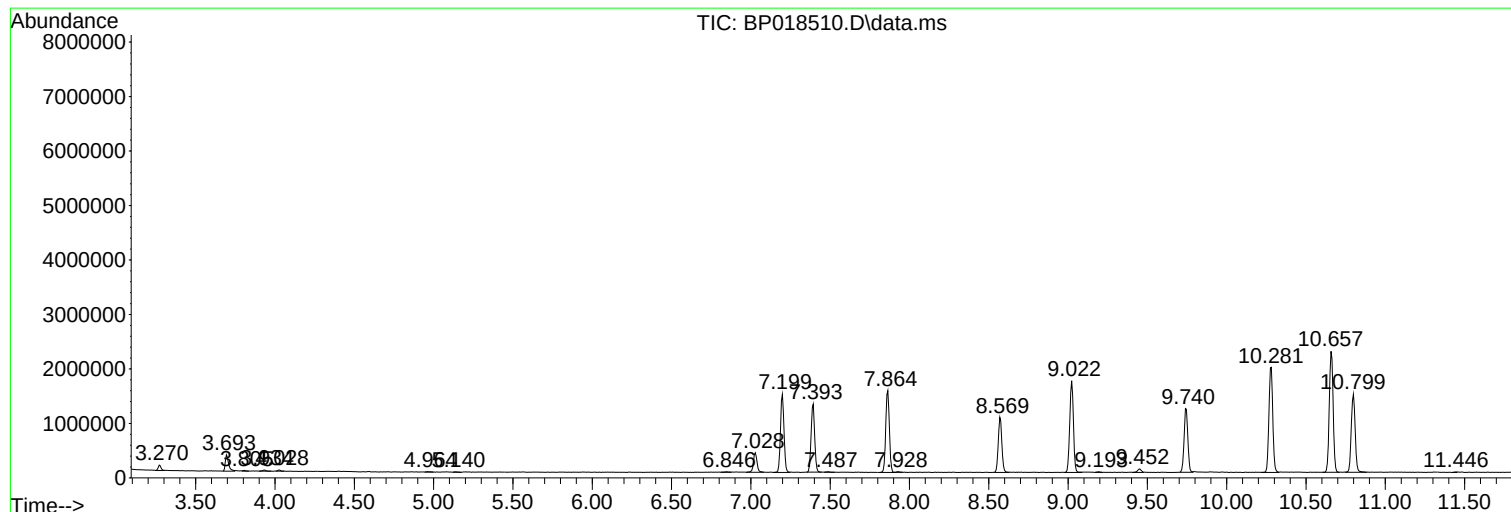

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018510.D
Acq On : 02 Dec 2023 11:31
Operator : MA/JU
Sample : 05328-07
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A49W7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018510.D
Acq On : 02 Dec 2023 11:31
Operator : MA/JU
Sample : 05328-07
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A49W7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------