

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018513.D
 Acq On : 02 Dec 2023 13:12
 Operator : MA/JU
 Sample : 05416-21
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018513.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	29	32	38	rVB	34716	48991	0.63%	0.071%
2	3.699	100	104	113	rBV	132693	201355	2.59%	0.293%
3	3.934	140	144	150	rVB2	44625	64491	0.83%	0.094%
4	4.022	155	159	165	rVB2	36165	53344	0.69%	0.078%
5	4.258	195	199	203	rBV2	25951	32189	0.41%	0.047%
6	4.405	221	224	228	rVB5	11466	11971	0.15%	0.017%
7	4.669	266	269	274	rVB3	16661	21198	0.27%	0.031%
8	4.964	313	319	326	rVV2	52212	104784	1.35%	0.153%
9	5.052	330	334	338	rBV5	6401	10164	0.13%	0.015%
10	5.564	417	421	425	rBV5	6731	10791	0.14%	0.016%
11	5.722	445	448	453	rBV2	4934	9483	0.12%	0.014%
12	5.846	466	469	471	rBV4	6899	8133	0.10%	0.012%
13	6.246	534	537	543	rBV3	4882	9498	0.12%	0.014%
14	6.846	637	639	644	rVB3	9447	12567	0.16%	0.018%
15	7.028	662	670	684	rVB	682364	1144512	14.70%	1.666%
16	7.199	692	699	707	rBV	684424	1053278	13.53%	1.533%
17	7.393	724	732	739	rBV	747826	1198537	15.39%	1.744%
18	7.487	741	748	756	rVB6	22752	50085	0.64%	0.073%
19	7.675	778	780	786	rVB4	8309	11819	0.15%	0.017%
20	7.863	802	812	820	rBV	1761468	2813239	36.13%	4.095%
21	7.934	820	824	827	rVB2	8920	14043	0.18%	0.020%
22	8.516	919	923	926	rBV3	4600	8030	0.10%	0.012%
23	8.569	926	932	941	rVV	821672	1267659	16.28%	1.845%
24	8.687	946	952	960	rVV	240207	380041	4.88%	0.553%
25	8.816	969	974	975	rBV4	6479	8804	0.11%	0.013%
26	8.828	975	976	983	rVB2	10675	12215	0.16%	0.018%
27	9.022	1002	1009	1018	rBV	740021	1181627	15.17%	1.720%
28	9.193	1032	1038	1041	rBV6	8957	14664	0.19%	0.021%
29	9.269	1045	1051	1053	rBV4	8384	13094	0.17%	0.019%
30	9.452	1077	1082	1088	rVB3	10752	22912	0.29%	0.033%
31	9.740	1124	1131	1140	rBV	509010	840909	10.80%	1.224%
32	9.881	1150	1155	1164	rBV2	39233	78231	1.00%	0.114%
33	10.104	1181	1193	1199	rBV3	29495	55887	0.72%	0.081%
34	10.275	1215	1222	1230	rVV	868355	1443252	18.53%	2.101%
35	10.657	1279	1287	1294	rBV	2414711	4040952	51.89%	5.881%
36	10.704	1294	1295	1301	rVB3	10163	12679	0.16%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018513.D
 Acq On : 02 Dec 2023 13:12
 Operator : MA/JU
 Sample : 05416-21
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	10.799	1301	1311	1321	rBV	773779	1322544	16.98%	1.925%
38	11.199	1373	1379	1384	rBV4	19063	38063	0.49%	0.055%
39	11.310	1394	1398	1402	rBV5	5457	11377	0.15%	0.017%
40	11.446	1413	1421	1429	rBV	29039	49078	0.63%	0.071%
41	11.498	1429	1430	1437	rVB	7258	9261	0.12%	0.013%
42	12.022	1514	1519	1523	rBV4	8538	14341	0.18%	0.021%
43	12.081	1526	1529	1530	rBV2	9234	9038	0.12%	0.013%
44	12.240	1553	1556	1563	rVB4	12860	22485	0.29%	0.033%
45	12.316	1565	1569	1573	rVB2	14998	20796	0.27%	0.030%
46	12.534	1602	1606	1613	rVB3	13902	23166	0.30%	0.034%
47	13.034	1688	1691	1696	rVV5	5756	8699	0.11%	0.013%
48	13.328	1737	1741	1746	rVV3	13641	19266	0.25%	0.028%
49	13.398	1746	1753	1759	rVV2	52153	93424	1.20%	0.136%
50	13.457	1761	1763	1768	rVB4	7196	9360	0.12%	0.014%
51	13.816	1818	1824	1829	rBV5	18771	36875	0.47%	0.054%
52	13.904	1833	1839	1845	rVV	1640902	2187207	28.09%	3.183%
53	13.975	1848	1851	1855	rVB3	9693	14272	0.18%	0.021%
54	14.181	1878	1886	1896	rBV2	1796694	2657471	34.13%	3.868%
55	14.392	1916	1922	1926	rVB4	15869	25858	0.33%	0.038%
56	14.487	1930	1938	1945	rBV	3564262	5290442	67.94%	7.700%
57	14.557	1945	1950	1954	rVB2	10756	18792	0.24%	0.027%
58	14.610	1954	1959	1965	rBV3	8759	12062	0.15%	0.018%
59	14.681	1966	1971	1980	rBV	285845	430554	5.53%	0.627%
60	14.839	1994	1998	2002	rBV3	15601	22879	0.29%	0.033%
61	14.910	2003	2010	2015	rVB7	29804	53455	0.69%	0.078%
62	15.145	2048	2050	2056	rVB2	6523	7945	0.10%	0.012%
63	15.292	2072	2075	2081	rVV3	9540	14407	0.19%	0.021%
64	15.345	2081	2084	2089	rVB3	14935	20027	0.26%	0.029%
65	15.481	2100	2107	2114	rBV	2392827	3384171	43.46%	4.926%
66	15.592	2121	2126	2132	rBV	224681	313513	4.03%	0.456%
67	15.716	2144	2147	2151	rBV5	11821	16475	0.21%	0.024%
68	16.204	2227	2230	2234	rBV4	16312	25189	0.32%	0.037%
69	16.551	2287	2289	2292	rBV2	7050	8281	0.11%	0.012%
70	16.634	2301	2303	2307	rVB4	9053	9584	0.12%	0.014%
71	16.692	2310	2313	2316	rBV3	8901	11099	0.14%	0.016%
72	16.781	2324	2328	2332	rBV4	14479	22444	0.29%	0.033%
73	17.004	2363	2366	2373	rVB5	13563	23988	0.31%	0.035%
74	17.116	2382	2385	2390	rBV5	7466	11216	0.14%	0.016%
75	17.233	2398	2405	2411	rBV	4302676	6044120	77.61%	8.797%
76	17.275	2411	2412	2416	rVV	40273	42585	0.55%	0.062%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018513.D
 Acq On : 02 Dec 2023 13:12
 Operator : MA/JU
 Sample : 05416-21
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AH4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

77	17.333	2416	2422	2433	rVV	2522987	3462906	44.47%	5.040%
78	17.428	2434	2438	2446	rVB4	48313	73950	0.95%	0.108%
79	17.745	2488	2492	2495	rVB4	17287	21705	0.28%	0.032%
80	17.910	2517	2520	2525	rBV4	14033	18729	0.24%	0.027%
81	18.004	2532	2536	2544	rVB5	34657	57757	0.74%	0.084%
82	18.128	2551	2557	2565	rBV2	161462	242222	3.11%	0.353%
83	18.286	2581	2584	2588	rBV3	15855	22767	0.29%	0.033%
84	18.410	2603	2605	2608	rBV4	15436	18801	0.24%	0.027%
85	18.539	2625	2627	2631	rBV2	11910	15173	0.19%	0.022%
86	18.680	2647	2651	2654	rBV2	39782	50914	0.65%	0.074%
87	18.898	2685	2688	2693	rVB2	31002	35610	0.46%	0.052%
88	19.145	2727	2730	2735	rVB2	44581	52241	0.67%	0.076%
89	19.245	2743	2747	2755	rVB	162622	220954	2.84%	0.322%
90	19.357	2763	2766	2770	rBV2	78614	99876	1.28%	0.145%
91	19.569	2796	2802	2814	rBV	3653633	4687504	60.19%	6.823%
92	21.039	3048	3052	3060	rVB	237238	342661	4.40%	0.499%
93	21.322	3094	3100	3105	rBV	5337328	7059178	90.65%	10.274%
94	21.933	3201	3204	3214	rBV4	148010	224430	2.88%	0.327%
95	22.974	3378	3381	3386	rVB	293871	421030	5.41%	0.613%
96	23.539	3470	3477	3483	rBV2	2388458	4633316	59.50%	6.744%
97	23.692	3496	3503	3518	rVB	3860310	7787404	100.00%	11.334%
98	24.327	3607	3611	3619	rVB2	279980	536157	6.88%	0.780%




Sum of corrected areas: 68706522

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018513.D
Acq On : 02 Dec 2023 13:12
Operator : MA/JU
Sample : 05416-21
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AH4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

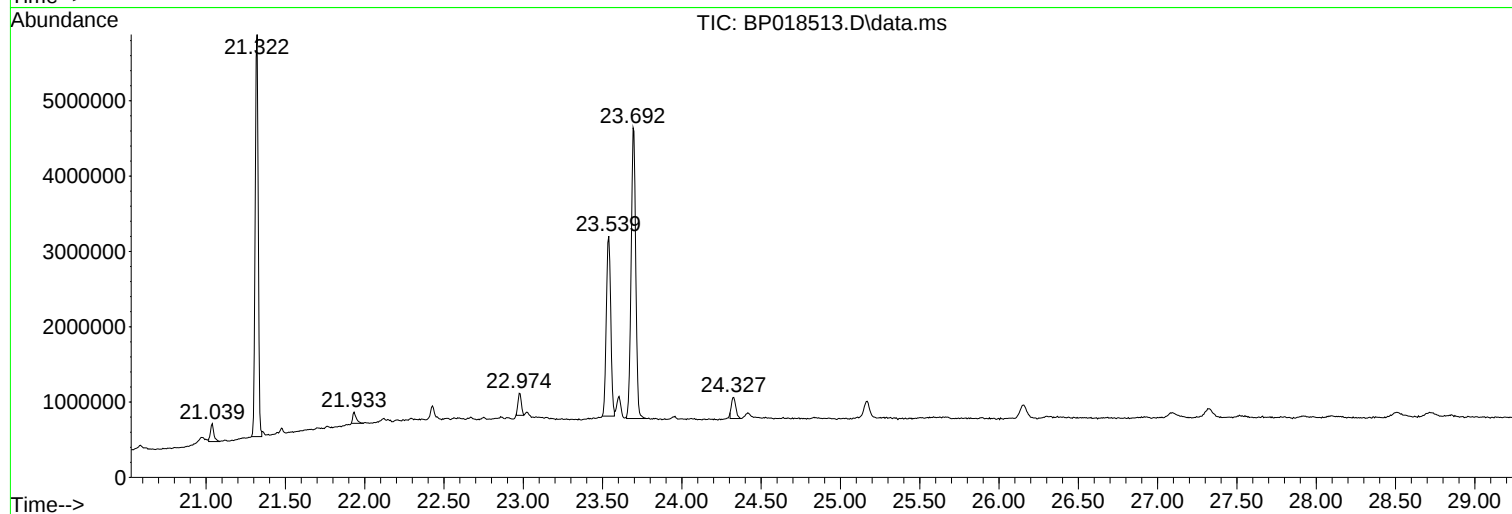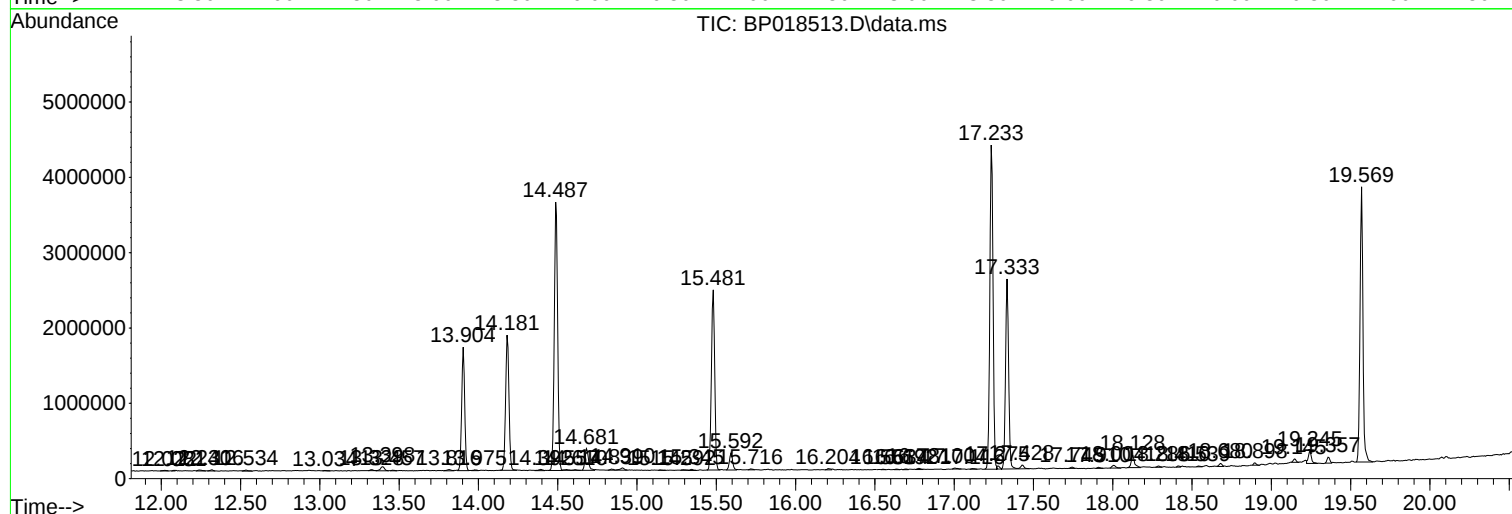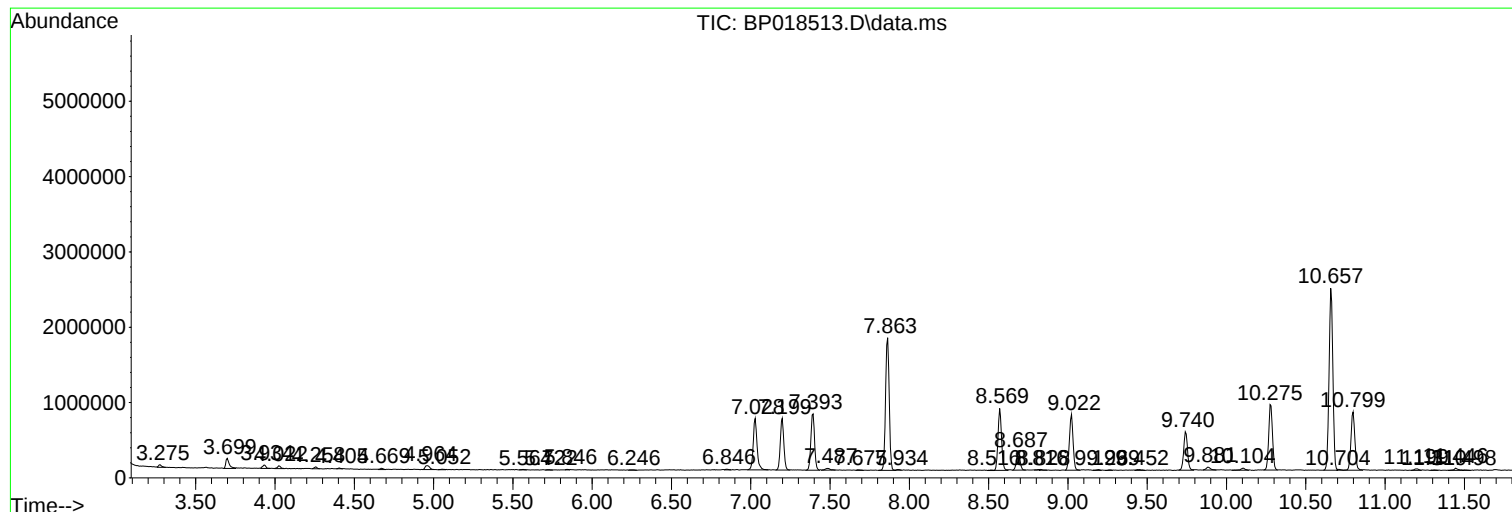

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018513.D
Acq On : 02 Dec 2023 13:12
Operator : MA/JU
Sample : 05416-21
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AH4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018513.D
Acq On : 02 Dec 2023 13:12
Operator : MA/JU
Sample : 05416-21
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AH4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc