

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018517.D
 Acq On : 02 Dec 2023 16:02
 Operator : MA/JU
 Sample : PB157321BL
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK321

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018517.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	37	rBV	133001	168037	1.52%	0.153%
2	3.687	98	102	116	rBV	1550782	2255786	20.43%	2.059%
3	4.022	155	159	163	rBV2	22762	34931	0.32%	0.032%
4	7.028	662	670	678	rBV	1969917	3009262	27.26%	2.746%
5	7.199	691	699	707	rBV	1663555	2531776	22.93%	2.311%
6	7.393	723	732	744	rBV	1922378	3032991	27.47%	2.768%
7	7.863	804	812	819	rBV	1453070	2294494	20.78%	2.094%
8	8.569	924	932	943	rBV	2384190	3828979	34.68%	3.495%
9	9.022	1001	1009	1016	rBV	1825916	2940589	26.64%	2.684%
10	9.199	1034	1039	1042	rVB5	7709	15175	0.14%	0.014%
11	9.740	1123	1131	1145	rBV	1426738	2329090	21.10%	2.126%
12	10.275	1212	1222	1234	rBV	2291234	3857503	34.94%	3.521%
13	10.657	1280	1287	1295	rBV	2082848	3421885	31.00%	3.123%
14	10.798	1302	1311	1322	rBV	1862847	3128320	28.34%	2.855%
15	12.245	1550	1557	1564	rVB3	44516	78558	0.71%	0.072%
16	13.392	1748	1752	1757	rBV2	22601	31736	0.29%	0.029%
17	13.904	1832	1839	1846	rBV	3912148	5430818	49.19%	4.956%
18	14.181	1880	1886	1895	rBV	4593460	6787262	61.48%	6.194%
19	14.486	1932	1938	1946	rBV	3131544	4542359	41.15%	4.146%
20	14.686	1964	1972	1989	rBV	1830434	2662881	24.12%	2.430%
21	14.851	1997	2000	2004	rVB2	9325	13113	0.12%	0.012%
22	14.892	2004	2007	2012	rBV3	9197	13227	0.12%	0.012%
23	15.481	2100	2107	2117	rBV	5863779	8217625	74.44%	7.500%
24	15.592	2120	2126	2141	rVV	1404663	1980631	17.94%	1.808%
25	15.722	2144	2148	2153	rVB2	27228	45872	0.42%	0.042%
26	16.263	2237	2240	2245	rBV4	9430	12338	0.11%	0.011%
27	16.722	2314	2318	2322	rBV4	5696	11305	0.10%	0.010%
28	17.016	2367	2368	2377	rVB3	10912	18817	0.17%	0.017%
29	17.233	2399	2405	2412	rBV	3655739	5069048	45.92%	4.626%
30	17.333	2415	2422	2434	rBV	6122647	8458346	76.62%	7.720%
31	18.122	2553	2556	2562	rBV3	28925	35796	0.32%	0.033%
32	18.439	2607	2610	2611	rBV2	11732	12386	0.11%	0.011%
33	19.145	2726	2730	2735	rBV3	79146	108825	0.99%	0.099%
34	19.216	2737	2742	2747	rBV	76547	109729	0.99%	0.100%
35	19.357	2764	2766	2770	rBV3	24996	23522	0.21%	0.021%
36	19.569	2796	2802	2809	rBV	7691026	9940573	90.04%	9.072%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018517.D
Acq On : 02 Dec 2023 16:02
Operator : MA/JU
Sample : PB157321BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK321

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	21.316	3094	3099	3108	rBV	4387507	5734550	51.94%	5.234%
38	23.539	3470	3477	3485	rBV2	5789717	11039817	100.00%	10.076%
39	23.692	3496	3503	3513	rVB	3161677	6342487	57.45%	5.789%




Sum of corrected areas: 109570439

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018517.D
Acq On : 02 Dec 2023 16:02
Operator : MA/JU
Sample : PB157321BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK321

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

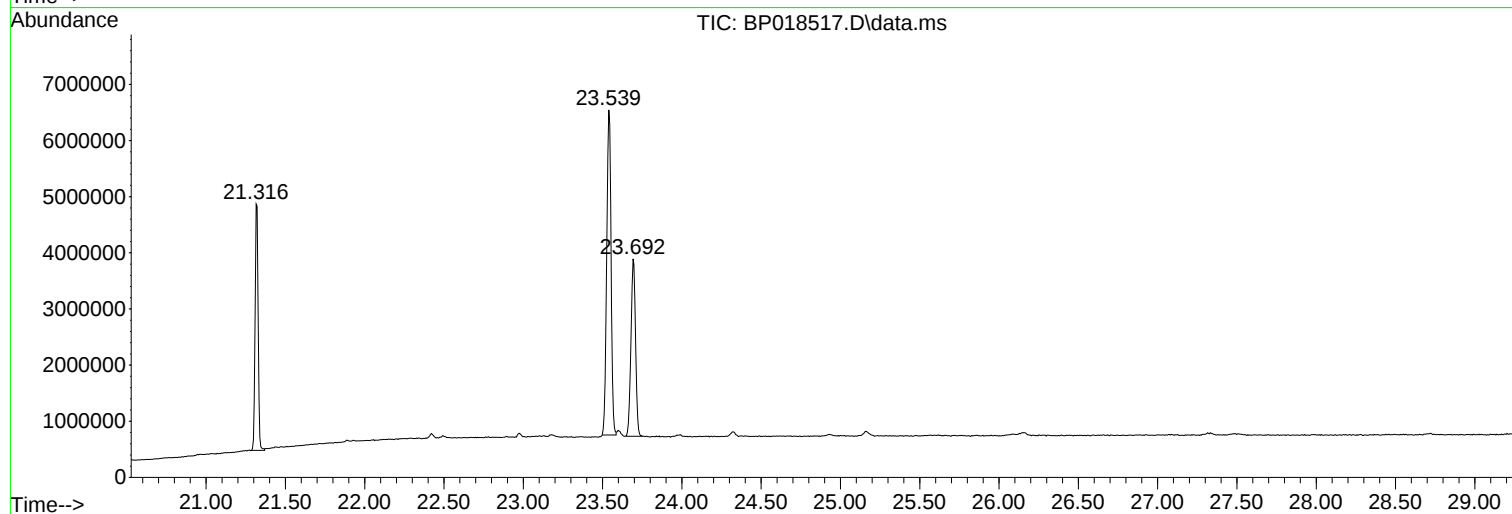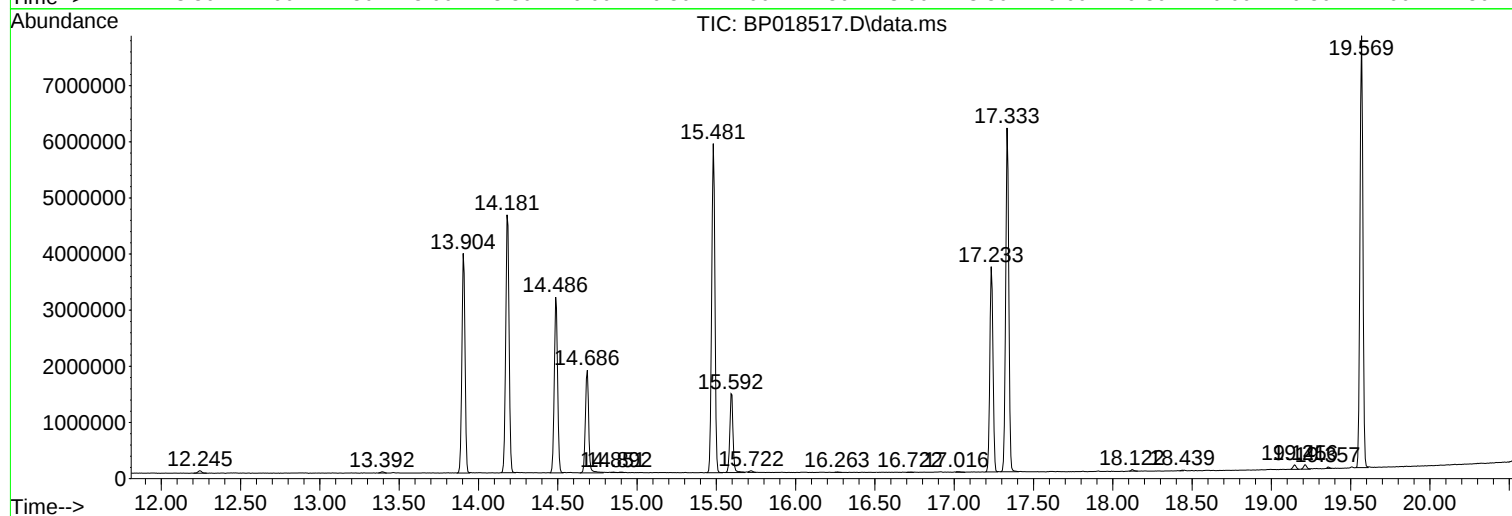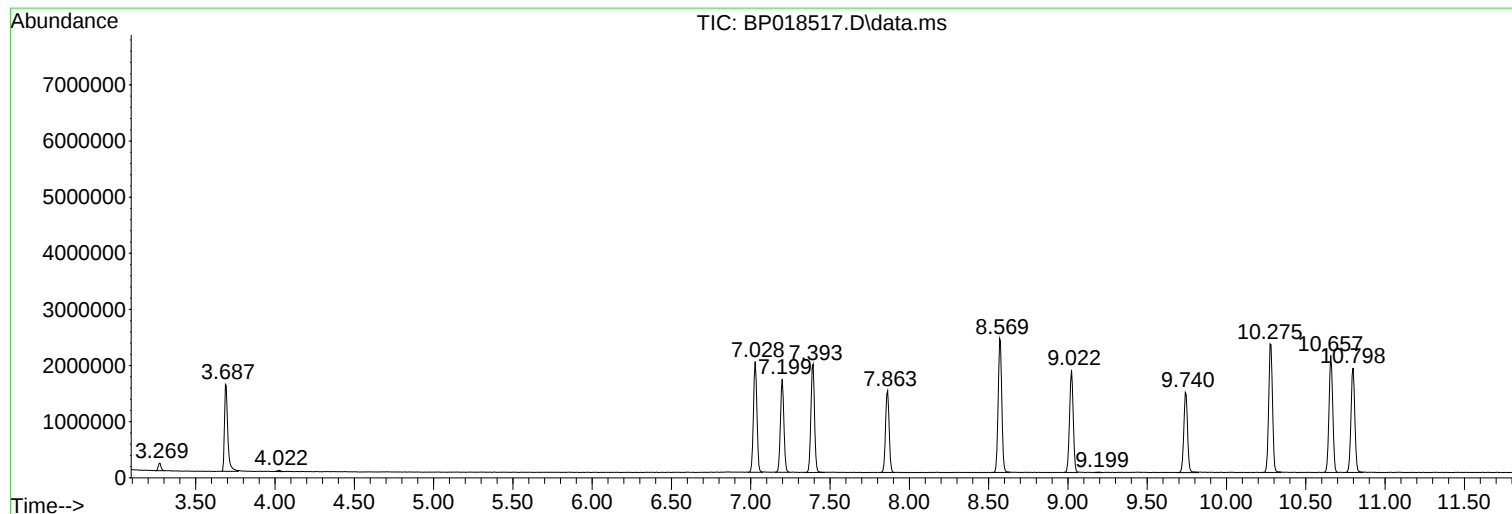

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018517.D
Acq On : 02 Dec 2023 16:02
Operator : MA/JU
Sample : PB157321BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK321

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018517.D
Acq On : 02 Dec 2023 16:02
Operator : MA/JU
Sample : PB157321BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK321

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc