

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018518.D
 Acq On : 02 Dec 2023 16:36
 Operator : MA/JU
 Sample : PB157322BL
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK322

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018518.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	39	rVB	135896	168409	1.50%	0.150%
2	3.687	98	102	117	rBV	1565392	2238527	20.00%	1.990%
3	4.028	155	160	163	rBV2	22747	31647	0.28%	0.028%
4	7.028	663	670	680	rBV	1915916	2920134	26.09%	2.596%
5	7.199	692	699	708	rVB	1621404	2471831	22.09%	2.197%
6	7.393	724	732	741	rBV	1805455	2892058	25.84%	2.571%
7	7.858	803	811	821	rBV	1329376	2160454	19.31%	1.920%
8	8.569	924	932	944	rBV	2387614	3800775	33.96%	3.378%
9	9.022	1000	1009	1017	rBV	1822009	2953377	26.39%	2.625%
10	9.193	1031	1038	1043	rVB4	12326	23104	0.21%	0.021%
11	9.740	1124	1131	1141	rBV	1442829	2307270	20.62%	2.051%
12	10.275	1212	1222	1234	rBV	2403747	3929624	35.11%	3.493%
13	10.658	1277	1287	1295	rBV	2027428	3368719	30.10%	2.994%
14	10.799	1302	1311	1323	rBV	1955628	3292904	29.43%	2.927%
15	12.240	1551	1556	1562	rVB3	48483	80690	0.72%	0.072%
16	13.399	1747	1753	1757	rBV3	27817	44981	0.40%	0.040%
17	13.463	1760	1764	1768	rBV5	8671	11689	0.10%	0.010%
18	13.904	1833	1839	1846	rBV	4851255	6504196	58.12%	5.781%
19	14.181	1879	1886	1895	rBV	5039067	7644305	68.31%	6.795%
20	14.487	1930	1938	1946	rBV	3496120	5027840	44.93%	4.469%
21	14.569	1950	1952	1956	rVB3	9074	11825	0.11%	0.011%
22	14.687	1965	1972	1988	rBV	2169220	3060768	27.35%	2.721%
23	14.840	1996	1998	2003	rVB2	8472	13233	0.12%	0.012%
24	14.898	2006	2008	2019	rVB3	11057	20339	0.18%	0.018%
25	15.481	2099	2107	2116	rBV	6856270	9708719	86.76%	8.630%
26	15.593	2119	2126	2140	rBV	1684058	2398959	21.44%	2.132%
27	15.716	2143	2147	2153	rVB3	33937	59894	0.54%	0.053%
28	16.916	2345	2351	2355	rVB4	10994	21393	0.19%	0.019%
29	17.016	2365	2368	2376	rVB3	9854	17805	0.16%	0.016%
30	17.234	2399	2405	2412	rVB	4337953	5996609	53.59%	5.330%
31	17.334	2415	2422	2437	rBV2	7315104	10210212	91.24%	9.076%
32	17.616	2468	2470	2474	rVB3	11539	13829	0.12%	0.012%
33	18.128	2553	2557	2561	rVB4	27161	35672	0.32%	0.032%
34	19.145	2726	2730	2736	rBV	90468	122176	1.09%	0.109%
35	19.216	2737	2742	2746	rBV	89690	121993	1.09%	0.108%
36	19.569	2796	2802	2808	rBV	8565478	11190762	100.00%	9.947%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018518.D
Acq On : 02 Dec 2023 16:36
Operator : MA/JU
Sample : PB157322BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK322

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	21.322	3095	3100	3106	rBV	3978825	5019523	44.85%	4.462%
38	23.539	3470	3477	3484	rBV2	4221510	8056559	71.99%	7.161%
39	23.692	3496	3503	3514	rVB	2372289	4547660	40.64%	4.042%




Sum of corrected areas: 112500464

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018518.D
Acq On : 02 Dec 2023 16:36
Operator : MA/JU
Sample : PB157322BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK322

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

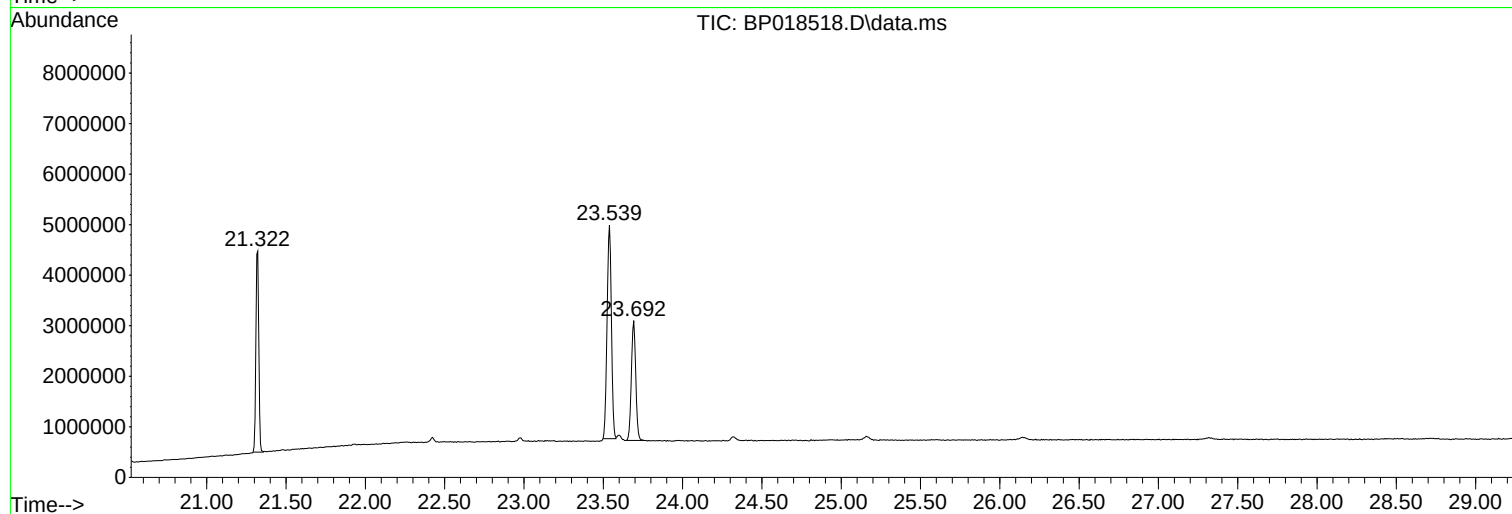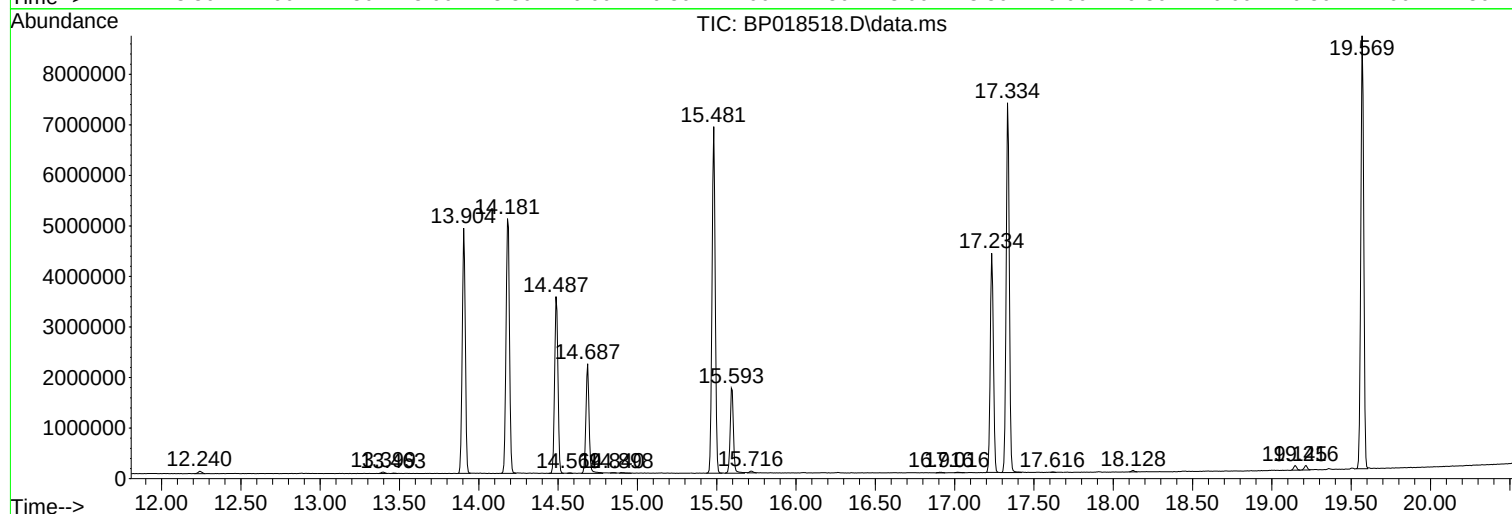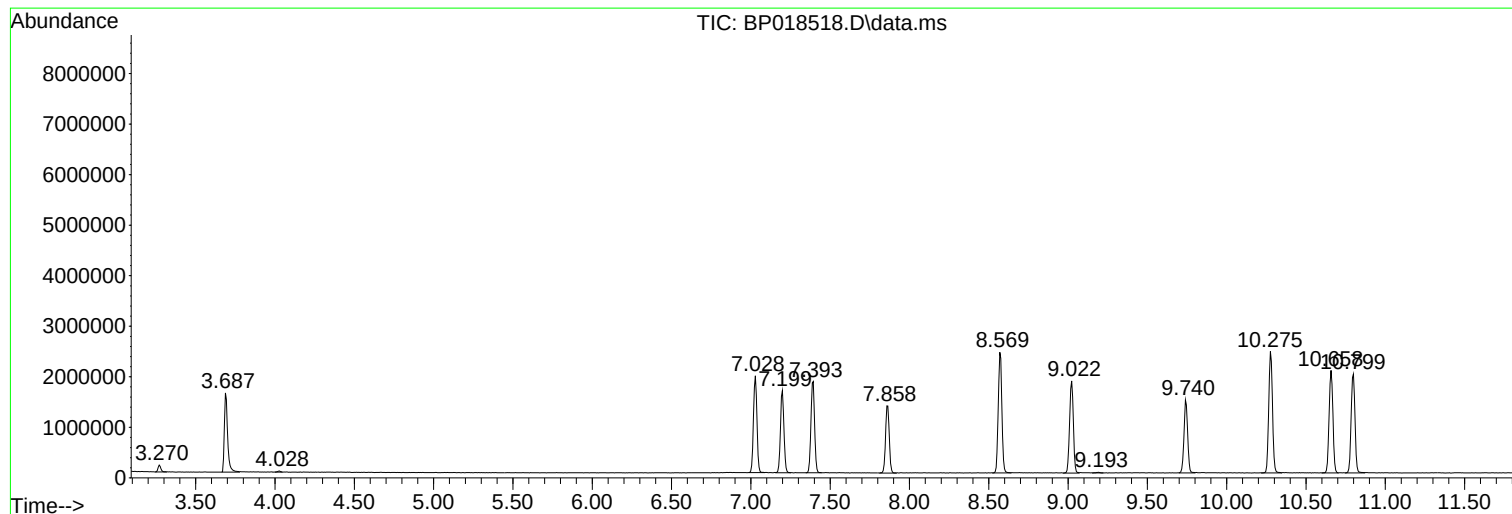

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018518.D
Acq On : 02 Dec 2023 16:36
Operator : MA/JU
Sample : PB157322BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK322

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018518.D
Acq On : 02 Dec 2023 16:36
Operator : MA/JU
Sample : PB157322BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK322

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------