

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018522.D
 Acq On : 02 Dec 2023 18:52
 Operator : MA/JU
 Sample : 05411-05
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018522.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	28	31	37	rVB	94034	119237	1.03%	0.122%
2	3.693	99	103	114	rBV	544455	754884	6.55%	0.770%
3	3.934	140	144	149	rVB	23906	35575	0.31%	0.036%
4	4.022	155	159	163	rBV	29356	35297	0.31%	0.036%
5	4.975	315	321	325	rVB4	10322	19950	0.17%	0.020%
6	7.028	663	670	685	rVB	393891	638901	5.54%	0.652%
7	7.193	691	698	712	rBV	1463682	2322435	20.15%	2.369%
8	7.387	723	731	740	rBV	1374333	2145881	18.62%	2.189%
9	7.487	743	748	752	rVB4	10394	14081	0.12%	0.014%
10	7.858	804	811	821	rBV	1544643	2473213	21.46%	2.523%
11	8.569	925	932	940	rBV	1103452	1724738	14.97%	1.760%
12	9.022	1000	1009	1015	rBV	1631447	2617835	22.71%	2.671%
13	9.193	1033	1038	1043	rVB3	13663	20331	0.18%	0.021%
14	9.452	1075	1082	1093	rVB5	9753	23009	0.20%	0.023%
15	9.740	1123	1131	1138	rBV	1153994	1874922	16.27%	1.913%
16	10.275	1215	1222	1233	rBV	1855162	3050653	26.47%	3.112%
17	10.657	1278	1287	1297	rBV	2140905	3542593	30.74%	3.614%
18	10.793	1302	1310	1318	rBV	1667028	2825221	24.51%	2.882%
19	12.240	1550	1556	1564	rVB2	39419	68470	0.59%	0.070%
20	13.393	1748	1752	1759	rVB2	31112	49992	0.43%	0.051%
21	13.457	1759	1763	1766	rBV	12030	16819	0.15%	0.017%
22	13.904	1832	1839	1849	rBV	3484388	4718487	40.94%	4.814%
23	14.181	1878	1886	1899	rBV	3998076	5832536	50.61%	5.950%
24	14.487	1928	1938	1945	rBV	3185718	4579263	39.73%	4.672%
25	14.681	1966	1971	1979	rBV	309235	460823	4.00%	0.470%
26	14.904	2005	2009	2013	rBV5	18095	29650	0.26%	0.030%
27	15.481	2098	2107	2114	rBV	5342127	7548301	65.49%	7.701%
28	15.592	2120	2126	2134	rBV	1314813	1761591	15.28%	1.797%
29	15.722	2143	2148	2152	rVB	24700	35346	0.31%	0.036%
30	16.263	2236	2240	2244	rVB3	14766	15133	0.13%	0.015%
31	17.022	2363	2369	2371	rBV3	10832	20345	0.18%	0.021%
32	17.234	2399	2405	2412	rVB	3664369	5144152	44.63%	5.248%
33	17.334	2415	2422	2435	rVV	5904599	8380414	72.71%	8.550%
34	17.428	2435	2438	2442	rVB3	13602	18970	0.16%	0.019%
35	17.904	2517	2519	2525	rVB7	11510	14513	0.13%	0.015%
36	18.122	2552	2556	2562	rBV	153421	210250	1.82%	0.214%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018522.D
Acq On : 02 Dec 2023 18:52
Operator : MA/JU
Sample : 05411-05
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	19.145	2726	2730	2736	rBV2	79202	98161	0.85%	0.100%
38	19.210	2737	2741	2745	rBV	84858	122544	1.06%	0.125%
39	19.357	2762	2766	2773	rBV2	152490	202279	1.76%	0.206%
40	19.504	2789	2791	2795	rBV5	19181	21617	0.19%	0.022%
41	19.569	2796	2802	2808	rVV	7852236	10112970	87.75%	10.317%
42	21.322	3094	3100	3109	rBV	4537404	6009763	52.15%	6.131%
43	23.539	3469	3477	3485	rBV2	5796899	11525040	100.00%	11.758%
44	23.692	3496	3503	3515	rVB	3374407	6783744	58.86%	6.921%




Sum of corrected areas: 98019929

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018522.D
Acq On : 02 Dec 2023 18:52
Operator : MA/JU
Sample : 05411-05
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

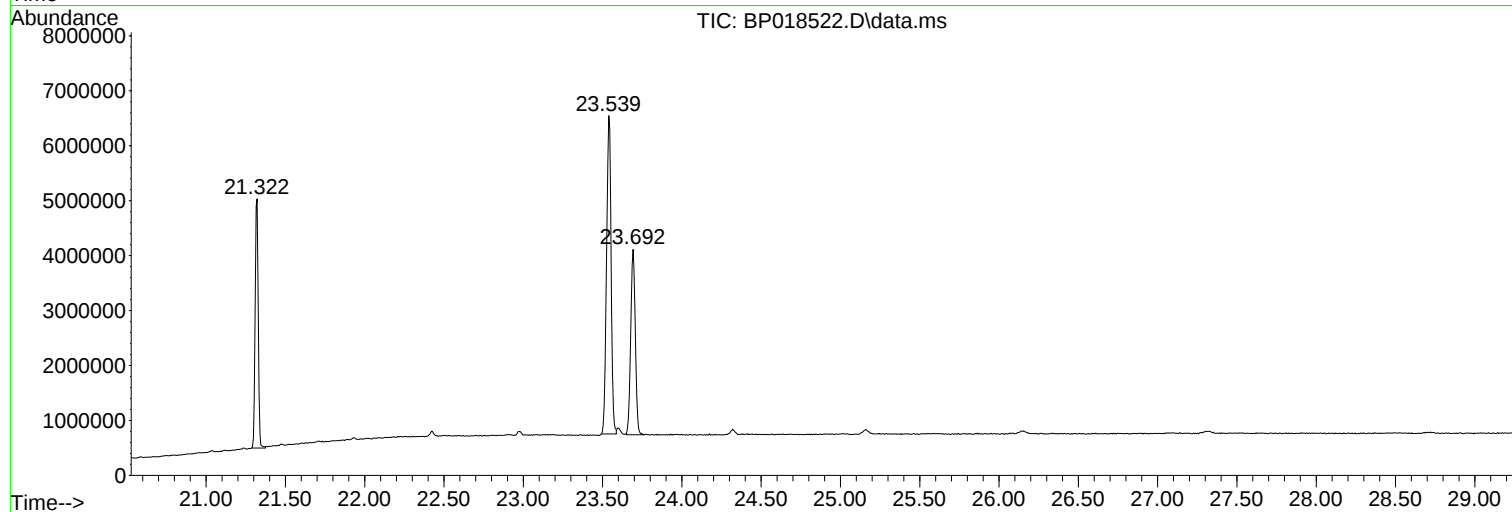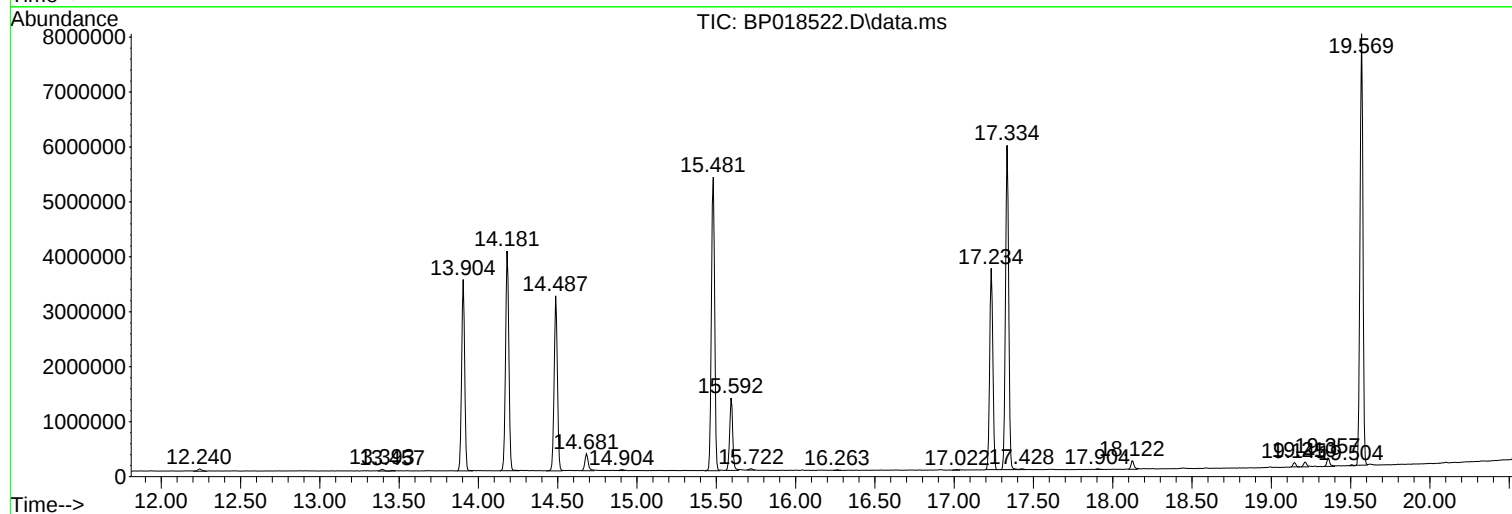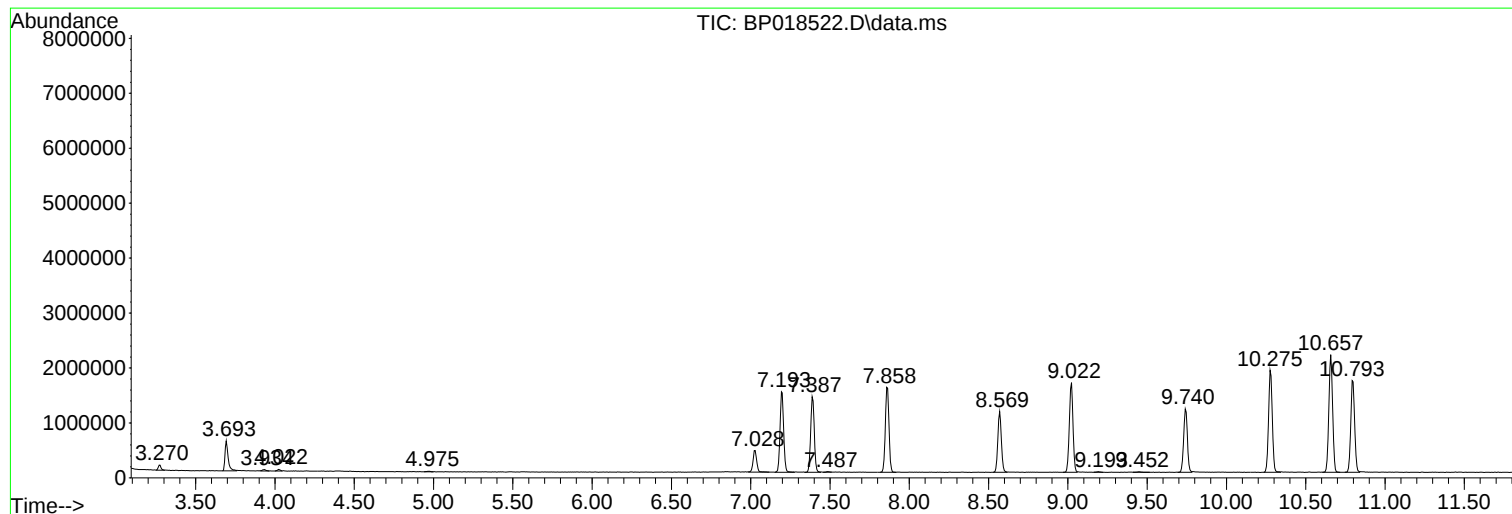

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018522.D
Acq On : 02 Dec 2023 18:52
Operator : MA/JU
Sample : 05411-05
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018522.D
Acq On : 02 Dec 2023 18:52
Operator : MA/JU
Sample : 05411-05
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc