

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018524.D
 Acq On : 02 Dec 2023 20:00
 Operator : MA/JU
 Sample : 05411-07
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018524.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	39	rVB	98626	124249	0.97%	0.109%
2	3.693	99	103	117	rBV	419475	607472	4.73%	0.531%
3	3.934	139	144	150	rVB2	27361	44524	0.35%	0.039%
4	4.022	155	159	164	rVB	29768	42051	0.33%	0.037%
5	7.028	664	670	676	rVB	351364	549136	4.27%	0.480%
6	7.193	691	698	707	rVB	1506634	2393559	18.63%	2.091%
7	7.387	725	731	739	rBV	1318029	2063931	16.07%	1.803%
8	7.858	803	811	819	rBV	1659444	2657308	20.68%	2.321%
9	8.569	924	932	942	rBV	1113329	1709329	13.31%	1.493%
10	9.022	1001	1009	1020	rBV	1777890	2864803	22.30%	2.502%
11	9.193	1034	1038	1042	rVB3	11330	17085	0.13%	0.015%
12	9.740	1124	1131	1147	rBV	1268381	2057469	16.02%	1.797%
13	10.275	1214	1222	1232	rBV	2035189	3363166	26.18%	2.938%
14	10.657	1279	1287	1295	rBV	2563773	4204578	32.73%	3.673%
15	10.793	1302	1310	1323	rBV	2000234	3427354	26.68%	2.994%
16	11.934	1498	1504	1510	rVB5	5731	12854	0.10%	0.011%
17	12.240	1552	1556	1562	rVB2	44918	72891	0.57%	0.064%
18	13.116	1700	1705	1710	rVB2	26400	42144	0.33%	0.037%
19	13.393	1747	1752	1760	rBV2	40128	65952	0.51%	0.058%
20	13.457	1760	1763	1767	rBV3	9730	16451	0.13%	0.014%
21	13.904	1832	1839	1846	rBV	4749231	6461065	50.29%	5.644%
22	14.181	1877	1886	1894	rBV	5145548	7459310	58.06%	6.515%
23	14.487	1931	1938	1947	rBV	4257080	6304517	49.07%	5.507%
24	14.681	1965	1971	1981	rBV	354659	534094	4.16%	0.467%
25	14.904	2005	2009	2014	rVB4	24230	39982	0.31%	0.035%
26	15.481	2099	2107	2117	rBV	6906942	9878905	76.90%	8.629%
27	15.592	2119	2126	2137	rBV	1882768	2540094	19.77%	2.219%
28	15.716	2143	2147	2151	rVB3	30191	43828	0.34%	0.038%
29	16.263	2237	2240	2245	rVB3	12588	17311	0.13%	0.015%
30	16.775	2323	2327	2332	rBV3	10820	16589	0.13%	0.014%
31	16.910	2346	2350	2356	rVB3	12056	21978	0.17%	0.019%
32	17.022	2362	2369	2372	rBV3	13486	23999	0.19%	0.021%
33	17.234	2398	2405	2412	rBV	5428410	7680262	59.78%	6.708%
34	17.334	2415	2422	2434	rVV2	7953335	11287592	87.86%	9.859%
35	17.616	2466	2470	2474	rVB3	11265	16103	0.13%	0.014%
36	17.910	2517	2520	2524	rVB5	12510	16902	0.13%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018524.D
 Acq On : 02 Dec 2023 20:00
 Operator : MA/JU
 Sample : 05411-07
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	18.122	2552	2556	2565	rBV	180686	255744	1.99%	0.223%
38	19.145	2726	2730	2735	rBV3	102002	138499	1.08%	0.121%
39	19.210	2737	2741	2746	rBV	109515	150433	1.17%	0.131%
40	19.357	2762	2766	2773	rBV3	167941	226234	1.76%	0.198%
41	19.510	2789	2792	2795	rBV4	28825	32497	0.25%	0.028%
42	19.569	2796	2802	2809	rVV	9940479	12847064	100.00%	11.222%
43	19.792	2837	2840	2845	rVB	83496	89789	0.70%	0.078%
44	21.316	3094	3099	3105	rBV	5517287	6854611	53.36%	5.987%
45	23.539	3469	3477	3484	rBV2	4777168	9306494	72.44%	8.129%
46	23.692	3496	3503	3516	rVB	3084918	5905557	45.97%	5.158%




Sum of corrected areas: 114485759

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018524.D
Acq On : 02 Dec 2023 20:00
Operator : MA/JU
Sample : 05411-07
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

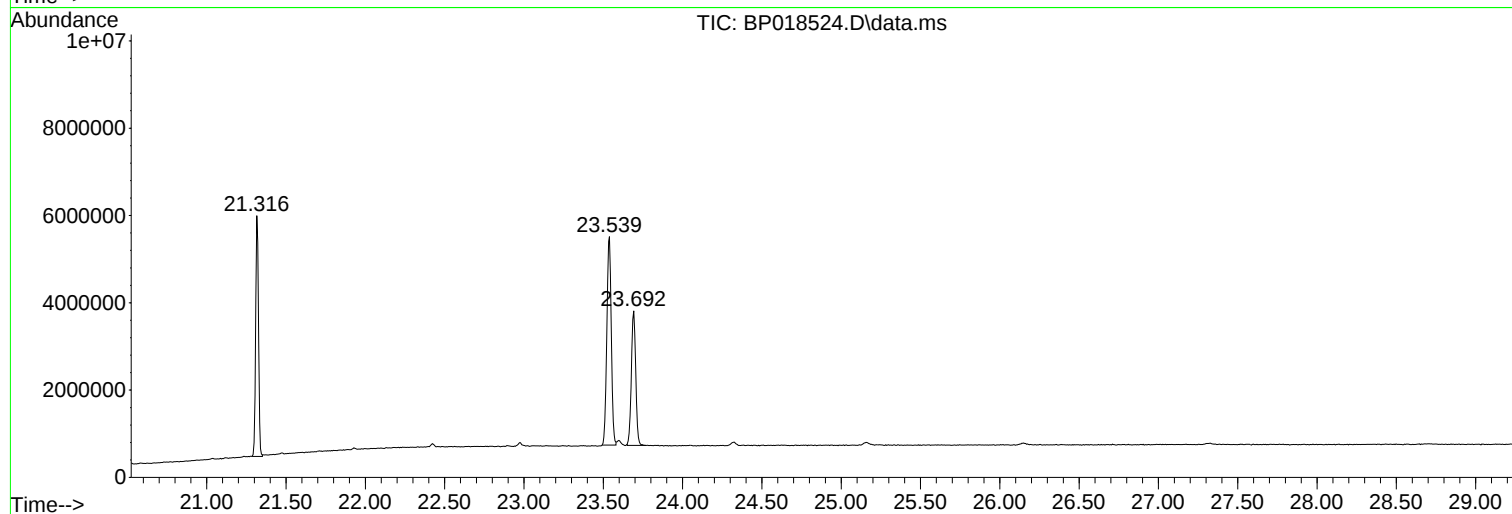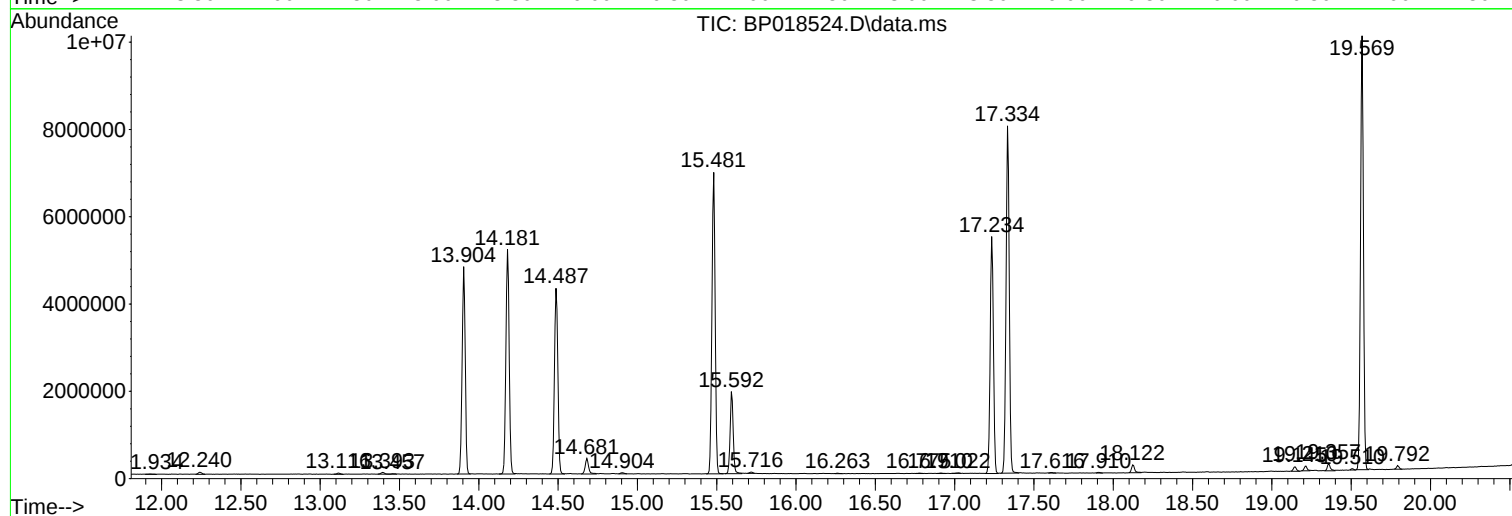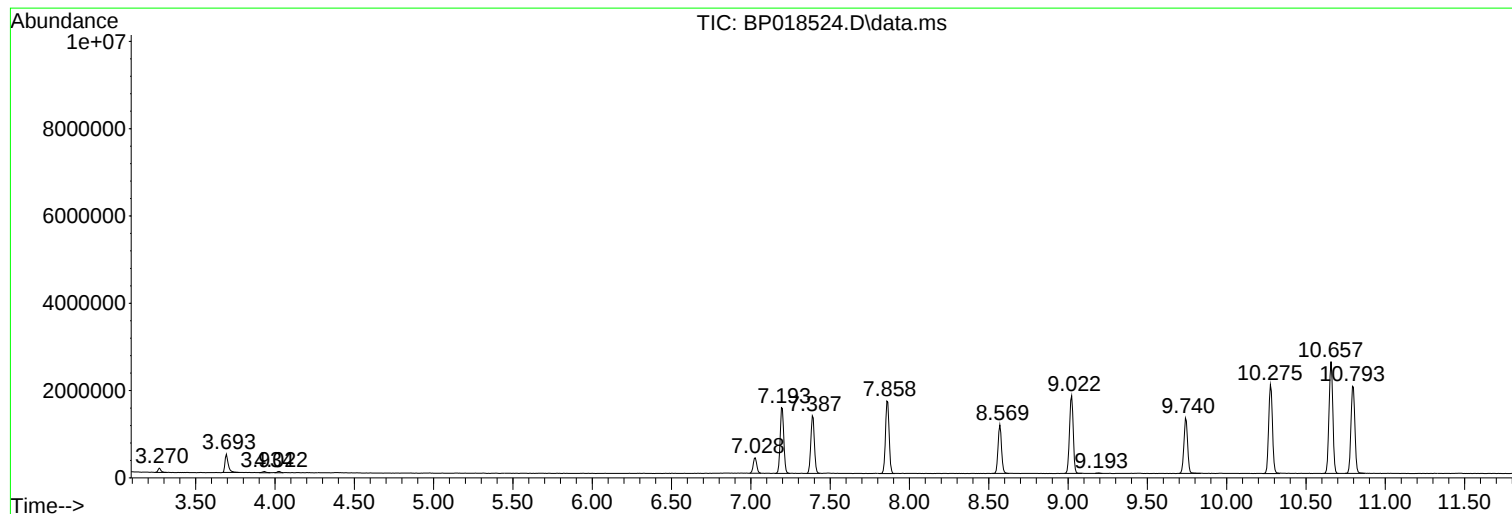

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018524.D
Acq On : 02 Dec 2023 20:00
Operator : MA/JU
Sample : 05411-07
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018524.D
Acq On : 02 Dec 2023 20:00
Operator : MA/JU
Sample : 05411-07
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc