

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018525.D
 Acq On : 02 Dec 2023 20:34
 Operator : MA/JU
 Sample : 05411-08
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QH0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018525.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	28	31	37	rVB	105159	123312	1.15%	0.127%
2	3.693	99	103	115	rBV	597589	842400	7.88%	0.866%
3	3.934	138	144	149	rBV2	26574	43212	0.40%	0.044%
4	4.028	156	160	168	rVB	26470	36549	0.34%	0.038%
5	4.964	316	319	325	rBV5	8585	12413	0.12%	0.013%
6	5.134	345	348	351	rBV	12176	14491	0.14%	0.015%
7	6.852	635	640	644	rBV4	6622	14374	0.13%	0.015%
8	7.028	662	670	678	rVB	381227	604062	5.65%	0.621%
9	7.199	691	699	707	rBV	1593414	2492721	23.32%	2.563%
10	7.387	723	731	738	rBV	1407644	2222211	20.79%	2.285%
11	7.858	803	811	824	rBV	1489753	2407620	22.52%	2.476%
12	8.569	925	932	943	rBV	1179988	1790201	16.75%	1.841%
13	9.022	999	1009	1018	rBV	1781502	2883882	26.98%	2.966%
14	9.187	1033	1037	1044	rVB4	11847	19920	0.19%	0.020%
15	9.452	1077	1082	1086	rVB6	8674	14931	0.14%	0.015%
16	9.740	1122	1131	1140	rBV	1287181	2065895	19.33%	2.124%
17	10.275	1215	1222	1232	rBV	2033302	3300656	30.88%	3.394%
18	10.657	1279	1287	1295	rBV	2131443	3509215	32.83%	3.609%
19	10.793	1301	1310	1329	rVB	1820574	3071975	28.74%	3.159%
20	11.469	1424	1425	1431	rVB3	12847	16014	0.15%	0.016%
21	12.187	1541	1547	1551	rBV2	34435	58104	0.54%	0.060%
22	12.240	1551	1556	1562	rVB2	37979	61343	0.57%	0.063%
23	13.116	1699	1705	1708	rVB4	14149	19779	0.19%	0.020%
24	13.393	1748	1752	1758	rVB2	16401	24621	0.23%	0.025%
25	13.457	1760	1763	1769	rVB6	8751	13005	0.12%	0.013%
26	13.904	1832	1839	1848	rBV	3800491	5162541	48.29%	5.309%
27	14.181	1870	1886	1896	rBV	4447499	6374415	59.63%	6.555%
28	14.487	1931	1938	1946	rBV	3059250	4514361	42.23%	4.642%
29	14.681	1965	1971	1977	rBV	250048	373385	3.49%	0.384%
30	14.898	2004	2008	2015	rVB6	14436	28713	0.27%	0.030%
31	15.481	2100	2107	2119	rBV	5432116	7933199	74.21%	8.158%
32	15.592	2120	2126	2139	rVV	1275765	1734793	16.23%	1.784%
33	15.716	2143	2147	2155	rVB3	27417	50809	0.48%	0.052%
34	16.263	2237	2240	2248	rBV6	9689	13118	0.12%	0.013%
35	16.910	2348	2350	2355	rVB5	8614	11822	0.11%	0.012%
36	17.234	2398	2405	2411	rBV	3513130	4912461	45.95%	5.052%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018525.D
 Acq On : 02 Dec 2023 20:34
 Operator : MA/JU
 Sample : 05411-08
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QH0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	17.334	2415	2422	2435	rVV2	5609362	8147405	76.22%	8.378%
38	17.616	2466	2470	2473	rBV3	9578	13449	0.13%	0.014%
39	17.710	2482	2486	2491	rBV3	50819	69438	0.65%	0.071%
40	17.904	2516	2519	2524	rVB5	16338	22304	0.21%	0.023%
41	18.122	2552	2556	2560	rBV3	109738	140677	1.32%	0.145%
42	18.328	2587	2591	2595	rBV	40233	51201	0.48%	0.053%
43	18.586	2633	2635	2641	rBV4	10567	17222	0.16%	0.018%
44	19.145	2726	2730	2736	rBV2	76250	109184	1.02%	0.112%
45	19.216	2737	2742	2746	rBV	76758	118435	1.11%	0.122%
46	19.357	2762	2766	2771	rBV3	108958	138438	1.30%	0.142%
47	19.569	2796	2802	2808	rBV	7321808	9446934	88.37%	9.715%
48	21.316	3094	3099	3108	rBV	4245071	5399674	50.51%	5.553%
49	23.539	3469	3477	3485	rBV2	5564650	10689787	100.00%	10.993%
50	23.692	3496	3503	3514	rVB	3175551	6105978	57.12%	6.279%




Sum of corrected areas: 97242649

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018525.D
Acq On : 02 Dec 2023 20:34
Operator : MA/JU
Sample : 05411-08
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QH0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

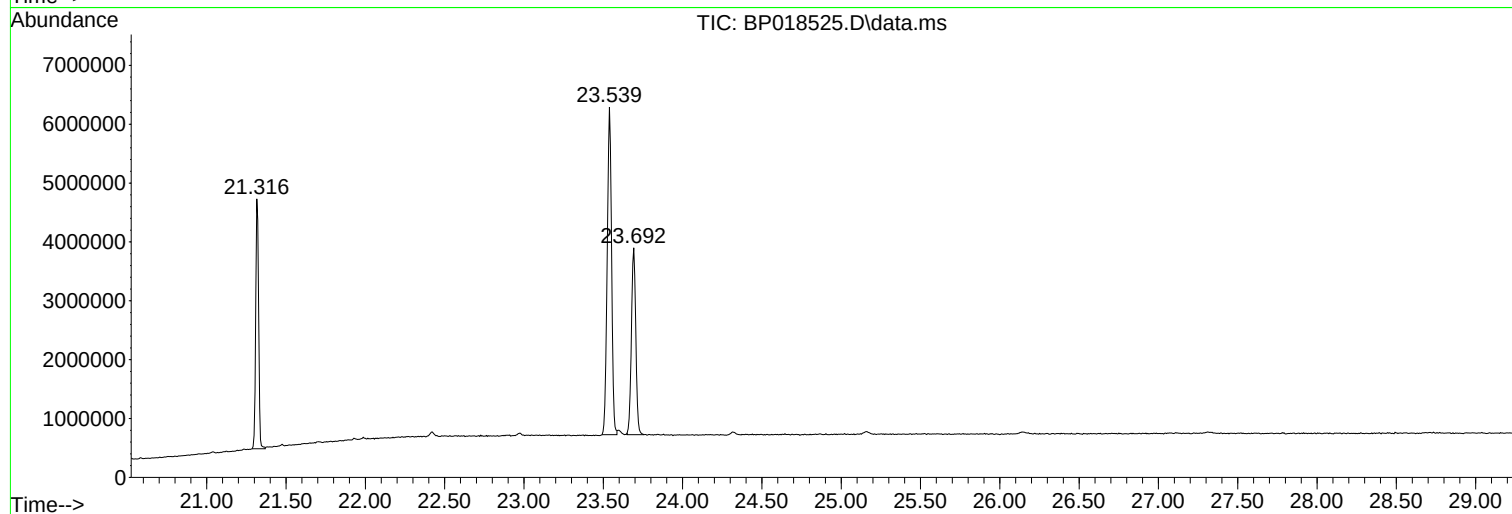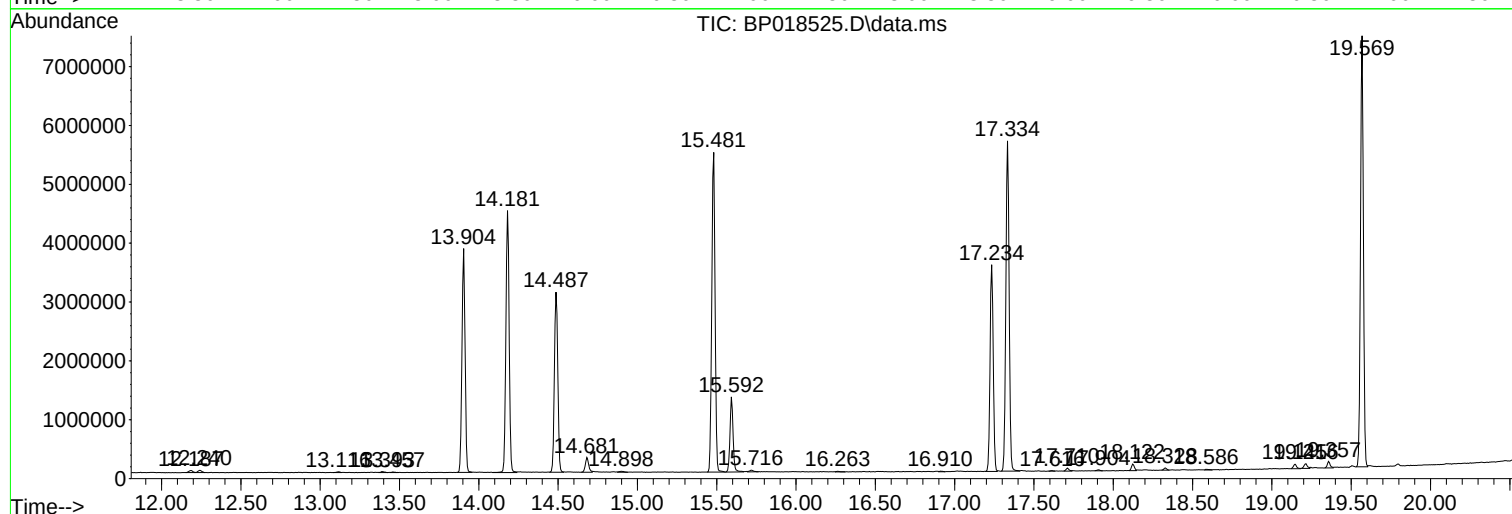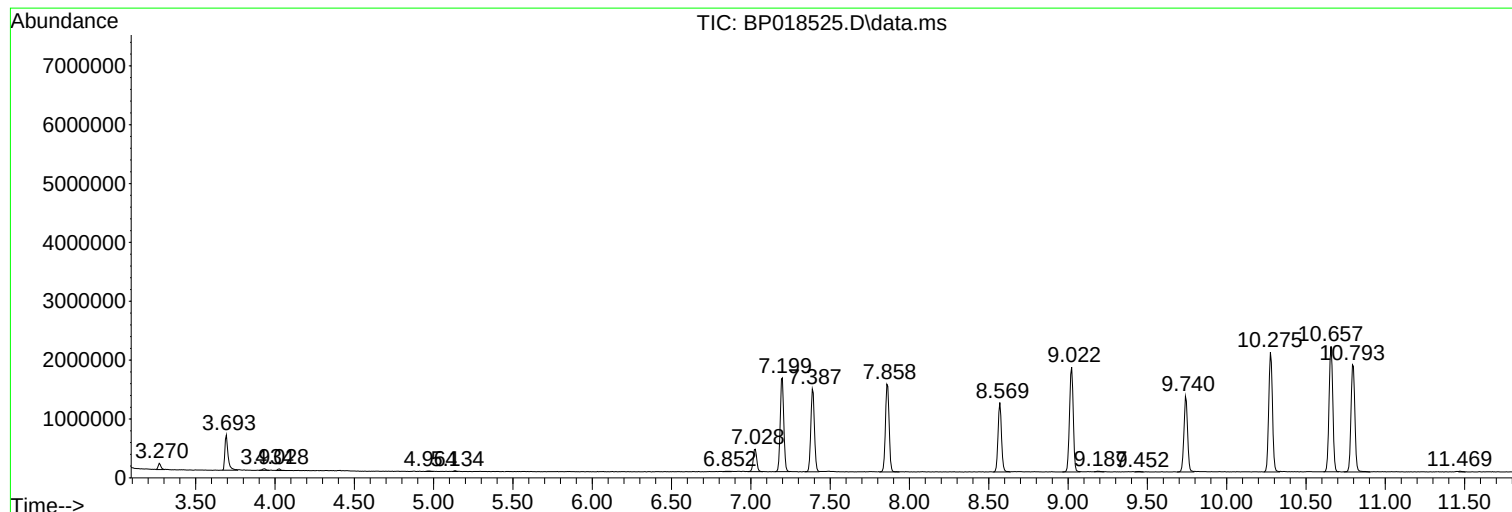

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018525.D
Acq On : 02 Dec 2023 20:34
Operator : MA/JU
Sample : 05411-08
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QH0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018525.D
Acq On : 02 Dec 2023 20:34
Operator : MA/JU
Sample : 05411-08
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QH0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
