

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018526.D
 Acq On : 02 Dec 2023 21:07
 Operator : MA/JU
 Sample : 05411-09
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QH2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018526.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	22	25	28	rBV	30674	36808	0.28%	0.031%
2	3.270	28	31	38	rVB	92492	111886	0.84%	0.094%
3	3.693	99	103	115	rBV	543838	810125	6.10%	0.680%
4	3.928	139	143	147	rVB	23973	34846	0.26%	0.029%
5	4.022	155	159	165	rBV2	32571	48150	0.36%	0.040%
6	4.969	316	320	326	rVB5	14353	29322	0.22%	0.025%
7	7.022	663	669	676	rBV	393519	613056	4.62%	0.515%
8	7.193	692	698	708	rVB	1698199	2629226	19.81%	2.208%
9	7.387	724	731	740	rBV	1475414	2313505	17.43%	1.943%
10	7.858	803	811	819	rBV	1603496	2561716	19.30%	2.151%
11	8.569	925	932	944	rBV	1217198	1887107	14.22%	1.585%
12	9.022	1000	1009	1019	rBV	1912277	3187398	24.02%	2.677%
13	9.199	1034	1039	1044	rVB3	7899	15928	0.12%	0.013%
14	9.446	1077	1081	1085	rBV2	19044	28844	0.22%	0.024%
15	9.740	1123	1131	1146	rBV	1471310	2352812	17.73%	1.976%
16	10.275	1214	1222	1233	rBV	2320303	3768110	28.39%	3.164%
17	10.657	1279	1287	1296	rBV	2484614	4091062	30.82%	3.436%
18	10.793	1303	1310	1320	rBV	2127605	3585396	27.01%	3.011%
19	11.934	1501	1504	1510	rVB3	11502	17859	0.13%	0.015%
20	12.240	1551	1556	1563	rVB3	50093	75897	0.57%	0.064%
21	13.116	1700	1705	1711	rVB	17330	26021	0.20%	0.022%
22	13.275	1728	1732	1737	rBV3	8007	16513	0.12%	0.014%
23	13.322	1737	1740	1744	rVV5	9633	14038	0.11%	0.012%
24	13.393	1744	1752	1758	rVB3	42672	70985	0.53%	0.060%
25	13.457	1758	1763	1766	rBV4	9607	14308	0.11%	0.012%
26	13.904	1828	1839	1850	rBV	5305335	7270564	54.78%	6.106%
27	14.181	1879	1886	1901	rVB	5751834	8235889	62.05%	6.917%
28	14.487	1931	1938	1947	rBV	4052446	6049419	45.58%	5.080%
29	14.681	1965	1971	1983	rBV	388964	567448	4.28%	0.477%
30	14.904	2004	2009	2017	rVB7	27424	55452	0.42%	0.047%
31	15.481	2100	2107	2113	rBV	7568282	10966892	82.63%	9.210%
32	15.528	2113	2115	2119	rVB3	12977	16307	0.12%	0.014%
33	15.592	2119	2126	2137	rBV	2096979	2798518	21.09%	2.350%
34	15.716	2143	2147	2157	rVB2	36492	65312	0.49%	0.055%
35	16.040	2199	2202	2208	rVB5	9852	15481	0.12%	0.013%
36	16.534	2281	2286	2291	rBV4	10325	19312	0.15%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018526.D
 Acq On : 02 Dec 2023 21:07
 Operator : MA/JU
 Sample : 05411-09
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QH2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	16.875	2340	2344	2347	rBV3	8590	13352	0.10%	0.011%
38	16.910	2347	2350	2354	rVB4	12399	18975	0.14%	0.016%
39	17.016	2363	2368	2375	rBV2	17588	36570	0.28%	0.031%
40	17.234	2398	2405	2412	rBV	5270920	7179604	54.09%	6.029%
41	17.334	2415	2422	2434	rBV2	8416682	11929822	89.88%	10.019%
42	18.122	2552	2556	2563	rBV2	217538	303789	2.29%	0.255%
43	18.433	2607	2609	2615	rBV5	9859	17323	0.13%	0.015%
44	18.586	2632	2635	2637	rBV4	16023	16413	0.12%	0.014%
45	19.145	2725	2730	2734	rBV	106788	147952	1.11%	0.124%
46	19.210	2737	2741	2745	rBV	115792	164625	1.24%	0.138%
47	19.357	2762	2766	2773	rBV	216533	258848	1.95%	0.217%
48	19.504	2789	2791	2795	rVB4	30715	31116	0.23%	0.026%
49	19.569	2796	2802	2809	rVV	9963678	13272488	100.00%	11.146%
50	19.792	2837	2840	2845	rVB2	46675	54284	0.41%	0.046%
51	21.316	3094	3099	3105	rBV	4715930	6114904	46.07%	5.135%
52	23.539	3470	3477	3485	rBV2	5030441	9633249	72.58%	8.090%
53	23.692	3496	3503	3515	rVB	2784167	5480753	41.29%	4.603%




Sum of corrected areas: 119075579

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018526.D
Acq On : 02 Dec 2023 21:07
Operator : MA/JU
Sample : 05411-09
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QH2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

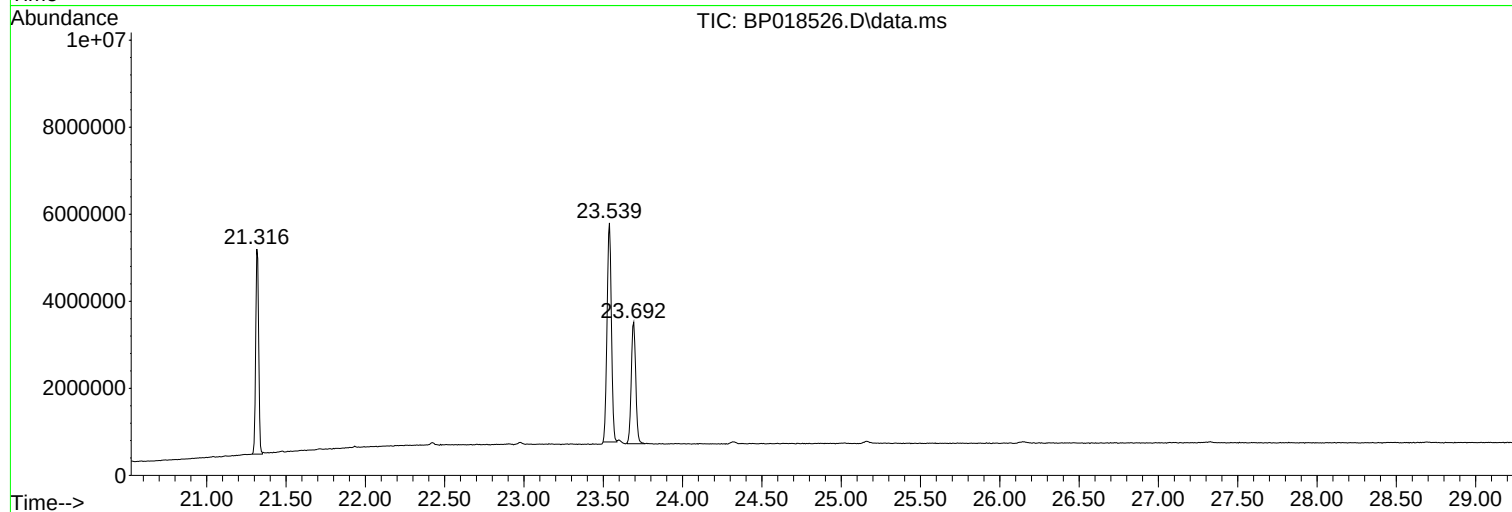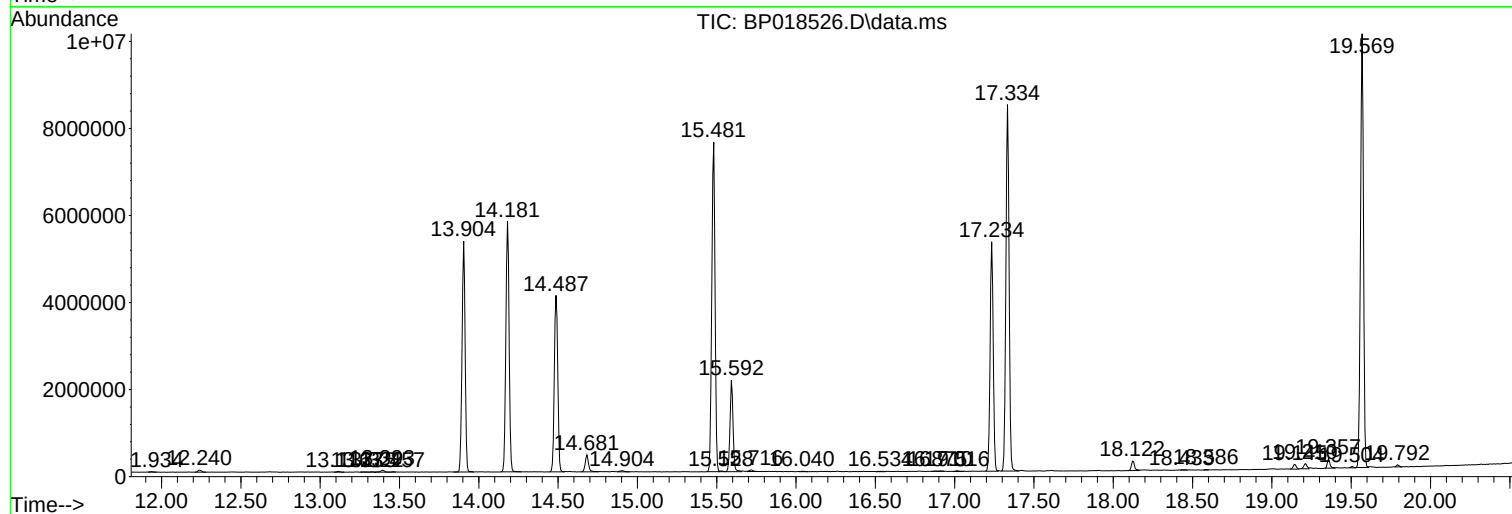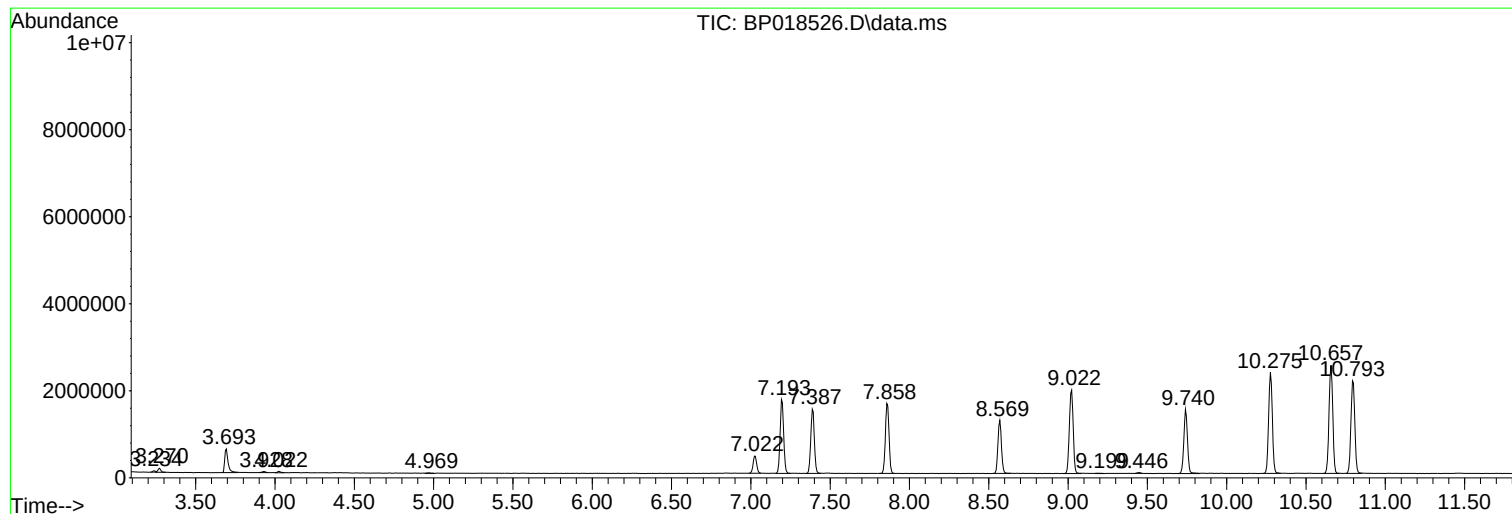

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018526.D
Acq On : 02 Dec 2023 21:07
Operator : MA/JU
Sample : 05411-09
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QH2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018526.D
Acq On : 02 Dec 2023 21:07
Operator : MA/JU
Sample : 05411-09
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QH2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
