

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018529.D
 Acq On : 02 Dec 2023 22:50
 Operator : MA/JU
 Sample : 05411-10
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QH5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018529.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	37	rVB	100352	125378	1.25%	0.118%
2	3.693	99	103	120	rBV	514322	750298	7.51%	0.706%
3	3.928	138	143	149	rVB2	24944	43762	0.44%	0.041%
4	4.023	155	159	166	rVB	36120	53814	0.54%	0.051%
5	5.564	417	421	425	rBV4	6015	10318	0.10%	0.010%
6	7.022	661	669	678	rVB	402267	635595	6.36%	0.598%
7	7.193	691	698	706	rBV	1682675	2608854	26.11%	2.454%
8	7.387	724	731	741	rBV	1452964	2281060	22.83%	2.146%
9	7.487	745	748	753	rVB4	9874	14375	0.14%	0.014%
10	7.858	803	811	818	rBV	1496666	2367927	23.70%	2.228%
11	8.569	925	932	940	rBV	1232963	1907046	19.08%	1.794%
12	9.022	1001	1009	1021	rBV	1974778	3176721	31.79%	2.988%
13	9.193	1032	1038	1041	rVB3	10460	15210	0.15%	0.014%
14	9.446	1076	1081	1089	rVB2	51838	85827	0.86%	0.081%
15	9.740	1123	1131	1141	rBV	1478066	2358547	23.60%	2.219%
16	10.275	1213	1222	1231	rBV	2272322	3706630	37.09%	3.487%
17	10.658	1279	1287	1298	rVB	2204646	3692742	36.95%	3.474%
18	10.793	1302	1310	1323	rBV	2158428	3723723	37.26%	3.503%
19	11.457	1416	1423	1425	rBV4	7524	14095	0.14%	0.013%
20	11.934	1498	1504	1513	rVB	64784	105456	1.06%	0.099%
21	12.240	1552	1556	1564	rVB3	51399	81311	0.81%	0.076%
22	13.116	1699	1705	1709	rBV2	30337	46558	0.47%	0.044%
23	13.393	1747	1752	1757	rBV2	46644	73363	0.73%	0.069%
24	13.904	1832	1839	1850	rVV	4773557	6613227	66.18%	6.221%
25	14.181	1878	1886	1898	rBV	5415854	7942575	79.48%	7.472%
26	14.487	1931	1938	1946	rBV	3561475	5206945	52.11%	4.898%
27	14.681	1965	1971	1980	rBV	291696	441736	4.42%	0.416%
28	14.904	2004	2009	2018	rVB6	25346	38386	0.38%	0.036%
29	15.481	2100	2107	2114	rBV	6852329	9808239	98.16%	9.227%
30	15.593	2120	2126	2137	rBV	1588780	2154123	21.56%	2.026%
31	15.716	2141	2147	2152	rVV2	37483	54387	0.54%	0.051%
32	15.975	2185	2191	2194	rBV3	5844	10642	0.11%	0.010%
33	16.263	2236	2240	2244	rBV3	11323	16914	0.17%	0.016%
34	16.640	2301	2304	2308	rBV2	6374	10075	0.10%	0.009%
35	16.775	2325	2327	2332	rBV3	7709	10288	0.10%	0.010%
36	16.910	2346	2350	2354	rBV5	9094	16226	0.16%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018529.D
 Acq On : 02 Dec 2023 22:50
 Operator : MA/JU
 Sample : 05411-10
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QH5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	17.022	2366	2369	2374	rVB3	10842	16711	0.17%	0.016%
38	17.234	2398	2405	2413	rBV	4028969	5624710	56.29%	5.291%
39	17.334	2415	2422	2434	rBV	6913136	9733361	97.41%	9.156%
40	17.904	2515	2519	2524	rVB6	8560	14360	0.14%	0.014%
41	18.122	2552	2556	2563	rBV	215828	282372	2.83%	0.266%
42	19.145	2726	2730	2736	rBV3	80870	104047	1.04%	0.098%
43	19.210	2737	2741	2745	rBV	84502	115127	1.15%	0.108%
44	19.357	2762	2766	2771	rBV2	203580	249738	2.50%	0.235%
45	19.504	2789	2791	2795	rVB4	21922	17918	0.18%	0.017%
46	19.569	2796	2802	2809	rBV	7793506	9992561	100.00%	9.400%
47	21.316	3094	3099	3108	rBV	3899131	4813057	48.17%	4.528%
48	23.539	3469	3477	3484	rBV	5157673	9800256	98.08%	9.219%
49	23.692	3496	3503	3519	rVB	2587143	5336783	53.41%	5.020%




Sum of corrected areas: 106303374

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018529.D
Acq On : 02 Dec 2023 22:50
Operator : MA/JU
Sample : 05411-10
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QH5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

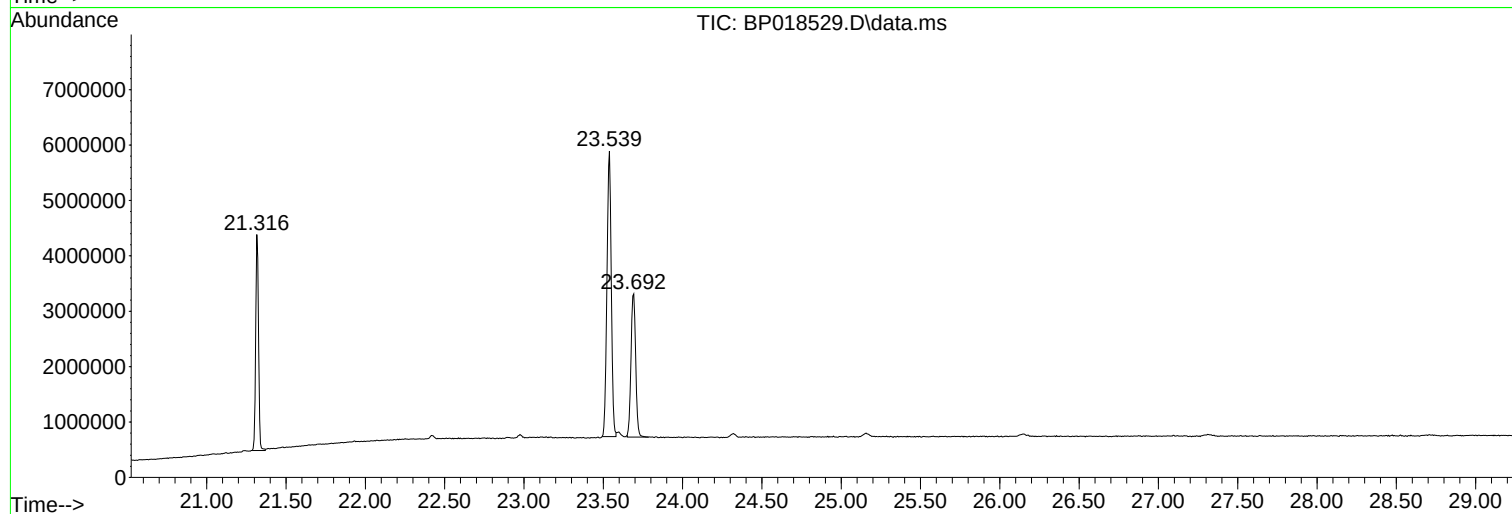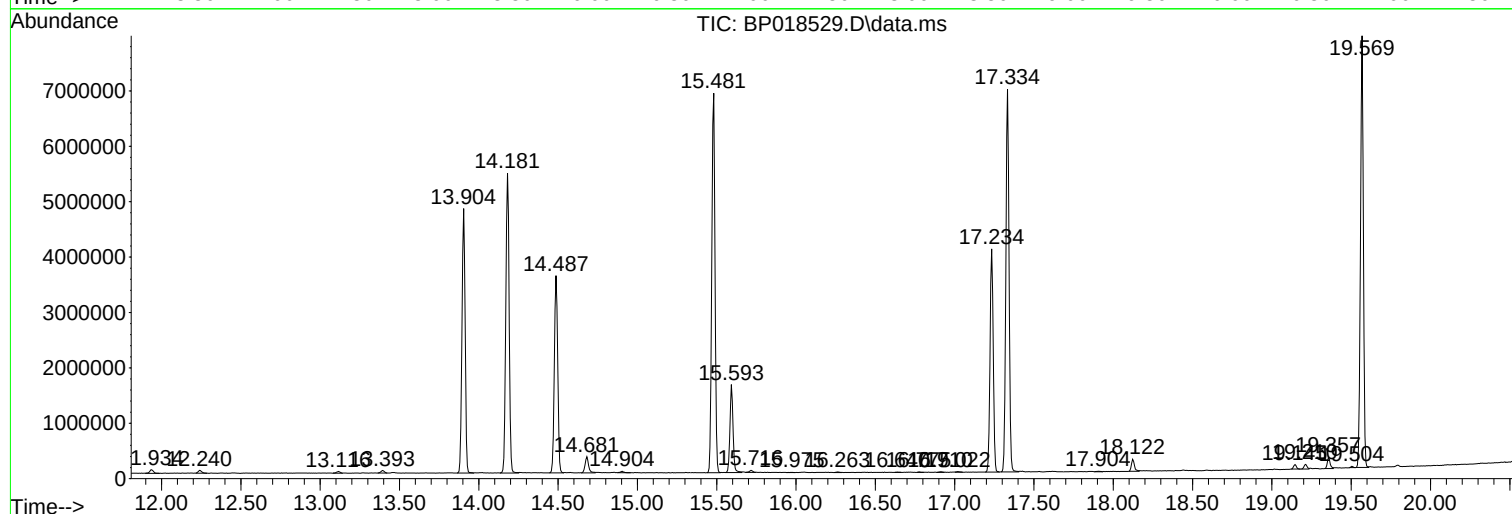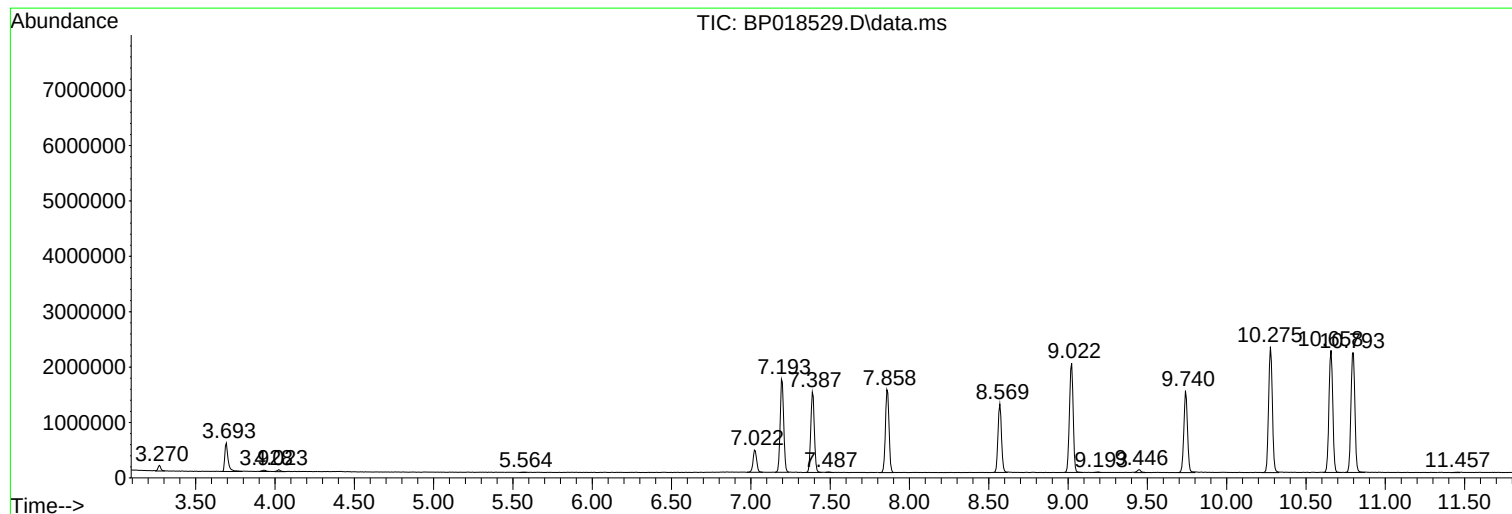

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018529.D
Acq On : 02 Dec 2023 22:50
Operator : MA/JU
Sample : 05411-10
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QH5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018529.D
Acq On : 02 Dec 2023 22:50
Operator : MA/JU
Sample : 05411-10
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QH5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc