

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018530.D
 Acq On : 02 Dec 2023 23:24
 Operator : MA/JU
 Sample : 05411-11
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QH6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018530.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	39	rVB	105458	134966	1.21%	0.130%
2	3.693	99	103	116	rBV	593324	856570	7.69%	0.824%
3	3.928	139	143	149	rVB2	28394	44867	0.40%	0.043%
4	4.022	155	159	163	rBV	34388	42581	0.38%	0.041%
5	4.969	316	320	324	rBV4	8100	11814	0.11%	0.011%
6	7.028	663	670	676	rBV	414129	650177	5.84%	0.625%
7	7.193	691	698	706	rBV	1685130	2661261	23.89%	2.559%
8	7.387	723	731	742	rBV	1510246	2390199	21.46%	2.299%
9	7.487	745	748	753	rVB5	8938	13318	0.12%	0.013%
10	7.858	804	811	819	rBV	1362553	2139075	19.20%	2.057%
11	8.569	925	932	947	rVB	1310568	2013308	18.07%	1.936%
12	9.022	1001	1009	1016	rBV	1927575	3178047	28.53%	3.056%
13	9.187	1031	1037	1040	rBV6	11385	18286	0.16%	0.018%
14	9.740	1122	1131	1146	rBV	1492127	2368827	21.26%	2.278%
15	10.275	1213	1222	1233	rBV	2309123	3761885	33.77%	3.618%
16	10.657	1277	1287	1297	rVB	1993070	3290646	29.54%	3.164%
17	10.799	1303	1311	1320	rBV	1939660	3305595	29.67%	3.179%
18	12.240	1550	1556	1562	rBV2	45146	76627	0.69%	0.074%
19	13.116	1701	1705	1713	rVB2	28000	37604	0.34%	0.036%
20	13.393	1745	1752	1757	rBV4	22828	38474	0.35%	0.037%
21	13.457	1760	1763	1766	rBV4	8827	13247	0.12%	0.013%
22	13.904	1832	1839	1848	rBV	4712233	6377154	57.24%	6.133%
23	14.181	1879	1886	1895	rBV	5193792	7634785	68.53%	7.342%
24	14.487	1930	1938	1948	rBV	3138756	4492067	40.32%	4.320%
25	14.581	1952	1954	1959	rVB2	10243	12724	0.11%	0.012%
26	14.681	1965	1971	1984	rBV	305173	482846	4.33%	0.464%
27	14.845	1995	1999	2002	rBV4	8303	11633	0.10%	0.011%
28	14.910	2004	2010	2015	rVB5	19109	33629	0.30%	0.032%
29	15.481	2099	2107	2119	rBV	6719450	9601442	86.19%	9.233%
30	15.592	2120	2126	2138	rVV	1645688	2150938	19.31%	2.068%
31	15.716	2144	2147	2155	rVB2	33133	49801	0.45%	0.048%
32	16.169	2221	2224	2227	rBV2	8208	12709	0.11%	0.012%
33	16.204	2227	2230	2233	rVB2	12516	14569	0.13%	0.014%
34	16.263	2238	2240	2245	rVV4	14022	12737	0.11%	0.012%
35	16.910	2347	2350	2354	rVB5	11127	15831	0.14%	0.015%
36	17.004	2362	2366	2368	rBV2	13352	18953	0.17%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018530.D
 Acq On : 02 Dec 2023 23:24
 Operator : MA/JU
 Sample : 05411-11
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QH6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	17.233	2398	2405	2412	rBV	3379791	4715123	42.32%	4.534%
38	17.333	2415	2422	2435	rBV	7058636	9747203	87.49%	9.373%
39	17.528	2452	2455	2461	rVB4	9687	18487	0.17%	0.018%
40	17.739	2488	2491	2494	rBV4	9684	13820	0.12%	0.013%
41	17.904	2516	2519	2524	rVB6	12134	20003	0.18%	0.019%
42	18.122	2552	2556	2563	rBV	134922	169898	1.53%	0.163%
43	18.539	2624	2627	2632	rBV7	18130	24599	0.22%	0.024%
44	19.145	2726	2730	2736	rBV4	86431	116709	1.05%	0.112%
45	19.210	2738	2741	2749	rVV	84725	124484	1.12%	0.120%
46	19.357	2762	2766	2773	rBV	130608	164604	1.48%	0.158%
47	19.504	2789	2791	2795	rVB4	22420	23539	0.21%	0.023%
48	19.569	2796	2802	2808	rVV	7865958	10401373	93.37%	10.003%
49	21.316	3094	3099	3105	rBV	3570925	4415034	39.63%	4.246%
50	23.539	3469	3477	3485	rBV2	5831860	11140433	100.00%	10.713%
51	23.692	3496	3503	3514	rVB	2465214	4923024	44.19%	4.734%




Sum of corrected areas: 103987525

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018530.D
Acq On : 02 Dec 2023 23:24
Operator : MA/JU
Sample : 05411-11
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QH6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

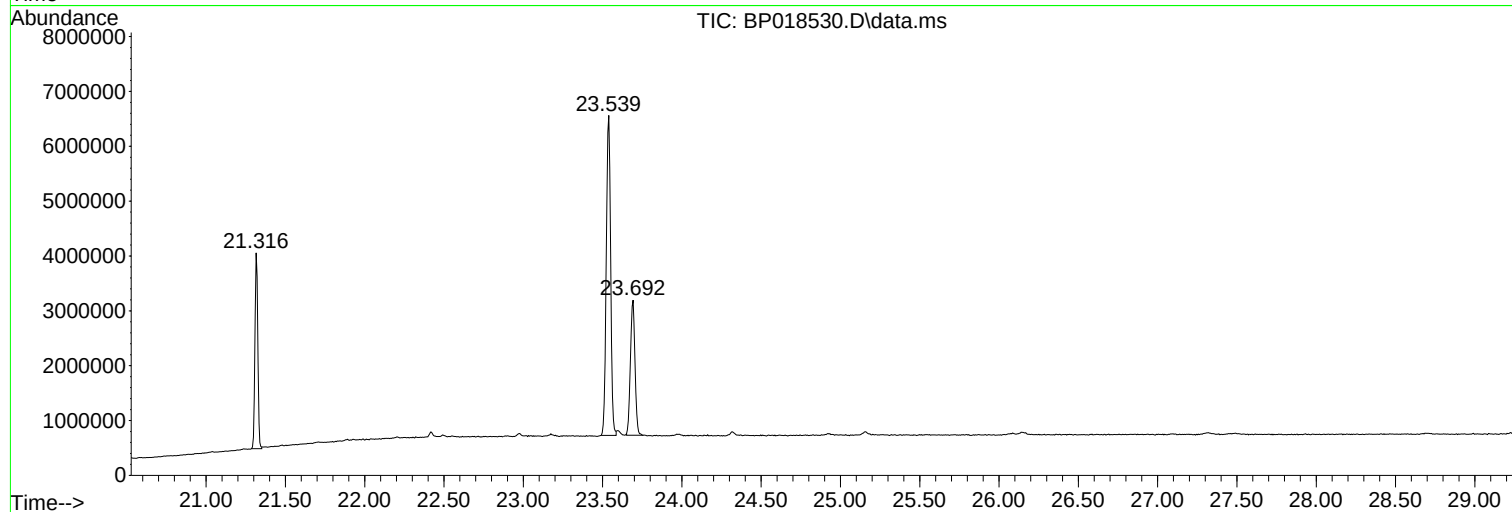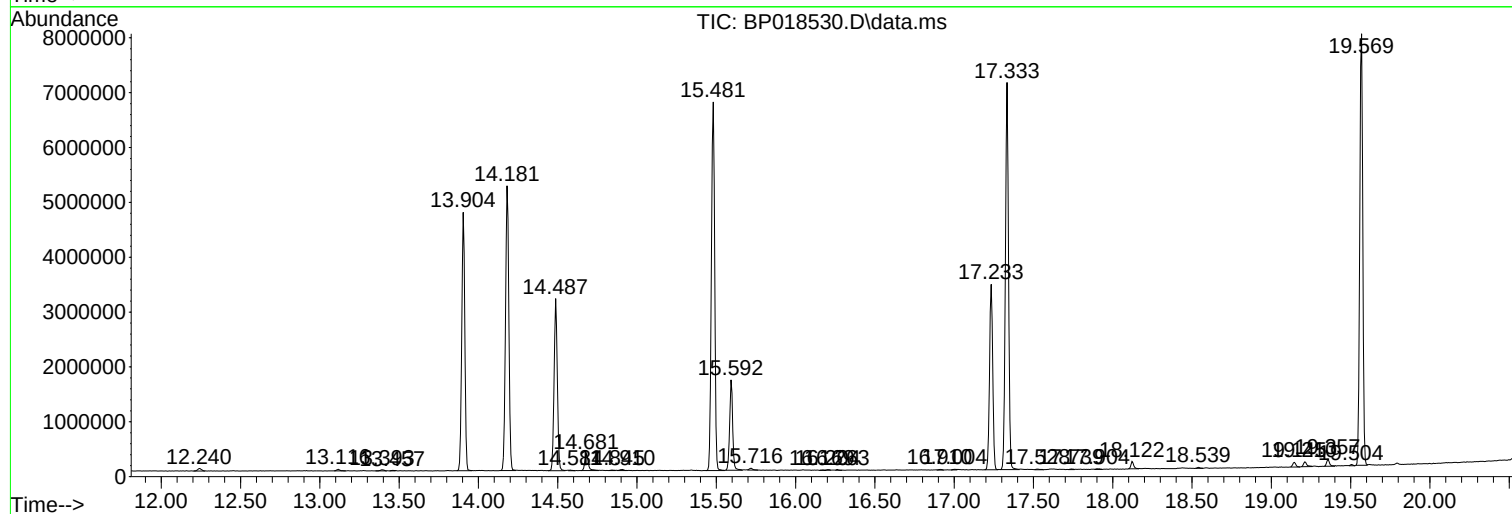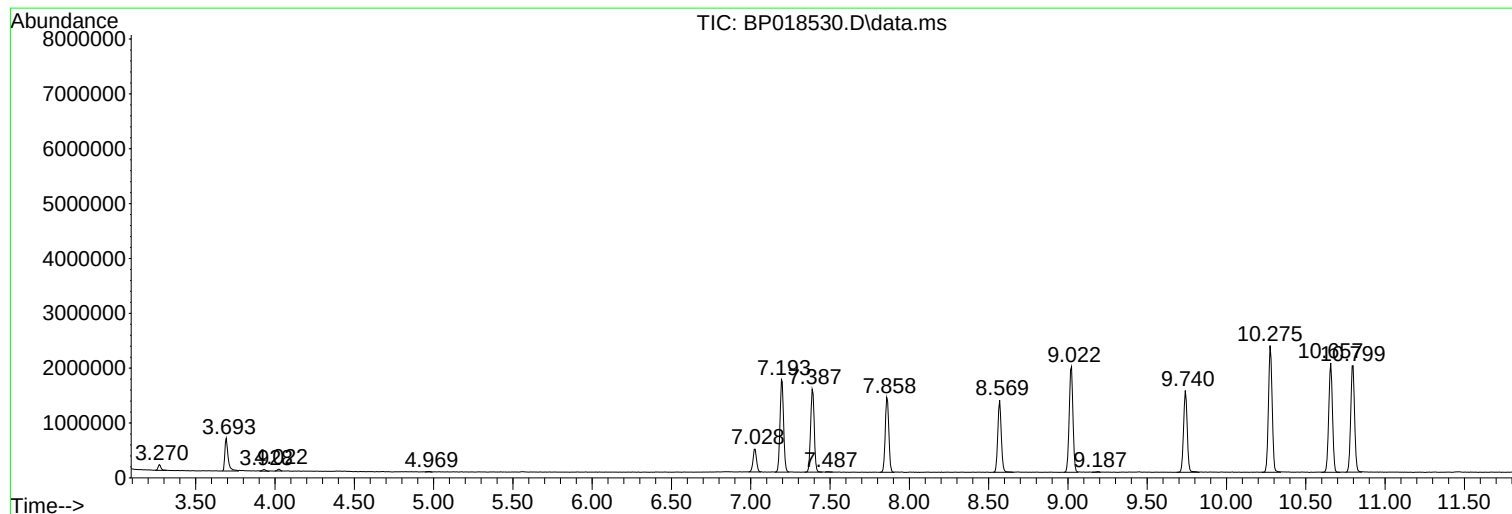

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018530.D
Acq On : 02 Dec 2023 23:24
Operator : MA/JU
Sample : 05411-11
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QH6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018530.D
Acq On : 02 Dec 2023 23:24
Operator : MA/JU
Sample : 05411-11
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QH6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc