

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018531.D
 Acq On : 02 Dec 2023 23:58
 Operator : MA/JU
 Sample : 05411-12
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QH7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018531.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	22	25	28	rBV2	52337	69288	0.63%	0.066%
2	3.270	28	31	40	rVB	99582	128607	1.16%	0.123%
3	3.693	99	103	114	rBV	443673	645121	5.84%	0.618%
4	3.934	138	144	150	rVB	25592	39847	0.36%	0.038%
5	4.023	155	159	166	rVB	47968	70519	0.64%	0.068%
6	6.264	535	540	548	rBV2	17803	34962	0.32%	0.034%
7	7.022	663	669	678	rVB	341989	527548	4.78%	0.505%
8	7.193	691	698	708	rVB	1514748	2311274	20.92%	2.215%
9	7.387	723	731	741	rBV	1324496	2023228	18.32%	1.939%
10	7.858	804	811	821	rBV	1633566	2521860	22.83%	2.416%
11	8.569	925	932	939	rBV	1033237	1588233	14.38%	1.522%
12	9.022	999	1009	1017	rBV	1698451	2786490	25.23%	2.670%
13	9.187	1033	1037	1041	rVB3	12297	16315	0.15%	0.016%
14	9.440	1077	1080	1086	rVB4	6985	13857	0.13%	0.013%
15	9.740	1123	1131	1141	rBV	1269658	2038450	18.45%	1.953%
16	10.275	1211	1222	1233	rBV	2020440	3292943	29.81%	3.155%
17	10.658	1279	1287	1296	rVB	2406064	3996235	36.18%	3.829%
18	10.793	1303	1310	1320	rBV	1491975	2474501	22.40%	2.371%
19	12.240	1550	1556	1563	rVV2	41632	71295	0.65%	0.068%
20	13.116	1701	1705	1710	rVB	24830	36310	0.33%	0.035%
21	13.393	1747	1752	1758	rVB3	30310	51434	0.47%	0.049%
22	13.457	1758	1763	1767	rBV4	8249	15794	0.14%	0.015%
23	13.904	1832	1839	1845	rBV	4645020	6310396	57.13%	6.047%
24	14.181	1875	1886	1901	rBV	5007604	7229501	65.45%	6.927%
25	14.487	1930	1938	1949	rBV	4016258	5873701	53.18%	5.628%
26	14.569	1949	1952	1958	rVB3	7729	15201	0.14%	0.015%
27	14.681	1965	1971	1981	rBV	324135	487307	4.41%	0.467%
28	14.904	2005	2009	2015	rVB6	21589	34819	0.32%	0.033%
29	15.146	2044	2050	2052	rBV4	11881	14589	0.13%	0.014%
30	15.481	2099	2107	2114	rBV	6879197	9464526	85.69%	9.069%
31	15.593	2119	2126	2139	rBV	1796618	2434755	22.04%	2.333%
32	15.716	2143	2147	2154	rVB3	31344	57246	0.52%	0.055%
33	16.263	2236	2240	2247	rVB5	12876	20722	0.19%	0.020%
34	16.916	2346	2351	2353	rBV4	11522	17590	0.16%	0.017%
35	17.016	2362	2368	2373	rBV3	12629	29372	0.27%	0.028%
36	17.234	2398	2405	2412	rBV	4748408	6740700	61.03%	6.459%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018531.D
 Acq On : 02 Dec 2023 23:58
 Operator : MA/JU
 Sample : 05411-12
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QH7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	17.334	2416	2422	2431	rVV	7324032	10143872	91.84%	9.720%
38	18.122	2552	2556	2565	rBV2	196968	272157	2.46%	0.261%
39	18.439	2607	2610	2615	rBV5	15483	25151	0.23%	0.024%
40	18.592	2632	2636	2639	rBV5	13791	19203	0.17%	0.018%
41	19.145	2726	2730	2735	rVB2	92850	118025	1.07%	0.113%
42	19.210	2737	2741	2745	rBV	98378	137842	1.25%	0.132%
43	19.357	2762	2766	2771	rBV2	174282	211937	1.92%	0.203%
44	19.504	2789	2791	2795	rVB4	30385	30559	0.28%	0.029%
45	19.569	2796	2802	2808	rBV	8446928	11045656	100.00%	10.584%
46	21.316	3094	3099	3106	rBV	4267787	5266473	47.68%	5.046%
47	23.539	3470	3477	3484	rBV2	4505348	8451706	76.52%	8.098%
48	23.692	3496	3503	3515	rVB	2535039	5156020	46.68%	4.940%




Sum of corrected areas: 104363137

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018531.D
Acq On : 02 Dec 2023 23:58
Operator : MA/JU
Sample : 05411-12
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QH7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

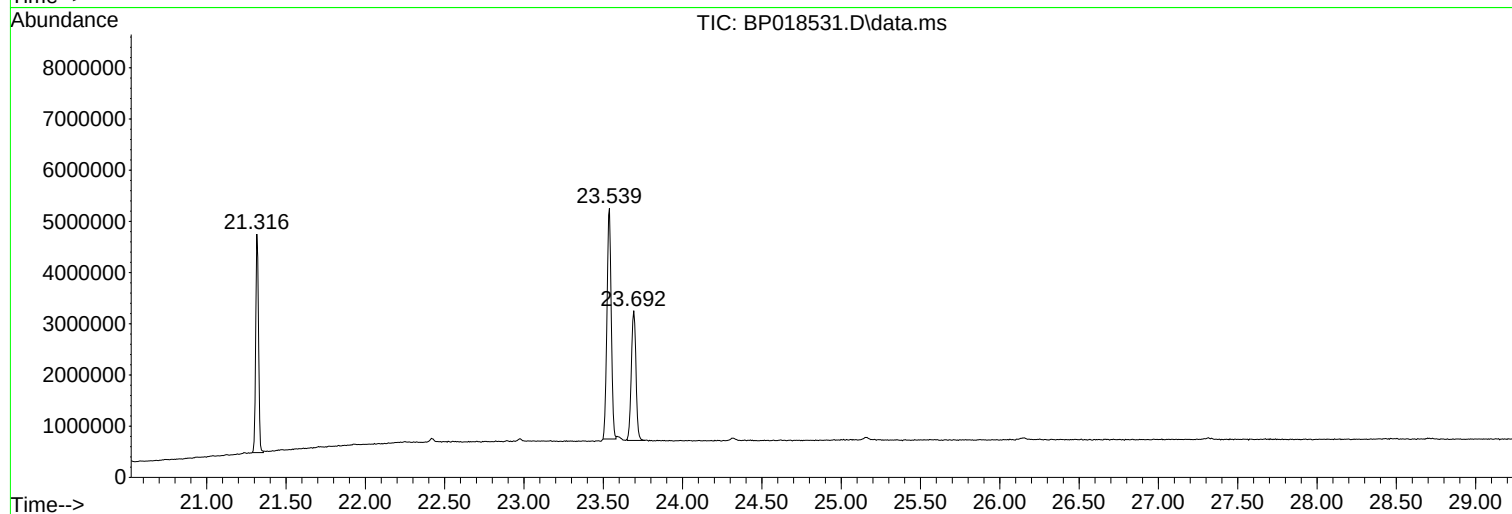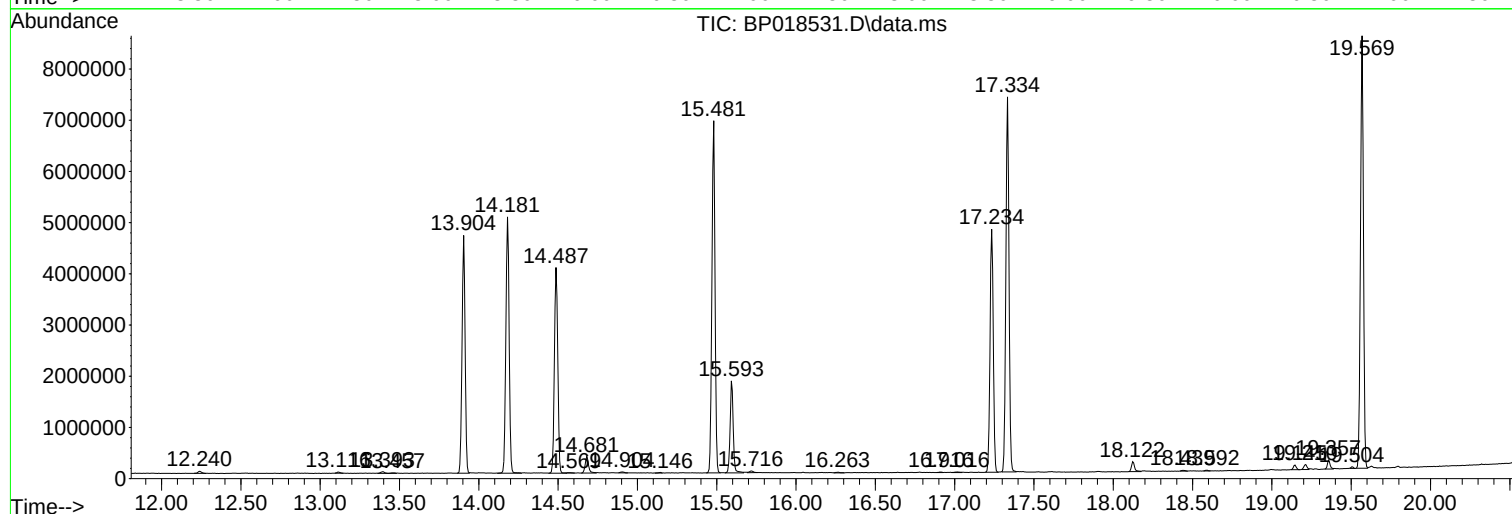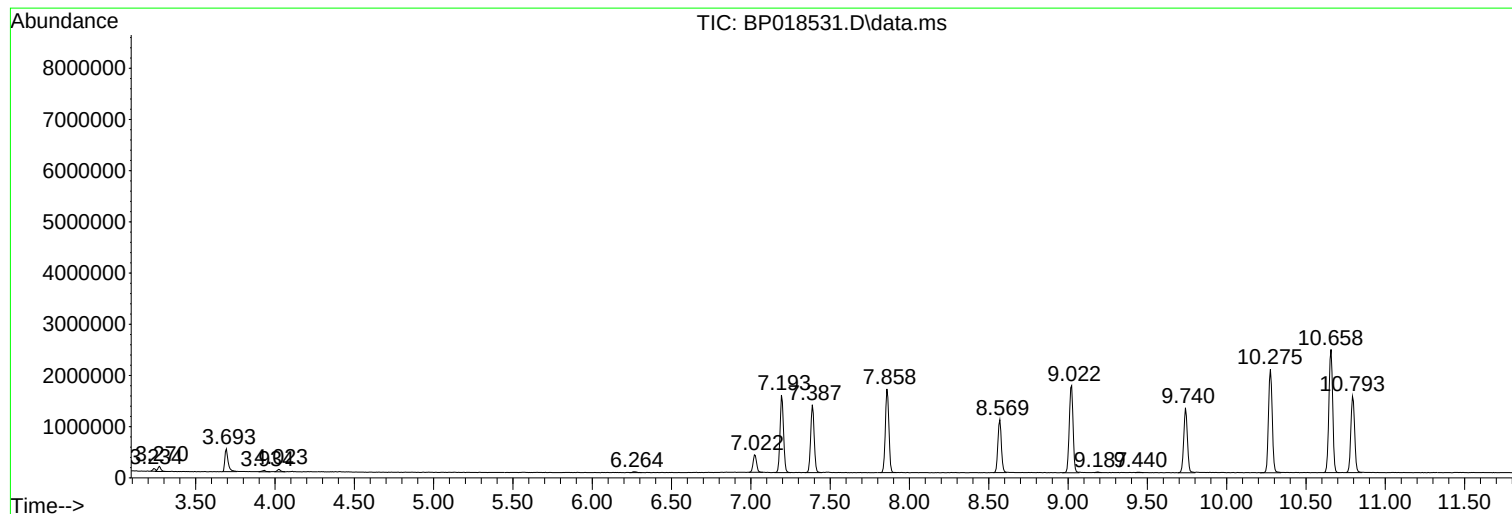

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018531.D
Acq On : 02 Dec 2023 23:58
Operator : MA/JU
Sample : 05411-12
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QH7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018531.D
Acq On : 02 Dec 2023 23:58
Operator : MA/JU
Sample : 05411-12
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QH7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
