

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018533.D
 Acq On : 03 Dec 2023 01:06
 Operator : MA/JU
 Sample : 05411-14
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QJ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018533.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	36	rBV	97555	113197	1.24%	0.122%
2	3.693	99	103	117	rBV	523096	772447	8.49%	0.831%
3	3.928	139	143	149	rVB2	25383	41687	0.46%	0.045%
4	4.022	155	159	165	rVB2	30787	45662	0.50%	0.049%
5	4.969	313	320	325	rBV4	13380	22338	0.25%	0.024%
6	7.028	664	670	679	rVB	362600	566886	6.23%	0.610%
7	7.193	692	698	707	rBV	1459744	2254892	24.79%	2.425%
8	7.322	715	720	722	rBV3	7594	11716	0.13%	0.013%
9	7.387	724	731	738	rBV	1302414	2023251	22.24%	2.176%
10	7.487	743	748	752	rVB6	8575	15812	0.17%	0.017%
11	7.858	804	811	820	rBV	1458171	2260584	24.85%	2.431%
12	8.569	923	932	943	rBV	1113272	1739173	19.12%	1.871%
13	9.022	999	1009	1018	rBV	1622777	2670642	29.36%	2.873%
14	9.181	1033	1036	1041	rVB3	14051	19552	0.21%	0.021%
15	9.740	1124	1131	1142	rBV	1194068	1883719	20.71%	2.026%
16	10.275	1215	1222	1234	rBV	1986187	3228589	35.49%	3.473%
17	10.451	1249	1252	1258	rVB5	9876	14670	0.16%	0.016%
18	10.657	1280	1287	1296	rVB	2093213	3450899	37.93%	3.712%
19	10.793	1303	1310	1321	rBV	1516840	2488515	27.35%	2.677%
20	11.310	1395	1398	1403	rVB3	5254	9810	0.11%	0.011%
21	11.393	1408	1412	1416	rBV4	6973	11255	0.12%	0.012%
22	12.181	1540	1546	1552	rBV	245050	384801	4.23%	0.414%
23	12.240	1552	1556	1562	rVB	43466	69387	0.76%	0.075%
24	13.116	1697	1705	1712	rBV2	26342	46242	0.51%	0.050%
25	13.393	1747	1752	1757	rVB3	20599	36106	0.40%	0.039%
26	13.904	1831	1839	1845	rBV	4144538	5647116	62.07%	6.074%
27	14.181	1878	1886	1895	rBV	4588861	6632044	72.90%	7.133%
28	14.487	1930	1938	1948	rBV	3380392	4950426	54.42%	5.325%
29	14.681	1966	1971	1983	rBV	238189	378976	4.17%	0.408%
30	14.904	2005	2009	2014	rBV7	16704	26061	0.29%	0.028%
31	15.234	2059	2065	2070	rBV4	7122	13368	0.15%	0.014%
32	15.481	2099	2107	2114	rBV	5886484	8530273	93.77%	9.175%
33	15.592	2120	2126	2138	rBV	1388168	1864439	20.49%	2.005%
34	15.716	2144	2147	2153	rVB3	26804	43654	0.48%	0.047%
35	15.963	2186	2189	2193	rVB	7450	10877	0.12%	0.012%
36	16.422	2264	2267	2270	rBV2	10265	10814	0.12%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018533.D
 Acq On : 03 Dec 2023 01:06
 Operator : MA/JU
 Sample : 05411-14
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QJ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	16.910	2346	2350	2354	rVB3	8365	16117	0.18%	0.017%
38	17.022	2365	2369	2372	rBV3	9444	15160	0.17%	0.016%
39	17.233	2398	2405	2412	rBV	3963220	5476988	60.20%	5.891%
40	17.333	2415	2422	2432	rVV	6287263	8938382	98.25%	9.614%
41	17.428	2436	2438	2443	rVB4	17448	23167	0.25%	0.025%
42	17.904	2517	2519	2523	rVB4	8876	9284	0.10%	0.010%
43	18.122	2552	2556	2561	rBV2	113390	146040	1.61%	0.157%
44	19.145	2726	2730	2736	rBV2	68041	92086	1.01%	0.099%
45	19.210	2737	2741	2746	rBV	76110	111023	1.22%	0.119%
46	19.357	2762	2766	2771	rBV3	104200	121426	1.33%	0.131%
47	19.504	2789	2791	2795	rVB4	20573	14846	0.16%	0.016%
48	19.569	2796	2802	2808	rBV	6910551	9097457	100.00%	9.785%
49	19.792	2837	2840	2844	rVB	45978	54155	0.60%	0.058%
50	21.316	3094	3099	3108	rBV	3453210	4300888	47.28%	4.626%
51	23.533	3469	3476	3484	rBV2	4127730	7721561	84.88%	8.305%
52	23.692	3496	3503	3516	rVB	2348153	4542433	49.93%	4.886%


Sum of corrected areas: 92970893

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018533.D
Acq On : 03 Dec 2023 01:06
Operator : MA/JU
Sample : 05411-14
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QJ3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

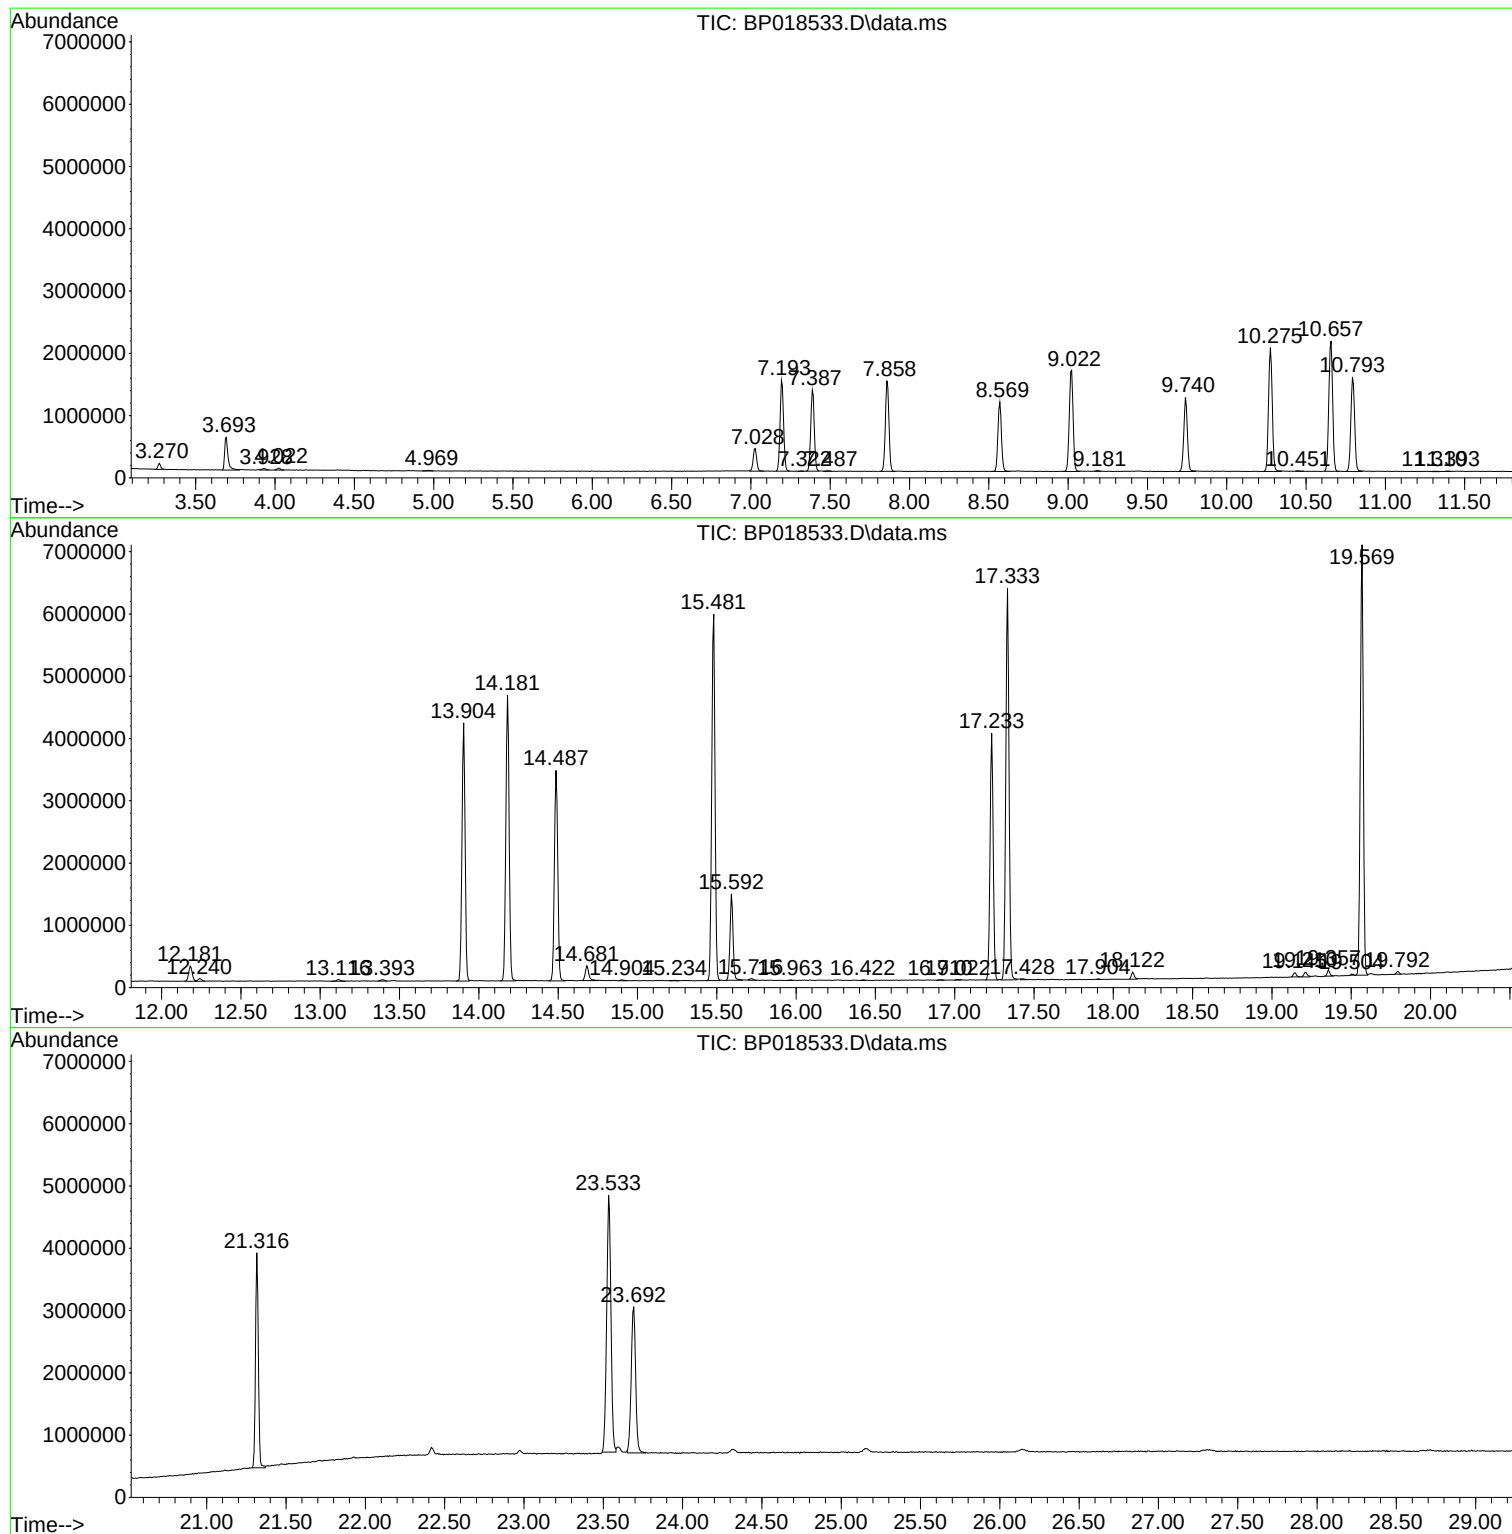

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018533.D
Acq On : 03 Dec 2023 01:06
Operator : MA/JU
Sample : 05411-14
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QJ3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.181	2.23 ng/ul	384801	Naphthalene-d8	10.657

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	6-Isopropylquinoline			171	C12H13N	000135-79-5	38
2	Chloroxyleneol			156	C8H9ClO	000088-04-0	32
3	Benzene, 2,5-cyclohexadien-1-yl-			156	C12H12	004794-05-2	28
4	Tebuthiuron			228	C9H16N4O5	034014-18-1	25
5	4-Chloro-3,5-dimethylphenol, O-i...			242	C12H15ClO3	1000487-39-3	23

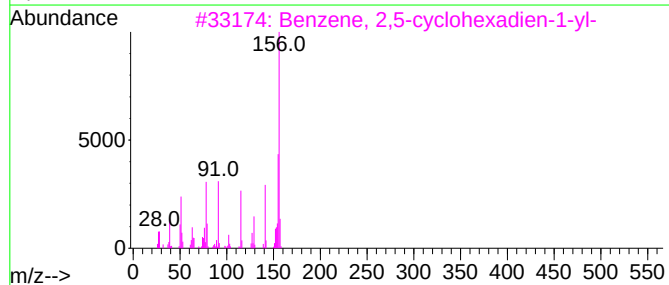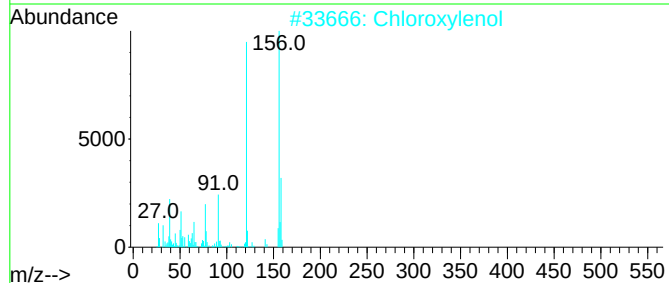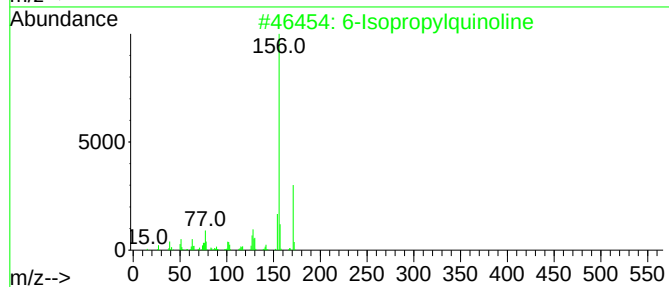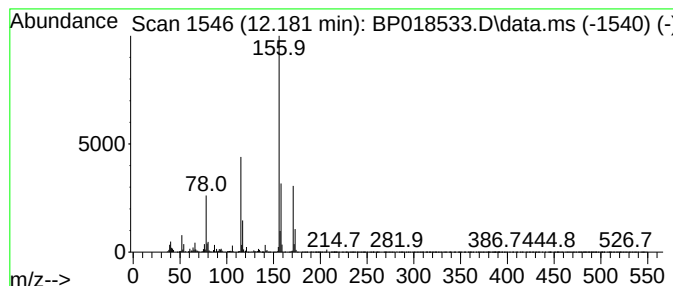

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018533.D
Acq On : 03 Dec 2023 01:06
Operator : MA/JU
Sample : 05411-14
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QJ3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	12.181	2.2	ng/u1	384801	2	10.657	3450900	20.0