

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018534.D
 Acq On : 03 Dec 2023 01:40
 Operator : MA/JU
 Sample : 05411-15
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QK0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018534.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	28	31	39	rVB	74670	94117	0.93%	0.110%
2	3.693	99	103	113	rBV	340487	485551	4.80%	0.566%
3	3.934	140	144	149	rVB	20699	29161	0.29%	0.034%
4	4.022	155	159	165	rBV2	25656	38400	0.38%	0.045%
5	7.022	663	669	678	rVB	305656	475403	4.70%	0.554%
6	7.193	692	698	708	rVB	1292141	2035626	20.13%	2.374%
7	7.387	723	731	742	rBV	1182243	1832752	18.13%	2.137%
8	7.487	742	748	752	rVB3	8975	15990	0.16%	0.019%
9	7.858	804	811	820	rVB	1378227	2159408	21.36%	2.518%
10	8.569	925	932	940	rBV	888526	1380033	13.65%	1.610%
11	9.022	1001	1009	1019	rBV	1414061	2323703	22.98%	2.710%
12	9.187	1032	1037	1041	rBV3	14674	24983	0.25%	0.029%
13	9.740	1123	1131	1142	rBV	999355	1594047	15.76%	1.859%
14	10.275	1214	1222	1233	rBV	1622625	2640028	26.11%	3.079%
15	10.657	1278	1287	1294	rBV	1838249	3063689	30.30%	3.573%
16	10.793	1304	1310	1318	rBV	1412143	2297582	22.72%	2.680%
17	12.181	1540	1546	1551	rBV2	27801	42557	0.42%	0.050%
18	12.240	1551	1556	1561	rVB	33607	50163	0.50%	0.059%
19	13.116	1701	1705	1708	rVB2	19156	23230	0.23%	0.027%
20	13.393	1747	1752	1756	rBV2	29808	45236	0.45%	0.053%
21	13.463	1758	1764	1768	rVV5	8394	12613	0.12%	0.015%
22	13.904	1832	1839	1846	rBV	3145560	4267152	42.20%	4.977%
23	14.181	1879	1886	1898	rBV	3616091	5132928	50.76%	5.986%
24	14.487	1931	1938	1950	rVB	2788320	3960250	39.16%	4.619%
25	14.681	1966	1971	1978	rBV2	217726	327130	3.24%	0.382%
26	14.904	2004	2009	2015	rVB7	17858	31592	0.31%	0.037%
27	15.481	2100	2107	2115	rBV	4630756	6760960	66.86%	7.885%
28	15.592	2120	2126	2135	rBV	1139058	1511218	14.95%	1.763%
29	15.716	2141	2147	2152	rBV2	20162	37033	0.37%	0.043%
30	16.257	2235	2239	2243	rBV3	9661	13086	0.13%	0.015%
31	17.016	2364	2368	2372	rBV3	9555	14994	0.15%	0.017%
32	17.234	2398	2405	2413	rBV	3284117	4536062	44.86%	5.290%
33	17.334	2415	2422	2434	rBV	5347013	7479304	73.97%	8.723%
34	17.610	2463	2469	2472	rBV4	15826	28257	0.28%	0.033%
35	18.122	2552	2556	2563	rBV2	175476	224471	2.22%	0.262%
36	19.145	2725	2730	2736	rBV4	72809	108915	1.08%	0.127%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018534.D
Acq On : 03 Dec 2023 01:40
Operator : MA/JU
Sample : 05411-15
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QK0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	19.210	2737	2741	2745	rBV	74889	110408	1.09%	0.129%
38	19.357	2762	2766	2772	rBV2	175555	218581	2.16%	0.255%
39	19.569	2796	2802	2808	rBV	6826645	9081599	89.81%	10.592%
40	19.792	2837	2840	2845	rBV2	34905	39968	0.40%	0.047%
41	21.316	3094	3099	3105	rBV	4246190	5251867	51.94%	6.125%
42	23.539	3469	3477	3484	rBV2	5212632	10111725	100.00%	11.793%
43	23.692	3496	3503	3516	rVB	3093879	5831037	57.67%	6.801%




Sum of corrected areas: 85742809

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018534.D
Acq On : 03 Dec 2023 01:40
Operator : MA/JU
Sample : 05411-15
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QK0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

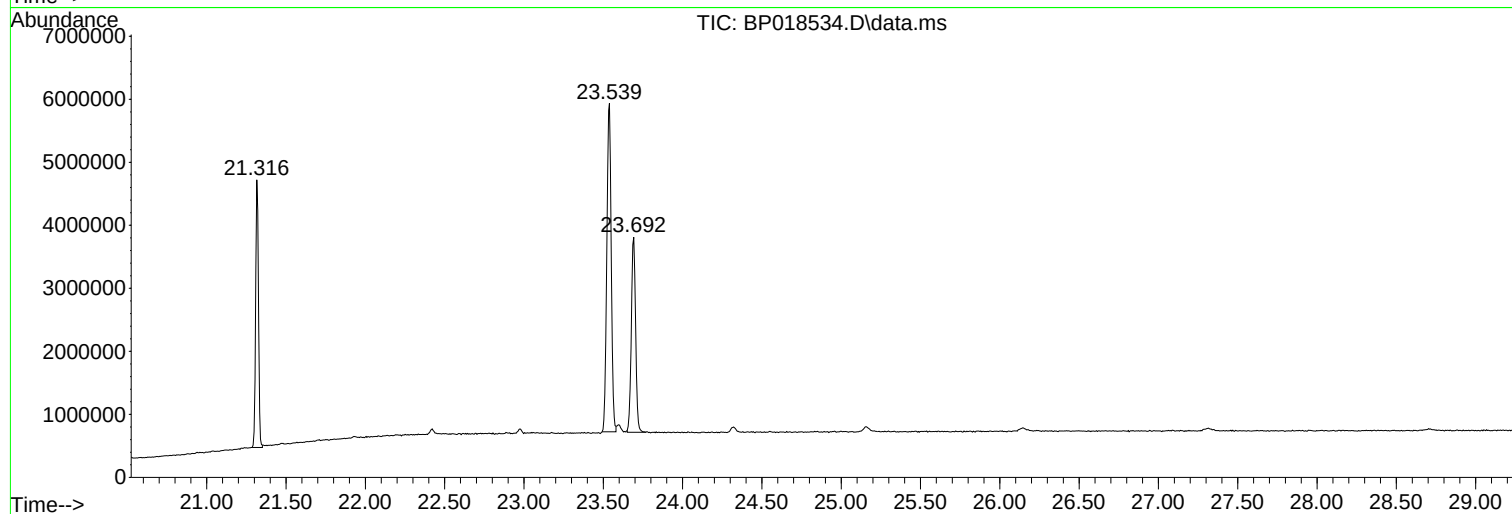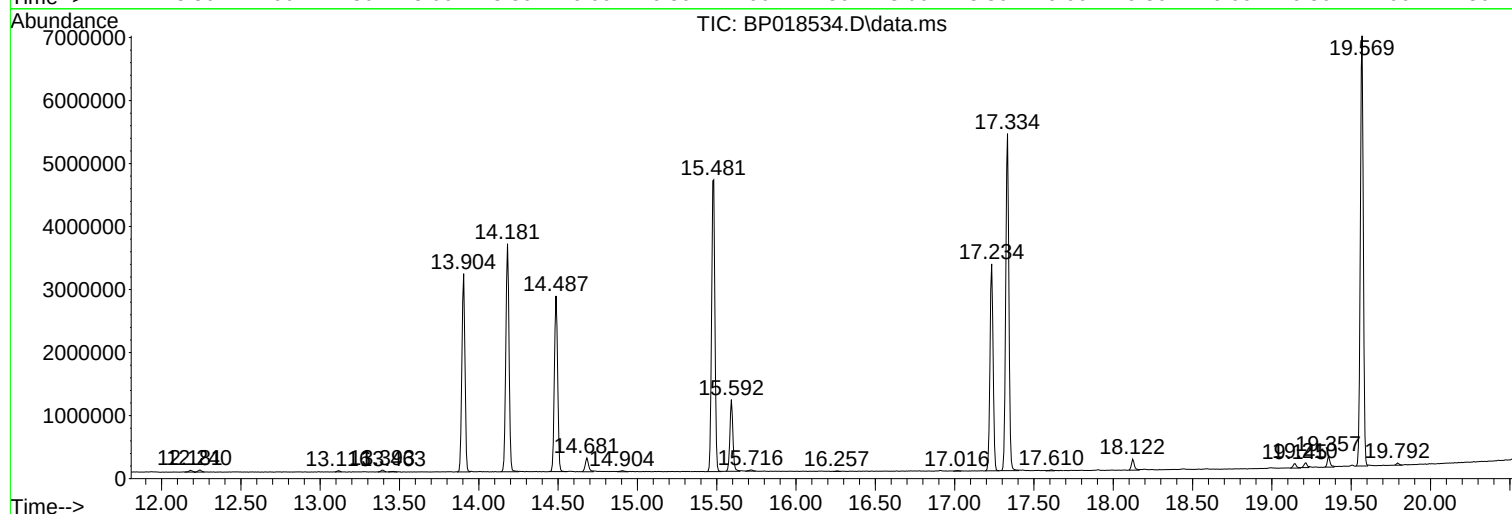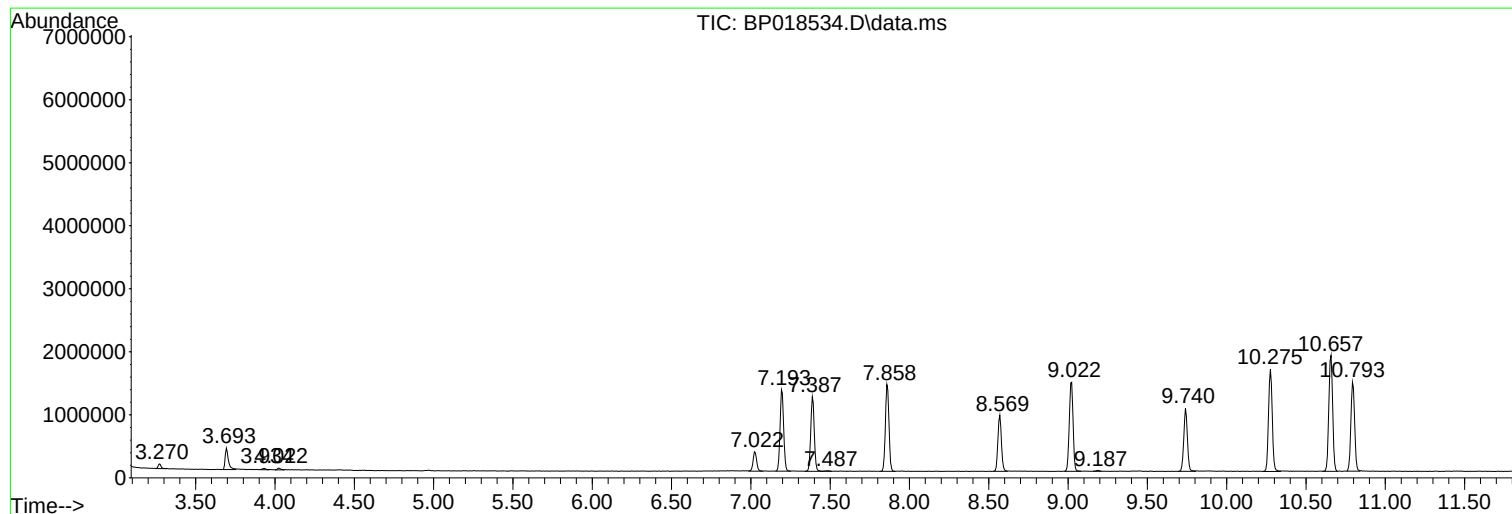

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018534.D
Acq On : 03 Dec 2023 01:40
Operator : MA/JU
Sample : 05411-15
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QK0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018534.D
Acq On : 03 Dec 2023 01:40
Operator : MA/JU
Sample : 05411-15
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QK0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
