

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018538.D
 Acq On : 03 Dec 2023 04:30
 Operator : MA/JU
 Sample : 05411-16
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QK1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018538.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	28	31	37	rVB	101267	116683	1.17%	0.128%
2	3.693	99	103	113	rBV	557040	781023	7.80%	0.859%
3	3.928	139	143	147	rVB2	24233	35288	0.35%	0.039%
4	4.022	155	159	164	rVB	27693	38631	0.39%	0.042%
5	4.469	233	235	241	rVB4	10298	11710	0.12%	0.013%
6	7.022	662	669	677	rVB	340541	529779	5.29%	0.582%
7	7.193	690	698	708	rVB	1445457	2232279	22.29%	2.454%
8	7.387	724	731	741	rBV	1289334	2000729	19.98%	2.200%
9	7.487	743	748	752	rVV6	10959	17498	0.17%	0.019%
10	7.857	803	811	820	rBV	1504043	2361332	23.58%	2.596%
11	8.569	926	932	940	rBV	1016883	1569558	15.68%	1.726%
12	9.022	1000	1009	1020	rBV	1536532	2567124	25.64%	2.822%
13	9.193	1033	1038	1042	rVB4	8974	14575	0.15%	0.016%
14	9.445	1076	1081	1087	rVB	60596	93879	0.94%	0.103%
15	9.740	1122	1131	1141	rBV	1106945	1786117	17.84%	1.964%
16	9.816	1141	1144	1148	rVB	8223	11762	0.12%	0.013%
17	10.275	1214	1222	1231	rBV	1773111	2912366	29.09%	3.202%
18	10.657	1279	1287	1295	rBV	2001997	3333180	33.29%	3.665%
19	10.792	1301	1310	1321	rBV	1719604	2919956	29.16%	3.210%
20	11.934	1499	1504	1511	rVB	96648	148451	1.48%	0.163%
21	12.239	1551	1556	1564	rVB2	34868	60133	0.60%	0.066%
22	12.445	1587	1591	1597	rVB4	6413	12686	0.13%	0.014%
23	13.116	1699	1705	1710	rBV2	20258	34318	0.34%	0.038%
24	13.392	1747	1752	1758	rBV	39484	59978	0.60%	0.066%
25	13.904	1832	1839	1850	rVB	3380269	4655699	46.50%	5.119%
26	14.181	1879	1886	1897	rBV	3953496	5662811	56.56%	6.226%
27	14.486	1931	1938	1947	rBV	2918158	4277207	42.72%	4.702%
28	14.681	1966	1971	1982	rBV2	232419	352939	3.52%	0.388%
29	14.857	1996	2001	2004	rVB4	7921	12679	0.13%	0.014%
30	14.904	2004	2009	2012	rBV5	14082	25902	0.26%	0.028%
31	15.480	2099	2107	2117	rBV	4892274	7168198	71.59%	7.881%
32	15.592	2120	2126	2140	rVV	1104814	1524441	15.22%	1.676%
33	15.716	2142	2147	2152	rVB4	25299	41810	0.42%	0.046%
34	16.157	2218	2222	2227	rBV5	6936	14566	0.15%	0.016%
35	16.727	2314	2319	2321	rBV2	8138	12136	0.12%	0.013%
36	17.022	2367	2369	2373	rVB2	8709	12189	0.12%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018538.D
 Acq On : 03 Dec 2023 04:30
 Operator : MA/JU
 Sample : 05411-16
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QK1

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	17.233	2398	2405	2415	rBV	3576997	4881614	48.75%	5.367%
38	17.333	2415	2422	2432	rBV	5407503	7516797	75.07%	8.264%
39	18.122	2552	2556	2561	rBV2	76833	97424	0.97%	0.107%
40	19.145	2726	2730	2736	rBV3	64918	87379	0.87%	0.096%
41	19.210	2737	2741	2745	rBV	75626	103869	1.04%	0.114%
42	19.357	2763	2766	2772	rVB4	70382	77330	0.77%	0.085%
43	19.568	2796	2802	2808	rBV	6897954	8986898	89.75%	9.880%
44	19.792	2837	2840	2846	rBV	50278	55237	0.55%	0.061%
45	21.315	3094	3099	3105	rBV	4514007	5532663	55.26%	6.083%
46	23.539	3469	3477	3484	rBV2	5197923	10012867	100.00%	11.008%
47	23.686	3496	3502	3515	rVB	3052084	6195752	61.88%	6.812%




Sum of corrected areas: 90957442

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018538.D
Acq On : 03 Dec 2023 04:30
Operator : MA/JU
Sample : 05411-16
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QK1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

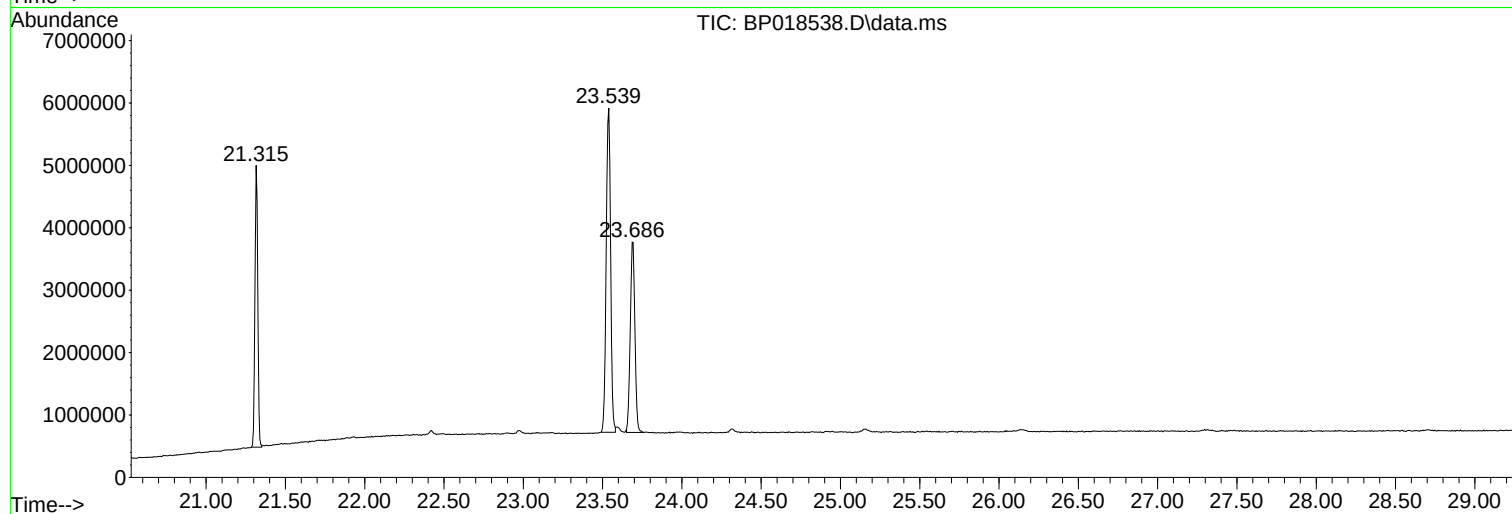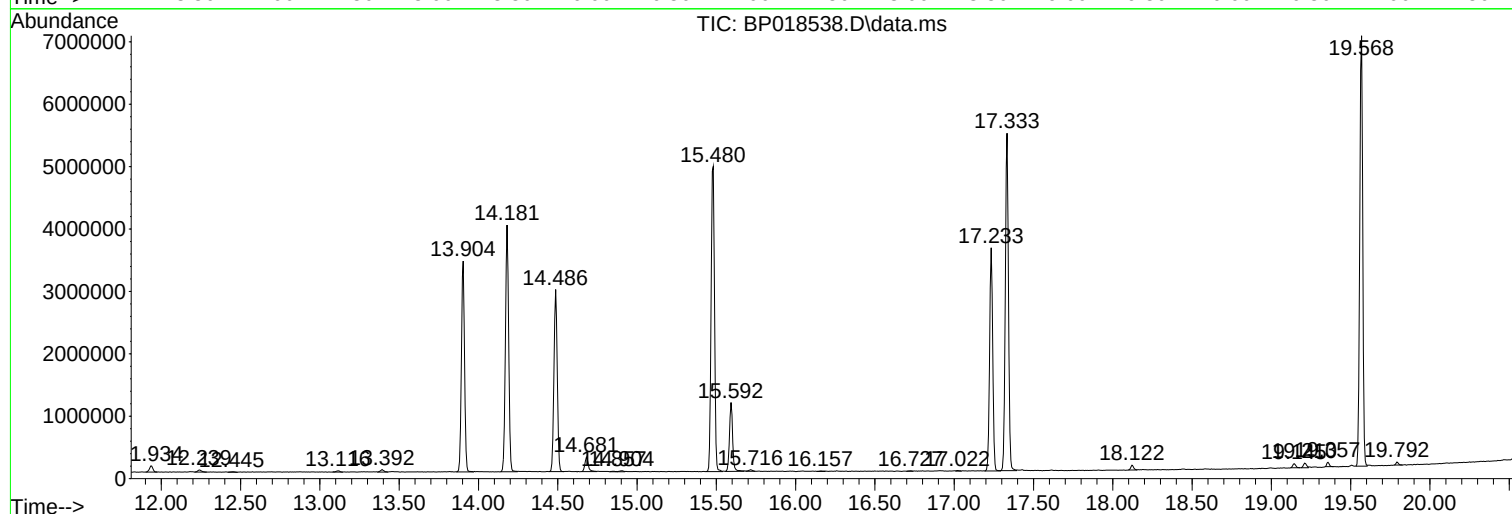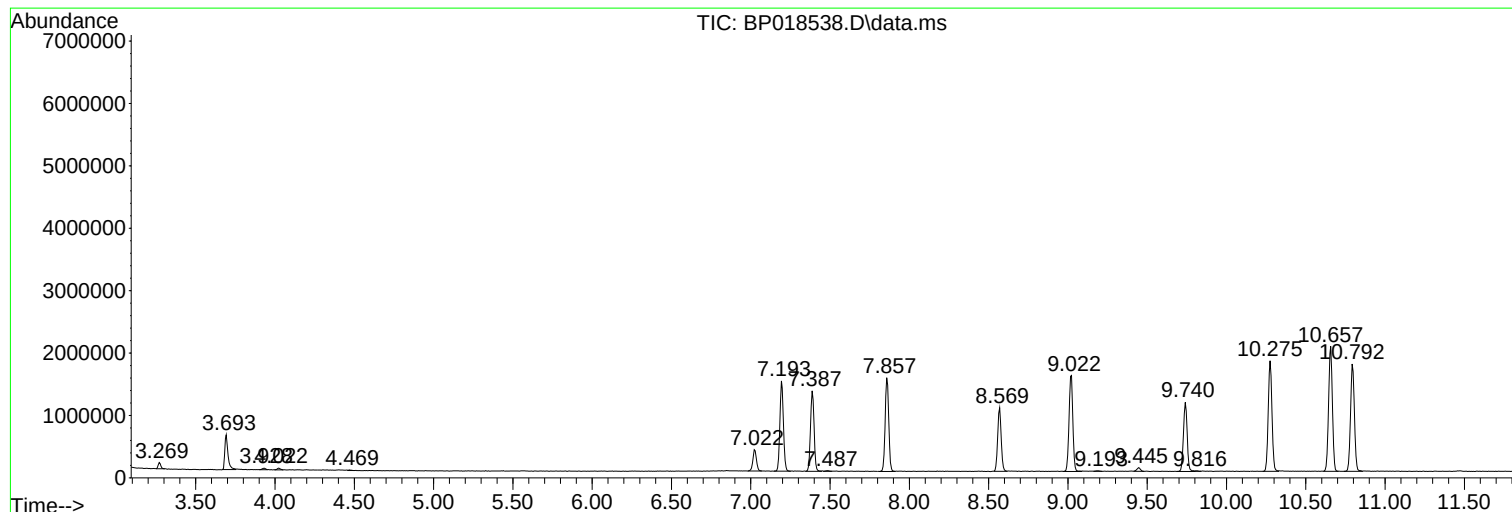

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018538.D
Acq On : 03 Dec 2023 04:30
Operator : MA/JU
Sample : 05411-16
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QK1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018538.D
Acq On : 03 Dec 2023 04:30
Operator : MA/JU
Sample : 05411-16
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QK1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------