

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018540.D
 Acq On : 03 Dec 2023 05:38
 Operator : MA/JU
 Sample : 05411-18
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QL6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018540.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	38	rVB	112930	137105	1.23%	0.144%
2	3.622	86	91	95	rBV2	52078	67640	0.61%	0.071%
3	3.693	99	103	118	rVV	624668	907597	8.17%	0.956%
4	3.928	139	143	147	rVB	29412	42860	0.39%	0.045%
5	4.022	154	159	165	rVB2	33070	49487	0.45%	0.052%
6	7.022	663	669	676	rBV	359303	562669	5.07%	0.593%
7	7.192	692	698	708	rVB	1442528	2277234	20.51%	2.399%
8	7.387	724	731	741	rBV	1299520	2024307	18.23%	2.132%
9	7.481	745	747	752	rVB3	10521	12067	0.11%	0.013%
10	7.857	803	811	818	rBV	1434418	2224236	20.03%	2.343%
11	7.928	818	823	831	rVB	79113	124370	1.12%	0.131%
12	8.569	923	932	943	rBV	1081538	1674760	15.08%	1.764%
13	8.963	995	999	1001	rBV2	8740	13277	0.12%	0.014%
14	9.016	1001	1008	1022	rVV	1627346	2645873	23.83%	2.787%
15	9.128	1024	1027	1033	rVV2	11771	22412	0.20%	0.024%
16	9.186	1033	1037	1045	rVB6	10644	18527	0.17%	0.020%
17	9.451	1076	1082	1085	rVV4	7213	14424	0.13%	0.015%
18	9.739	1122	1131	1137	rBV	987134	1578668	14.22%	1.663%
19	9.786	1137	1139	1145	rVB2	56600	80033	0.72%	0.084%
20	10.275	1214	1222	1231	rBV	1872216	3025756	27.25%	3.187%
21	10.657	1278	1287	1295	rBV	1939898	3261554	29.37%	3.436%
22	10.710	1295	1296	1302	rVB5	13164	17530	0.16%	0.018%
23	10.792	1302	1310	1321	rBV	1906668	3250485	29.27%	3.424%
24	11.457	1418	1423	1429	rBV4	7241	18233	0.16%	0.019%
25	11.939	1500	1505	1509	rBV3	11547	20725	0.19%	0.022%
26	12.239	1551	1556	1563	rVB2	40249	69759	0.63%	0.073%
27	12.445	1589	1591	1595	rBV	8950	14156	0.13%	0.015%
28	13.110	1698	1704	1709	rVB4	19282	36321	0.33%	0.038%
29	13.398	1745	1753	1760	rBV3	32036	59523	0.54%	0.063%
30	13.904	1828	1839	1848	rBV	3744811	5147996	46.36%	5.423%
31	14.180	1877	1886	1894	rBV	4216437	6154791	55.42%	6.483%
32	14.486	1930	1938	1948	rBV	2947572	4279621	38.54%	4.508%
33	14.616	1955	1960	1963	rBV2	18796	19363	0.17%	0.020%
34	14.680	1965	1971	1983	rBV	222695	354252	3.19%	0.373%
35	14.904	2004	2009	2014	rVB4	19329	30778	0.28%	0.032%
36	15.480	2100	2107	2114	rBV	5323260	7810927	70.34%	8.228%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018540.D
 Acq On : 03 Dec 2023 05:38
 Operator : MA/JU
 Sample : 05411-18
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QL6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	15.592	2120	2126	2137	rBV	884020	1196604	10.78%	1.260%
38	15.716	2143	2147	2153	rVB3	26264	40797	0.37%	0.043%
39	15.851	2166	2170	2173	rBV6	7750	13547	0.12%	0.014%
40	16.392	2256	2262	2266	rBV	22341	29671	0.27%	0.031%
41	16.827	2331	2336	2339	rBV4	8049	14022	0.13%	0.015%
42	16.910	2347	2350	2358	rVB3	12008	17390	0.16%	0.018%
43	17.233	2396	2405	2413	rBV	3246063	4702011	42.34%	4.953%
44	17.333	2415	2422	2435	rBV	5669860	8213963	73.96%	8.653%
45	17.904	2514	2519	2526	rBV2	171146	210861	1.90%	0.222%
46	18.121	2552	2556	2561	rBV3	54369	76705	0.69%	0.081%
47	19.145	2726	2730	2735	rBV	77666	95231	0.86%	0.100%
48	19.209	2737	2741	2747	rBV	74693	105427	0.95%	0.111%
49	19.357	2762	2766	2771	rBV5	54202	82271	0.74%	0.087%
50	19.568	2796	2802	2810	rBV	7347687	9966463	89.75%	10.499%
51	19.792	2838	2840	2846	rVB3	39253	44345	0.40%	0.047%
52	21.315	3094	3099	3108	rBV	4321119	5230525	47.10%	5.510%
53	23.533	3469	3476	3484	rBV2	5689674	11105248	100.00%	11.698%
54	23.686	3496	3502	3515	rVB	2888492	5737226	51.66%	6.044%




Sum of corrected areas: 94931623

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018540.D
Acq On : 03 Dec 2023 05:38
Operator : MA/JU
Sample : 05411-18
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QL6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

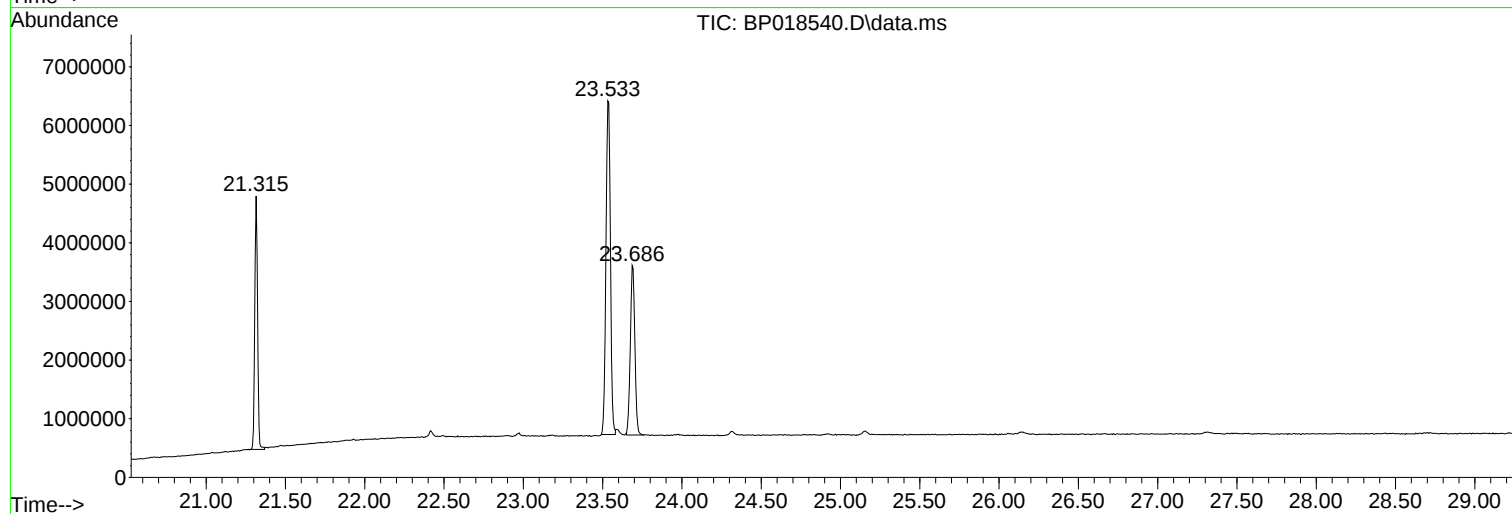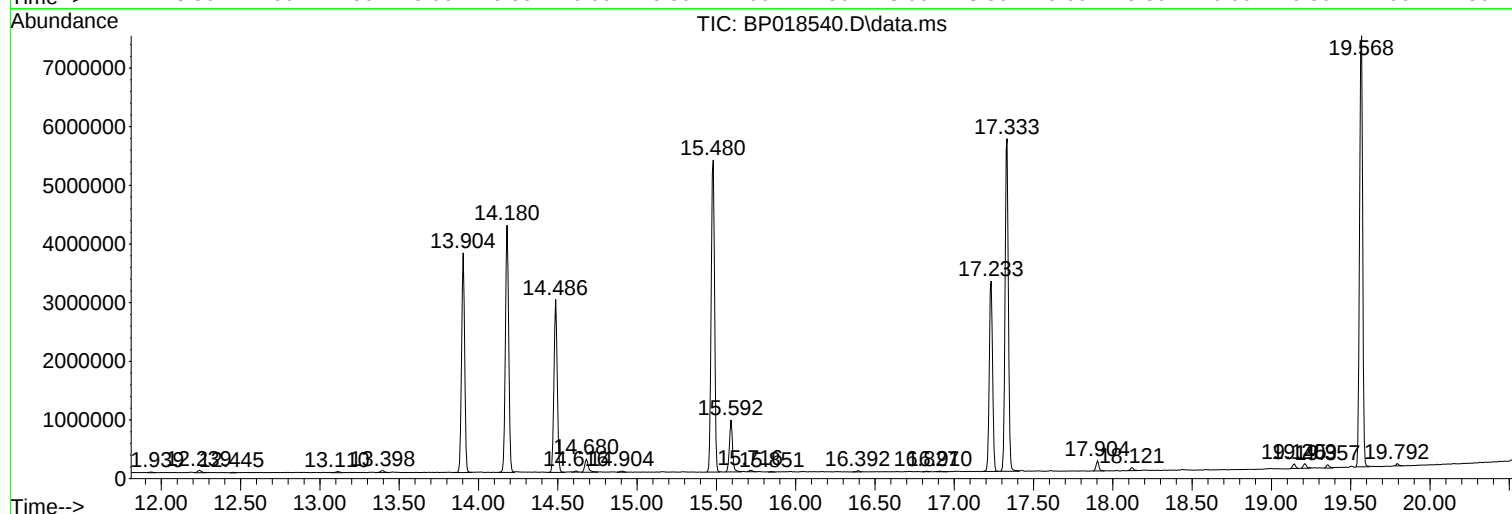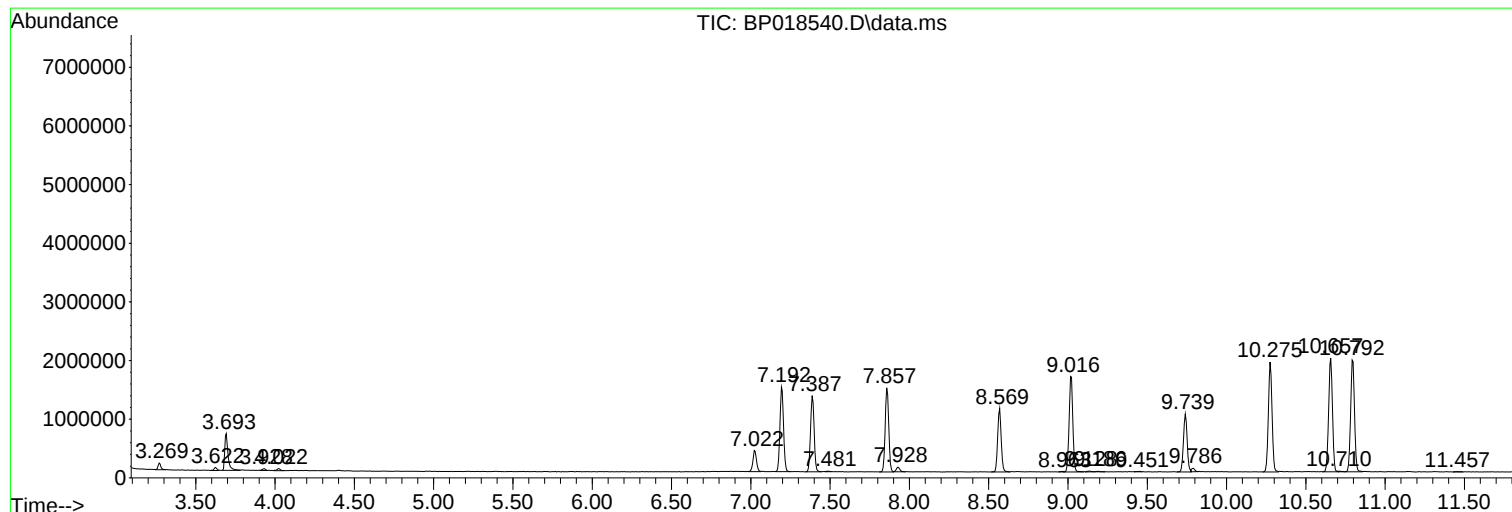

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018540.D
Acq On : 03 Dec 2023 05:38
Operator : MA/JU
Sample : 05411-18
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QL6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018540.D
Acq On : 03 Dec 2023 05:38
Operator : MA/JU
Sample : 05411-18
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QL6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc