

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018541.D
 Acq On : 03 Dec 2023 06:12
 Operator : MA/JU
 Sample : 05411-21
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QL5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018541.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	43	rVB	120150	160302	1.01%	0.117%
2	3.622	88	91	95	rVB2	43218	50599	0.32%	0.037%
3	3.693	99	103	116	rBV	514384	783586	4.93%	0.573%
4	3.928	138	143	147	rVB2	26526	40228	0.25%	0.029%
5	4.022	153	159	164	rVB2	36790	57930	0.36%	0.042%
6	7.022	661	669	677	rVB	493579	753325	4.74%	0.551%
7	7.193	692	698	710	rVB	2237673	3419563	21.53%	2.502%
8	7.387	722	731	740	rBV	1904905	2900669	18.26%	2.123%
9	7.858	801	811	820	rBV	1609041	2498855	15.73%	1.829%
10	7.928	820	823	828	rVB	18881	27631	0.17%	0.020%
11	8.569	925	932	943	rBV	1536141	2415544	15.21%	1.768%
12	8.687	947	952	958	rVB4	7422	16670	0.10%	0.012%
13	8.957	994	998	1001	rBV4	13480	23592	0.15%	0.017%
14	9.016	1001	1008	1018	rVB	2461199	4091622	25.76%	2.994%
15	9.187	1031	1037	1040	rBV5	12507	17187	0.11%	0.013%
16	9.446	1078	1081	1086	rVB5	11060	16571	0.10%	0.012%
17	9.740	1122	1131	1137	rBV	1783508	2790892	17.57%	2.042%
18	9.787	1137	1139	1147	rVB3	49274	73367	0.46%	0.054%
19	10.275	1213	1222	1233	rBV	2942160	4798025	30.21%	3.511%
20	10.440	1246	1250	1256	rVB2	9318	17915	0.11%	0.013%
21	10.657	1279	1287	1294	rBV	2401355	3986216	25.10%	2.917%
22	10.722	1294	1298	1302	rVB7	18032	30494	0.19%	0.022%
23	10.793	1302	1310	1323	rBV	2883950	4832337	30.42%	3.536%
24	11.934	1498	1504	1511	rVB2	14619	24353	0.15%	0.018%
25	12.240	1549	1556	1562	rVB3	61561	102230	0.64%	0.075%
26	13.393	1747	1752	1757	rBV2	35440	55475	0.35%	0.041%
27	13.457	1760	1763	1771	rVB3	12052	24014	0.15%	0.018%
28	13.904	1831	1839	1853	rBV	6294407	8625527	54.30%	6.312%
29	14.181	1877	1886	1895	rBV	6965240	10315632	64.94%	7.549%
30	14.487	1928	1938	1945	rBV	4105134	6002459	37.79%	4.393%
31	14.681	1963	1971	1985	rBV	383968	598605	3.77%	0.438%
32	14.904	2005	2009	2014	rVB5	22962	38320	0.24%	0.028%
33	15.169	2048	2054	2055	rBV3	10840	16010	0.10%	0.012%
34	15.287	2072	2074	2078	rBV3	12867	17784	0.11%	0.013%
35	15.481	2100	2107	2118	rVB	8904242	13094149	82.43%	9.582%
36	15.592	2120	2126	2140	rBV	1878881	2534298	15.95%	1.855%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018541.D
 Acq On : 03 Dec 2023 06:12
 Operator : MA/JU
 Sample : 05411-21
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QL5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	15.710	2142	2146	2154	rVV3	49420	87452	0.55%	0.064%
38	15.792	2156	2160	2165	rVB	58473	71125	0.45%	0.052%
39	16.263	2235	2240	2243	rBV6	11091	18868	0.12%	0.014%
40	16.910	2346	2350	2356	rVB3	14854	27073	0.17%	0.020%
41	17.234	2395	2405	2413	rBV	4818393	7069262	44.50%	5.173%
42	17.334	2415	2422	2436	rVV2	9674191	14486577	91.20%	10.601%
43	17.904	2514	2519	2526	rBV3	176737	228789	1.44%	0.167%
44	18.122	2551	2556	2564	rBV3	92887	133937	0.84%	0.098%
45	19.139	2725	2729	2734	rBV2	126199	178678	1.12%	0.131%
46	19.210	2737	2741	2746	rVV	121209	166376	1.05%	0.122%
47	19.357	2762	2766	2771	rBV5	70526	93375	0.59%	0.068%
48	19.504	2788	2791	2795	rVB4	30170	33490	0.21%	0.025%
49	19.569	2796	2802	2808	rBV	11777709	15884339	100.00%	11.624%
50	19.798	2838	2841	2846	rVB3	61251	76800	0.48%	0.056%
51	21.316	3094	3099	3107	rBV	4802497	5959243	37.52%	4.361%
52	23.539	3469	3477	3484	rBV	6129368	11674859	73.50%	8.544%
53	23.692	3496	3503	3515	rVB	2666004	5207263	32.78%	3.811%




Sum of corrected areas: 136649482

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018541.D
Acq On : 03 Dec 2023 06:12
Operator : MA/JU
Sample : 05411-21
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QL5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

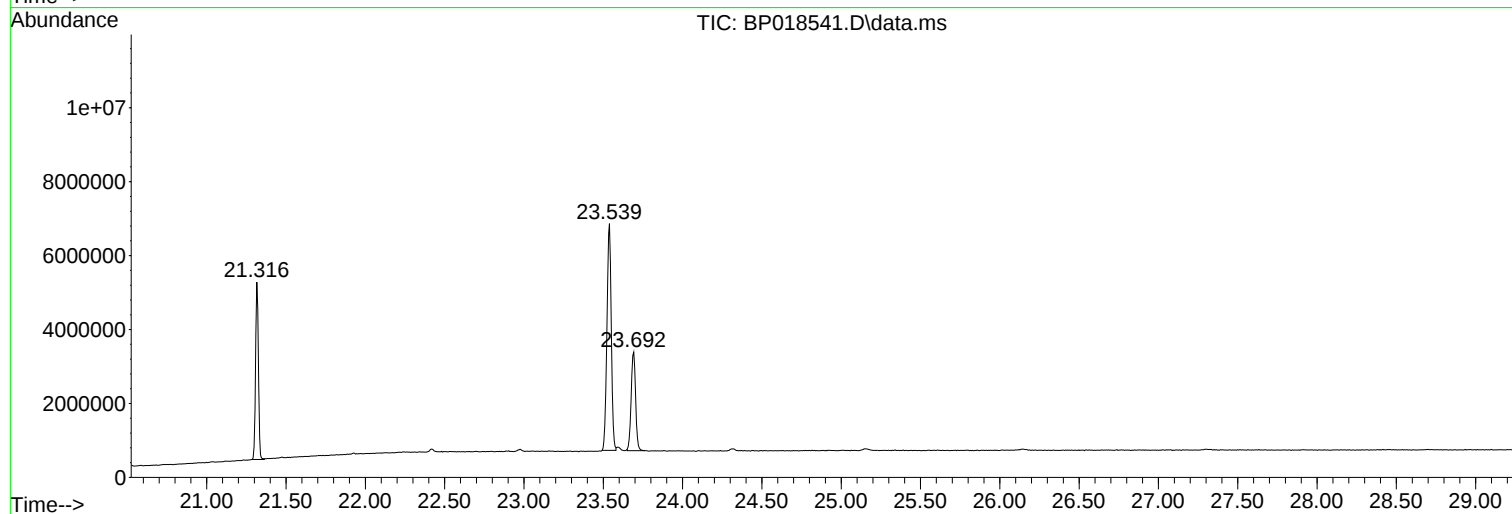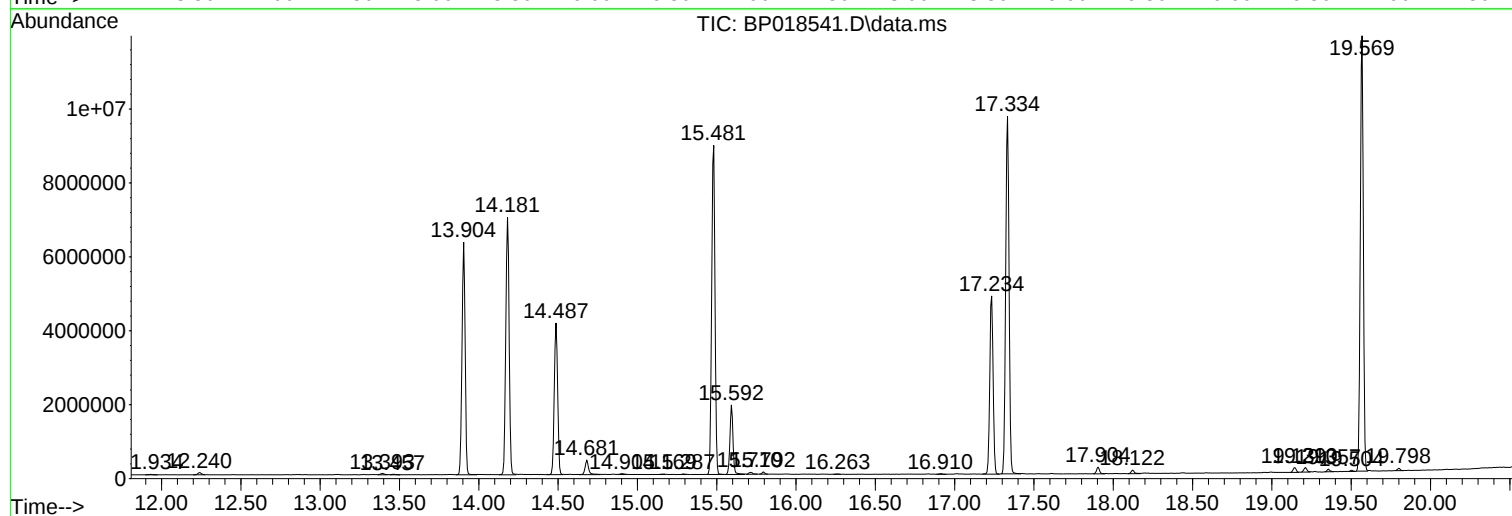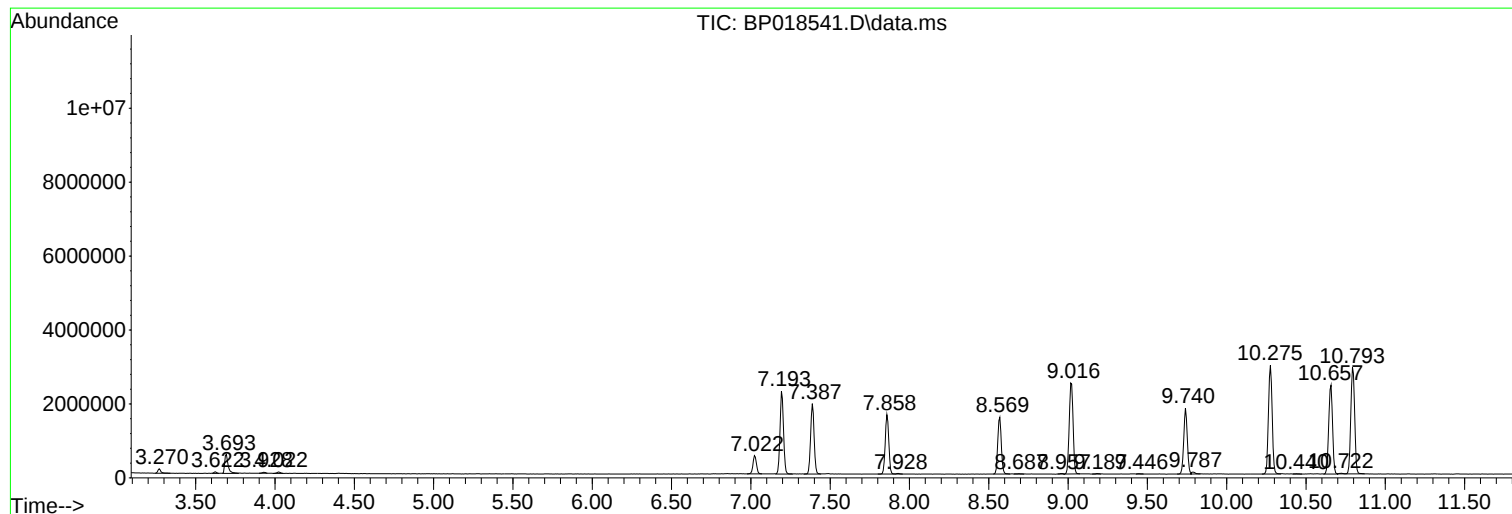

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018541.D
Acq On : 03 Dec 2023 06:12
Operator : MA/JU
Sample : 05411-21
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QL5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018541.D
Acq On : 03 Dec 2023 06:12
Operator : MA/JU
Sample : 05411-21
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QL5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
