

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018542.D
 Acq On : 03 Dec 2023 06:46
 Operator : MA/JU
 Sample : 05424-01
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCG56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018542.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	36	rBV	86805	105105	1.02%	0.105%
2	3.693	98	103	117	rBV	528332	793504	7.72%	0.793%
3	3.928	139	143	150	rVB3	26470	44963	0.44%	0.045%
4	4.016	154	158	163	rBV2	22908	41292	0.40%	0.041%
5	4.463	232	234	241	rVB2	9966	14382	0.14%	0.014%
6	7.022	662	669	679	rVB	356322	552423	5.38%	0.552%
7	7.193	688	698	710	rVB	1588467	2441231	23.76%	2.439%
8	7.387	724	731	741	rBV	1344994	2047927	19.93%	2.046%
9	7.469	741	745	755	rVB4	22868	45656	0.44%	0.046%
10	7.857	803	811	819	rBV	1553111	2385897	23.22%	2.384%
11	8.569	924	932	940	rBV	1073421	1674775	16.30%	1.673%
12	9.016	999	1008	1016	rBV	1745246	2833852	27.58%	2.831%
13	9.187	1031	1037	1044	rBV3	20956	35295	0.34%	0.035%
14	9.446	1075	1081	1085	rBV3	25859	40931	0.40%	0.041%
15	9.740	1123	1131	1139	rBV	1245166	1972075	19.19%	1.970%
16	10.275	1215	1222	1232	rBV	2038927	3262870	31.75%	3.260%
17	10.657	1279	1287	1294	rBV	2170360	3690767	35.92%	3.688%
18	10.793	1299	1310	1322	rBV	1853765	3150203	30.66%	3.148%
19	11.445	1416	1421	1424	rBV2	11524	22991	0.22%	0.023%
20	11.934	1498	1504	1509	rBV2	25777	42840	0.42%	0.043%
21	12.157	1535	1542	1544	rBV3	5333	10971	0.11%	0.011%
22	12.240	1549	1556	1563	rVV2	40959	78299	0.76%	0.078%
23	13.104	1700	1703	1710	rVB4	11294	20392	0.20%	0.020%
24	13.322	1736	1740	1745	rVB4	8463	16918	0.16%	0.017%
25	13.392	1745	1752	1758	rBV	215314	350358	3.41%	0.350%
26	13.457	1760	1763	1767	rVB2	14548	21916	0.21%	0.022%
27	13.710	1803	1806	1811	rBV5	6851	11219	0.11%	0.011%
28	13.904	1832	1839	1848	rBV	4390902	6046061	58.84%	6.041%
29	14.181	1878	1886	1900	rVV	4787474	6964519	67.78%	6.959%
30	14.487	1930	1938	1949	rBV	3565434	5367481	52.23%	5.363%
31	14.681	1966	1971	1981	rBV	285209	424589	4.13%	0.424%
32	14.839	1995	1998	2003	rBV6	10836	17849	0.17%	0.018%
33	14.910	2004	2010	2015	rVB5	21325	39328	0.38%	0.039%
34	15.286	2071	2074	2081	rBV3	8648	22308	0.22%	0.022%
35	15.481	2099	2107	2114	rBV	6275497	9214254	89.67%	9.206%
36	15.592	2120	2126	2137	rBV	1627542	2120215	20.63%	2.118%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018542.D
 Acq On : 03 Dec 2023 06:46
 Operator : MA/JU
 Sample : 05424-01
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCG56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	15.716	2143	2147	2152	rVB3	31339	43652	0.42%	0.044%
38	16.263	2236	2240	2244	rBV4	12022	20055	0.20%	0.020%
39	16.728	2315	2319	2322	rVB4	8404	13355	0.13%	0.013%
40	16.910	2346	2350	2357	rBV6	10922	19740	0.19%	0.020%
41	17.233	2398	2405	2412	rBV	4118849	5894452	57.36%	5.889%
42	17.333	2415	2422	2433	rBV	6682477	9561385	93.05%	9.553%
43	17.610	2464	2469	2472	rBV5	11540	19889	0.19%	0.020%
44	17.910	2516	2520	2525	rVB	37982	44836	0.44%	0.045%
45	18.122	2552	2556	2563	rBV2	190433	254563	2.48%	0.254%
46	18.192	2566	2568	2572	rVB3	16228	21073	0.21%	0.021%
47	18.586	2632	2635	2639	rVB3	20512	28818	0.28%	0.029%
48	19.010	2705	2707	2709	rBV2	20743	20160	0.20%	0.020%
49	19.045	2709	2713	2722	rVB2	171654	215532	2.10%	0.215%
50	19.145	2726	2730	2733	rBV3	86945	114108	1.11%	0.114%
51	19.210	2737	2741	2745	rBV	95093	123461	1.20%	0.123%
52	19.357	2762	2766	2771	rBV2	117406	147894	1.44%	0.148%
53	19.569	2796	2802	2808	rBV	7711365	10275794	100.00%	10.267%
54	21.316	3094	3099	3105	rBV	3850132	4596753	44.73%	4.593%
55	23.539	3469	3477	3484	rBV	4198498	8227088	80.06%	8.220%
56	23.686	3496	3502	3512	rVB	2309369	4516021	43.95%	4.512%




Sum of corrected areas: 100084285

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018542.D
Acq On : 03 Dec 2023 06:46
Operator : MA/JU
Sample : 05424-01
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCG56

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

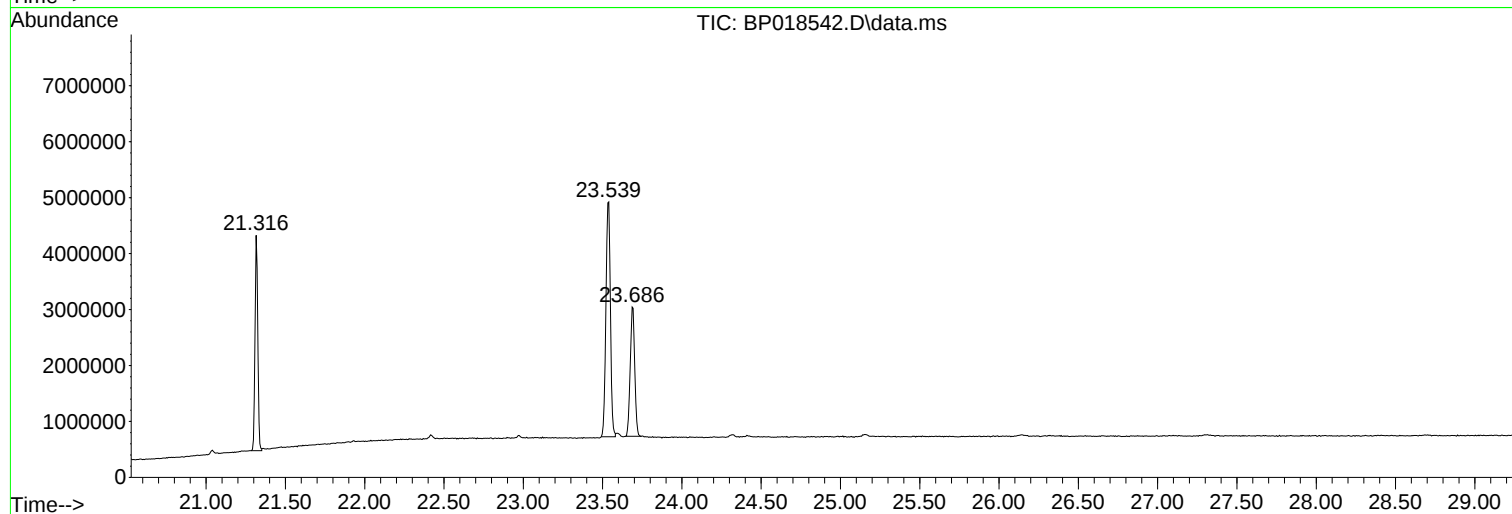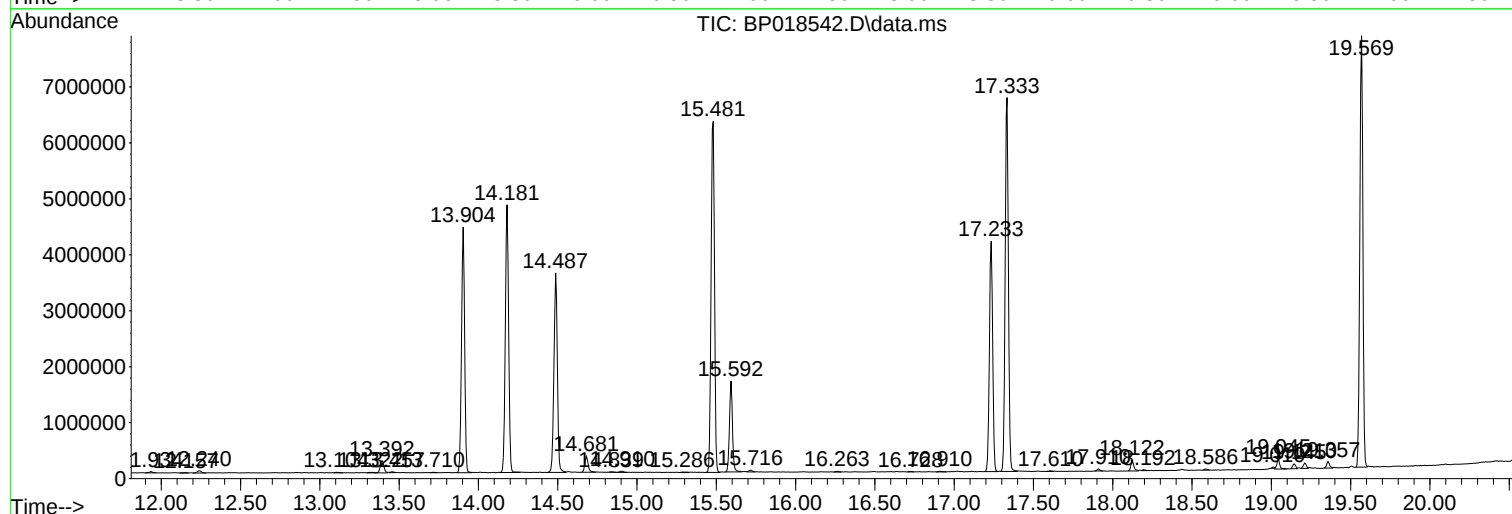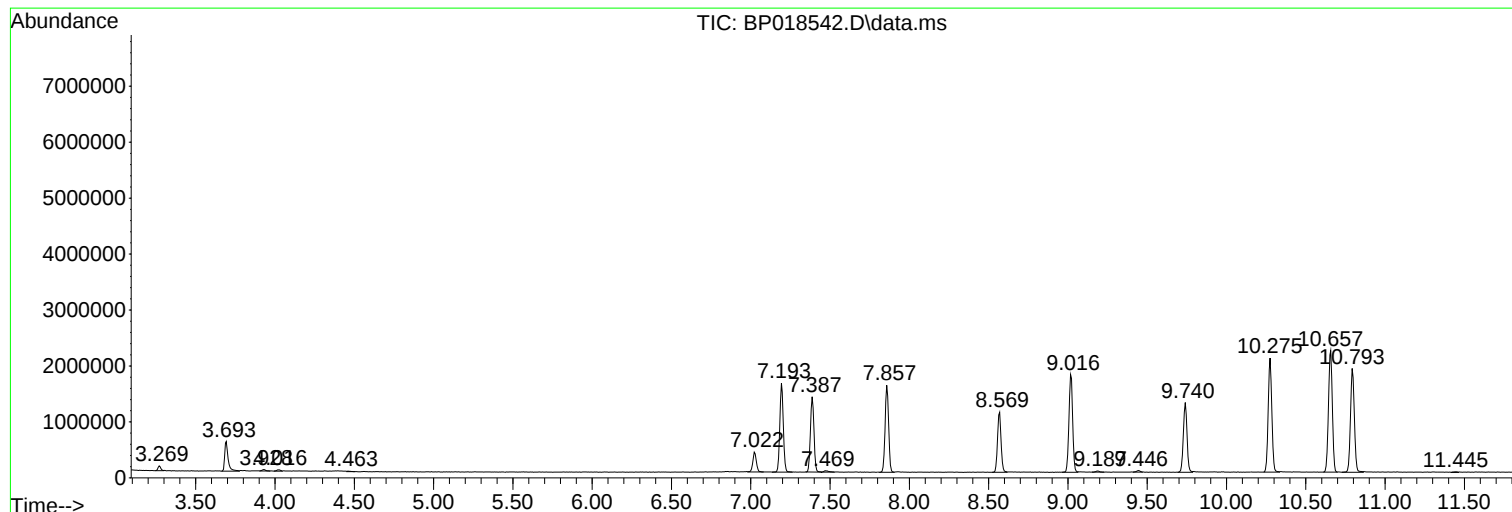

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018542.D
Acq On : 03 Dec 2023 06:46
Operator : MA/JU
Sample : 05424-01
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCG56

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018542.D
Acq On : 03 Dec 2023 06:46
Operator : MA/JU
Sample : 05424-01
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCG56

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc