

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018543.D
 Acq On : 03 Dec 2023 07:20
 Operator : MA/JU
 Sample : 05424-02
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCG58

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018543.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	28	31	38	rVB	85282	102635	0.88%	0.114%
2	3.693	99	103	115	rBV	526942	759643	6.48%	0.842%
3	3.934	139	144	148	rBV2	22381	33573	0.29%	0.037%
4	4.022	155	159	164	rBV2	26548	36175	0.31%	0.040%
5	7.022	662	669	679	rVB	321035	493813	4.21%	0.547%
6	7.193	691	698	711	rBV	1424233	2194600	18.72%	2.431%
7	7.387	724	731	739	rBV	1242781	1905102	16.25%	2.111%
8	7.481	742	747	755	rBV3	18441	36522	0.31%	0.040%
9	7.857	804	811	819	rBV	1332058	2072402	17.67%	2.296%
10	8.569	923	932	940	rBV	927198	1432429	12.22%	1.587%
11	9.016	1001	1008	1016	rBV	1494517	2446425	20.86%	2.710%
12	9.187	1033	1037	1041	rBV5	13871	21842	0.19%	0.024%
13	9.445	1076	1081	1085	rVB3	14556	26364	0.22%	0.029%
14	9.739	1123	1131	1141	rBV	1052417	1667389	14.22%	1.847%
15	10.275	1214	1222	1236	rBV	1694865	2754935	23.49%	3.052%
16	10.657	1278	1287	1296	rVB	1751667	2867633	24.46%	3.177%
17	10.792	1300	1310	1320	rBV	1576719	2655622	22.65%	2.942%
18	11.933	1500	1504	1507	rVB4	11369	15100	0.13%	0.017%
19	12.239	1551	1556	1561	rVB2	31508	49121	0.42%	0.054%
20	13.392	1745	1752	1757	rBV2	66676	110099	0.94%	0.122%
21	13.463	1759	1764	1770	rVB6	17625	31740	0.27%	0.035%
22	13.904	1832	1839	1853	rBV	3165340	4331176	36.94%	4.798%
23	14.180	1879	1886	1896	rBV	3685796	5253953	44.81%	5.821%
24	14.486	1932	1938	1948	rVB	2538567	3706548	31.61%	4.106%
25	14.680	1963	1971	1982	rBV	239001	382451	3.26%	0.424%
26	14.892	2004	2007	2013	rBV4	10873	22596	0.19%	0.025%
27	15.480	2100	2107	2114	rBV	4782538	6966682	59.41%	7.718%
28	15.592	2120	2126	2138	rBV	1201553	1597904	13.63%	1.770%
29	15.716	2143	2147	2155	rVB2	26392	44867	0.38%	0.050%
30	16.257	2234	2239	2248	rVB3	20467	42036	0.36%	0.047%
31	17.016	2365	2368	2374	rBV4	9949	16707	0.14%	0.019%
32	17.233	2398	2405	2412	rBV	3139479	4412422	37.63%	4.888%
33	17.333	2415	2422	2432	rBV	5682235	7979622	68.05%	8.840%
34	17.910	2517	2520	2524	rVB3	22523	24891	0.21%	0.028%
35	18.121	2552	2556	2561	rBV2	64617	90221	0.77%	0.100%
36	19.010	2701	2707	2709	rBV6	23241	46505	0.40%	0.052%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018543.D
Acq On : 03 Dec 2023 07:20
Operator : MA/JU
Sample : 05424-02
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCG58

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	19.045	2709	2713	2718	rVB4	77930	95869	0.82%	0.106%
38	19.139	2726	2729	2733	rBV2	80528	97534	0.83%	0.108%
39	19.210	2737	2741	2745	rBV	74977	106087	0.90%	0.118%
40	19.357	2763	2766	2770	rBV5	32837	39906	0.34%	0.044%
41	19.568	2796	2802	2808	rBV	7965464	10392884	88.63%	11.514%
42	21.315	3094	3099	3104	rBV	4431459	5337857	45.52%	5.914%
43	23.539	3469	3477	3485	rBV2	6040870	11726080	100.00%	12.991%
44	23.692	3496	3503	3512	rVB	2960769	5836642	49.77%	6.466%




Sum of corrected areas: 90264604

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018543.D
Acq On : 03 Dec 2023 07:20
Operator : MA/JU
Sample : 05424-02
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCG58

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

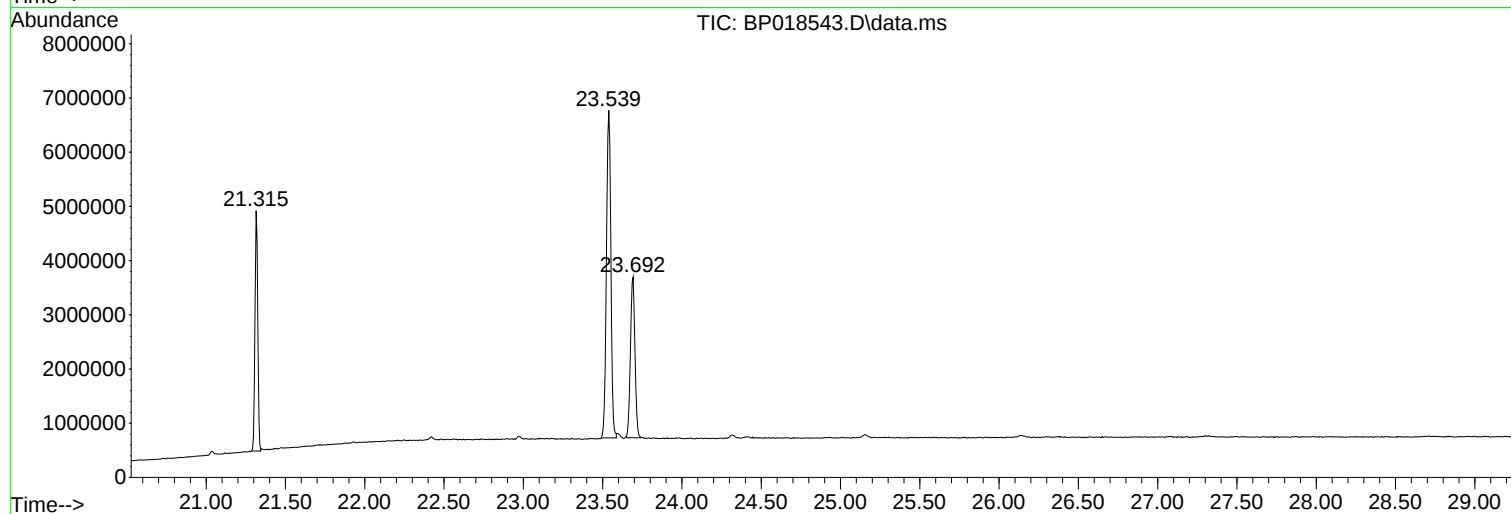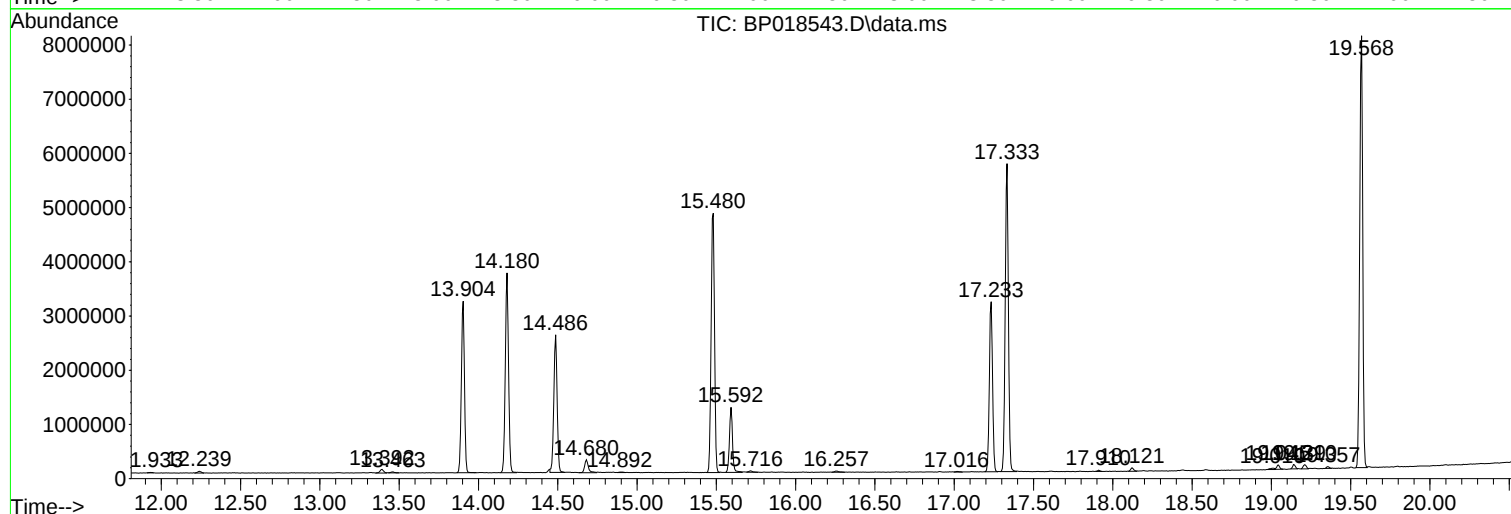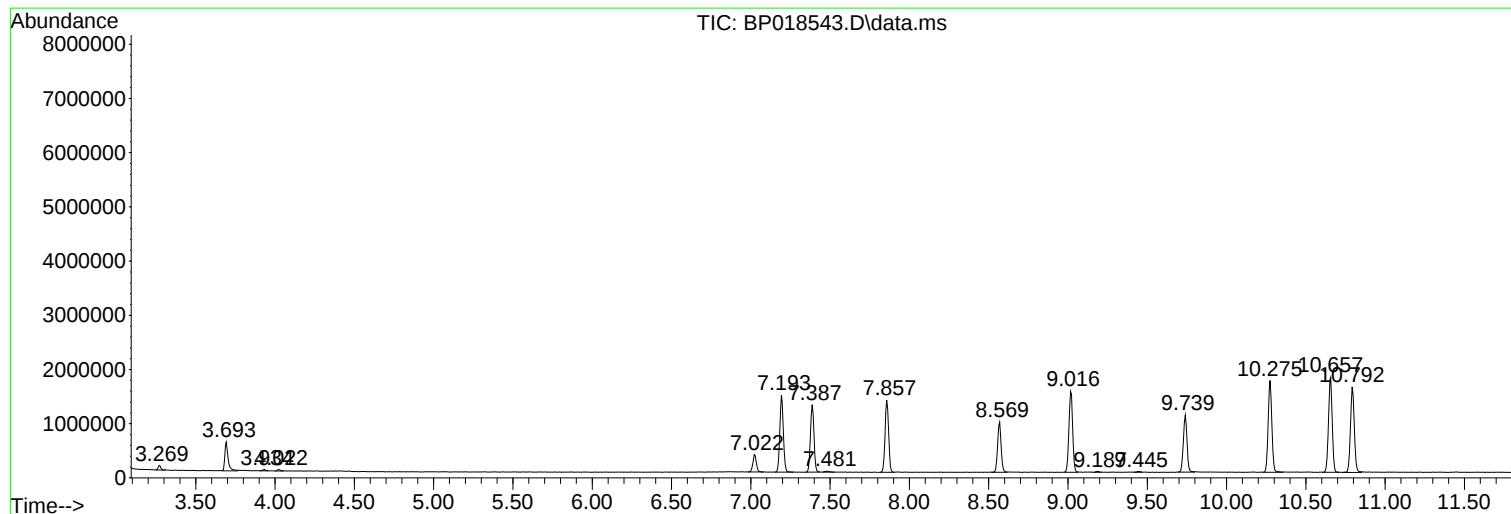

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018543.D
Acq On : 03 Dec 2023 07:20
Operator : MA/JU
Sample : 05424-02
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCG58

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018543.D
Acq On : 03 Dec 2023 07:20
Operator : MA/JU
Sample : 05424-02
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCG58

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------