

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018544.D
 Acq On : 03 Dec 2023 07:54
 Operator : MA/JU
 Sample : 05341-06
 Misc :
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018544.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	28	31	37	rVB	76796	92754	0.96%	0.104%
2	3.693	99	103	115	rBV	426111	626094	6.48%	0.700%
3	3.934	138	144	150	rBV2	21339	38710	0.40%	0.043%
4	4.022	156	159	164	rVB	25565	33265	0.34%	0.037%
5	6.581	592	594	600	rBV2	4363	10397	0.11%	0.012%
6	7.022	662	669	677	rBV	318178	487722	5.04%	0.546%
7	7.193	692	698	708	rVB	1396801	2135518	22.09%	2.389%
8	7.387	723	731	743	rBV	1227778	1882564	19.47%	2.106%
9	7.481	743	747	751	rVB2	7456	14040	0.15%	0.016%
10	7.858	802	811	822	rBV	1280141	1991735	20.60%	2.228%
11	8.569	924	932	944	rBV	961479	1512356	15.64%	1.692%
12	9.016	1000	1008	1015	rBV	1557099	2531781	26.18%	2.833%
13	9.187	1034	1037	1040	rBV2	7320	9866	0.10%	0.011%
14	9.446	1076	1081	1087	rVB4	13415	20171	0.21%	0.023%
15	9.740	1123	1131	1143	rBV	1146875	1811560	18.74%	2.027%
16	10.275	1213	1222	1233	rVV	1851195	3017323	31.21%	3.376%
17	10.652	1278	1286	1296	rBV	1790983	3007027	31.10%	3.364%
18	10.793	1301	1310	1321	rBV	1579724	2617278	27.07%	2.928%
19	11.316	1395	1399	1404	rBV2	5892	12558	0.13%	0.014%
20	11.934	1500	1504	1509	rVB5	6016	11485	0.12%	0.013%
21	12.240	1551	1556	1562	rVB3	38589	61913	0.64%	0.069%
22	13.393	1745	1752	1758	rBV3	44373	71185	0.74%	0.080%
23	13.904	1831	1839	1848	rBV	4250713	5796195	59.95%	6.485%
24	14.181	1877	1886	1897	rBV	4400484	6483267	67.05%	7.254%
25	14.487	1930	1938	1950	rBV	2947783	4317906	44.66%	4.831%
26	14.575	1950	1953	1956	rBV2	7165	10825	0.11%	0.012%
27	14.681	1965	1971	1983	rBV2	229736	378588	3.92%	0.424%
28	14.904	2003	2009	2013	rVB4	18393	34326	0.36%	0.038%
29	15.292	2070	2075	2080	rBV6	13365	29079	0.30%	0.033%
30	15.475	2100	2106	2116	rBV	6065234	8723186	90.22%	9.760%
31	15.592	2120	2126	2137	rBV	1410264	1897008	19.62%	2.122%
32	15.716	2143	2147	2153	rVB3	31131	47962	0.50%	0.054%
33	16.039	2200	2202	2207	rBV3	7436	11071	0.11%	0.012%
34	16.263	2237	2240	2244	rVB4	8610	11327	0.12%	0.013%
35	17.234	2398	2405	2414	rBV	3421187	4725722	48.87%	5.287%
36	17.334	2415	2422	2431	rBV	6437210	9535159	98.61%	10.668%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018544.D
Acq On : 03 Dec 2023 07:54
Operator : MA/JU
Sample : 05341-06
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QJ6

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	17.616	2464	2470	2474	rBV6	10723	19851	0.21%	0.022%
38	18.122	2552	2556	2561	rBV2	63306	79557	0.82%	0.089%
39	19.145	2726	2730	2734	rBV2	82800	103631	1.07%	0.116%
40	19.210	2737	2741	2745	rBV	82123	107499	1.11%	0.120%
41	19.357	2762	2766	2770	rBV3	55467	76773	0.79%	0.086%
42	19.569	2796	2802	2808	rBV	7517595	9669107	100.00%	10.818%
43	21.316	3094	3099	3105	rBV	2962923	3587879	37.11%	4.014%
44	23.539	3470	3477	3484	rBV	4176668	7973820	82.47%	8.921%
45	23.686	3496	3502	3516	rVB	1897131	3763948	38.93%	4.211%




Sum of corrected areas: 89380988

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018544.D
Acq On : 03 Dec 2023 07:54
Operator : MA/JU
Sample : 05341-06
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QJ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

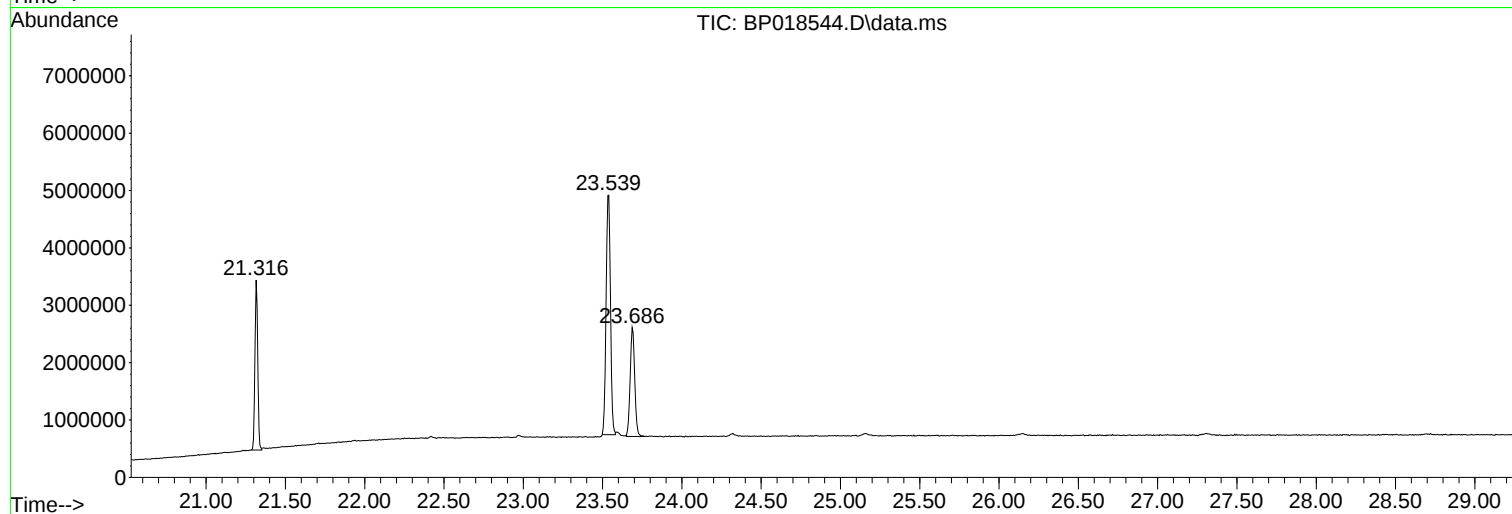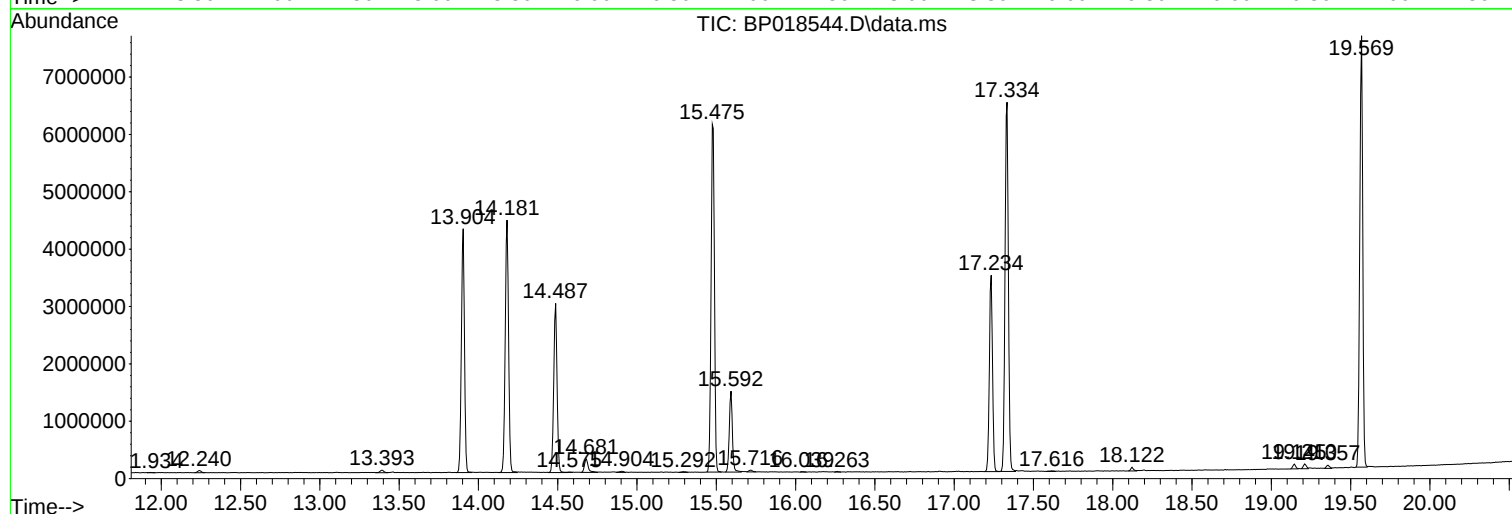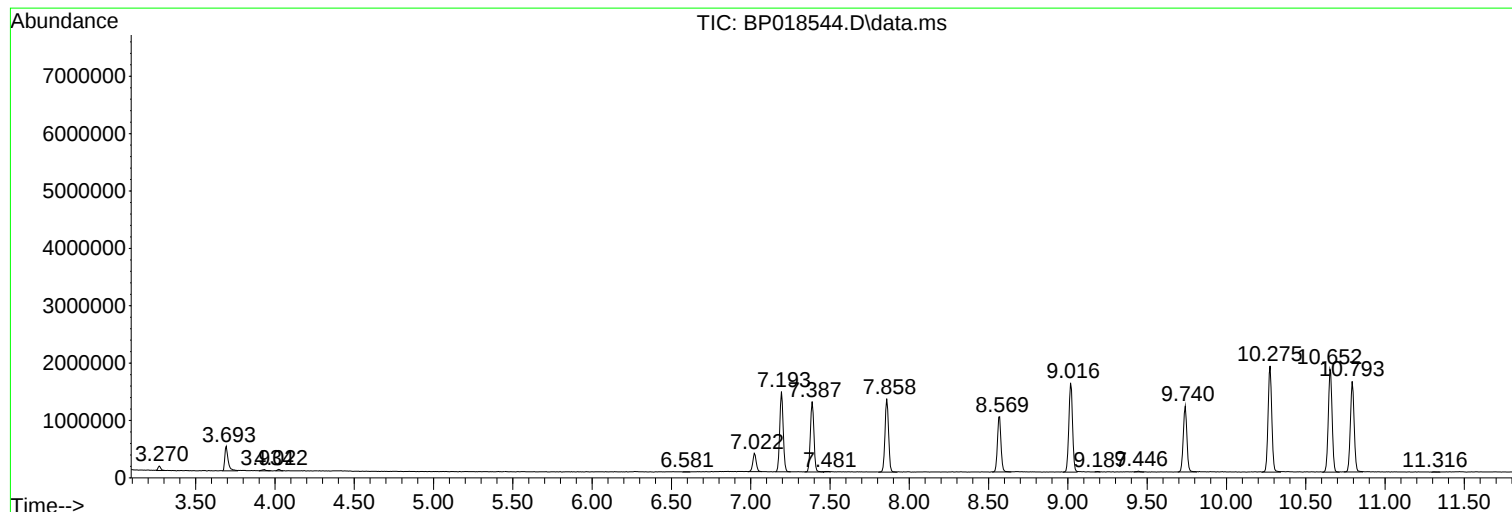

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018544.D
Acq On : 03 Dec 2023 07:54
Operator : MA/JU
Sample : 05341-06
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QJ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018544.D
Acq On : 03 Dec 2023 07:54
Operator : MA/JU
Sample : 05341-06
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QJ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
