

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018545.D
 Acq On : 03 Dec 2023 08:28
 Operator : MA/JU
 Sample : 05341-03
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QK4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018545.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	40	rVB	94959	123275	0.98%	0.114%
2	3.693	98	103	115	rBV	555327	836052	6.61%	0.774%
3	3.899	131	138	139	rBV2	6835	13978	0.11%	0.013%
4	3.934	139	144	148	rVB2	27237	47855	0.38%	0.044%
5	4.022	155	159	167	rVB3	22796	39878	0.32%	0.037%
6	4.104	169	173	181	rBV2	34606	51374	0.41%	0.048%
7	7.022	663	669	677	rVB	407878	616741	4.88%	0.571%
8	7.193	690	698	710	rVB	1517124	2330944	18.44%	2.158%
9	7.387	724	731	741	rBV	1373317	2076727	16.43%	1.923%
10	7.481	745	747	753	rVB4	9106	13641	0.11%	0.013%
11	7.857	803	811	818	rBV	1490698	2323180	18.38%	2.151%
12	8.569	923	932	941	rBV	1196385	1874622	14.83%	1.736%
13	9.016	1001	1008	1019	rBV	1702112	2730835	21.60%	2.529%
14	9.445	1076	1081	1088	rVB4	26161	52387	0.41%	0.049%
15	9.739	1123	1131	1143	rBV	1233264	1977311	15.64%	1.831%
16	10.275	1214	1222	1233	rBV	2060048	3325886	26.31%	3.080%
17	10.657	1279	1287	1295	rVB	2160411	3595105	28.44%	3.329%
18	10.792	1301	1310	1321	rBV	2017139	3420485	27.06%	3.167%
19	11.922	1498	1502	1507	rBV4	7816	15451	0.12%	0.014%
20	12.239	1551	1556	1561	rVB3	40082	64028	0.51%	0.059%
21	13.316	1737	1739	1744	rVB4	12088	15177	0.12%	0.014%
22	13.392	1746	1752	1759	rBV2	47588	81673	0.65%	0.076%
23	13.463	1759	1764	1767	rBV3	9890	17429	0.14%	0.016%
24	13.904	1832	1839	1848	rBV	4529404	6129168	48.48%	5.676%
25	14.022	1854	1859	1864	rBV3	6346	12938	0.10%	0.012%
26	14.180	1877	1886	1898	rBV	4931648	7088799	56.07%	6.564%
27	14.486	1931	1938	1947	rBV	3613593	5317034	42.06%	4.924%
28	14.680	1965	1971	1981	rBV	378180	553382	4.38%	0.512%
29	14.904	2004	2009	2015	rVB5	24359	40387	0.32%	0.037%
30	15.298	2071	2076	2080	rBV5	7911	17470	0.14%	0.016%
31	15.480	2099	2107	2119	rBV	6763895	9608045	76.00%	8.897%
32	15.592	2119	2126	2137	rBV	1806833	2378550	18.81%	2.203%
33	15.716	2143	2147	2154	rVB2	36469	58133	0.46%	0.054%
34	16.910	2346	2350	2356	rVB6	10394	16321	0.13%	0.015%
35	17.233	2398	2405	2411	rVV	4524866	6355033	50.27%	5.885%
36	17.333	2415	2422	2432	rBV	8055155	11320452	89.54%	10.483%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018545.D
Acq On : 03 Dec 2023 08:28
Operator : MA/JU
Sample : 05341-03
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QK4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	18.121	2551	2556	2563	rBV2	171438	235852	1.87%	0.218%
38	18.410	2603	2605	2609	rBV4	9841	13461	0.11%	0.012%
39	19.145	2725	2730	2734	rBV	102581	135499	1.07%	0.125%
40	19.210	2737	2741	2745	rBV	98366	133277	1.05%	0.123%
41	19.357	2762	2766	2774	rBV2	106200	154079	1.22%	0.143%
42	19.568	2796	2802	2809	rBV	9485821	12642648	100.00%	11.707%
43	21.039	3048	3052	3058	rBV3	106152	187748	1.49%	0.174%
44	21.315	3094	3099	3106	rBV	4567902	5679126	44.92%	5.259%
45	23.533	3469	3476	3484	rBV2	4749182	9337787	73.86%	8.647%
46	23.686	3496	3502	3517	rVB	2380875	4931828	39.01%	4.567%




Sum of corrected areas: 107991051

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018545.D
Acq On : 03 Dec 2023 08:28
Operator : MA/JU
Sample : 05341-03
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QK4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

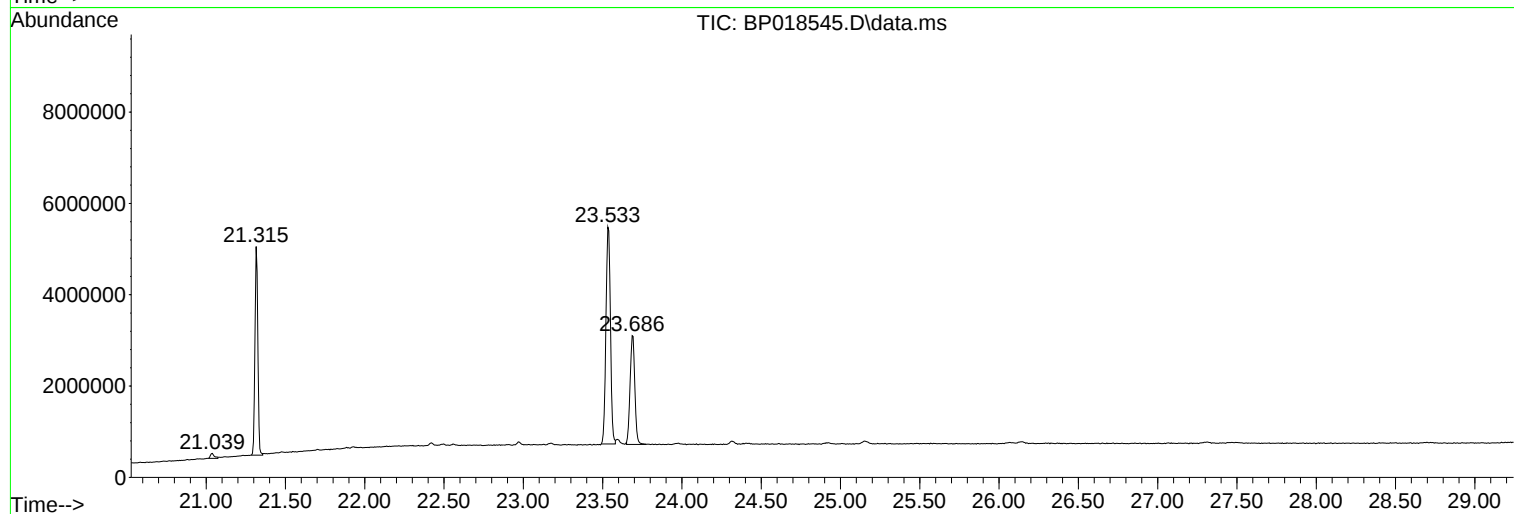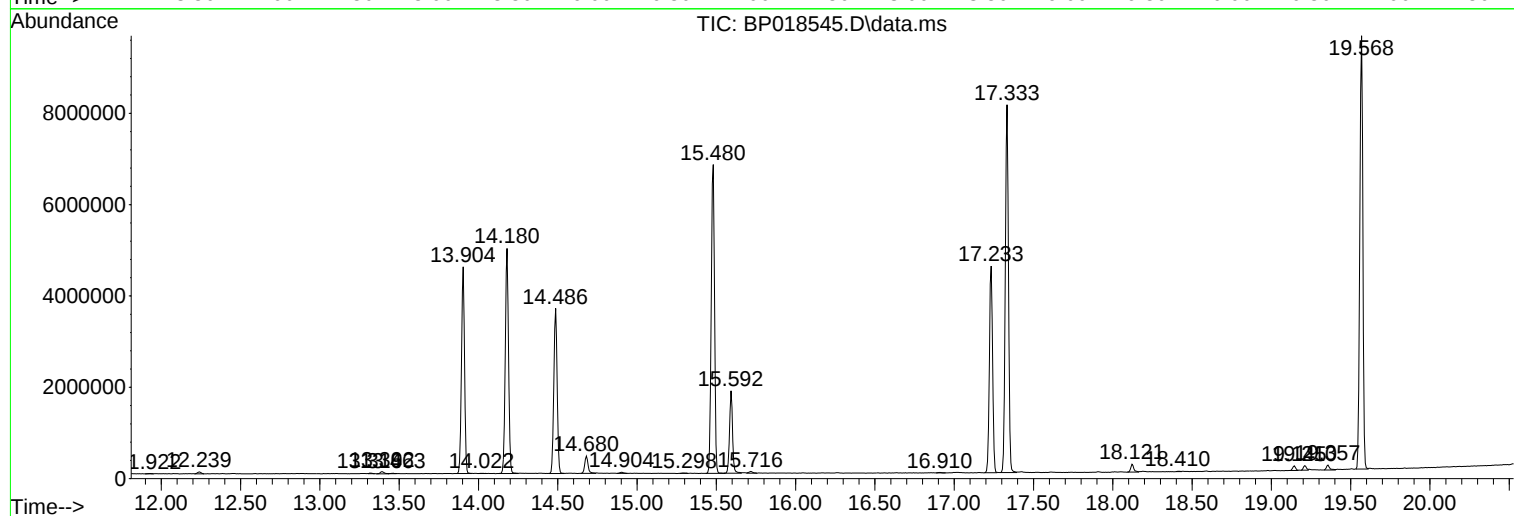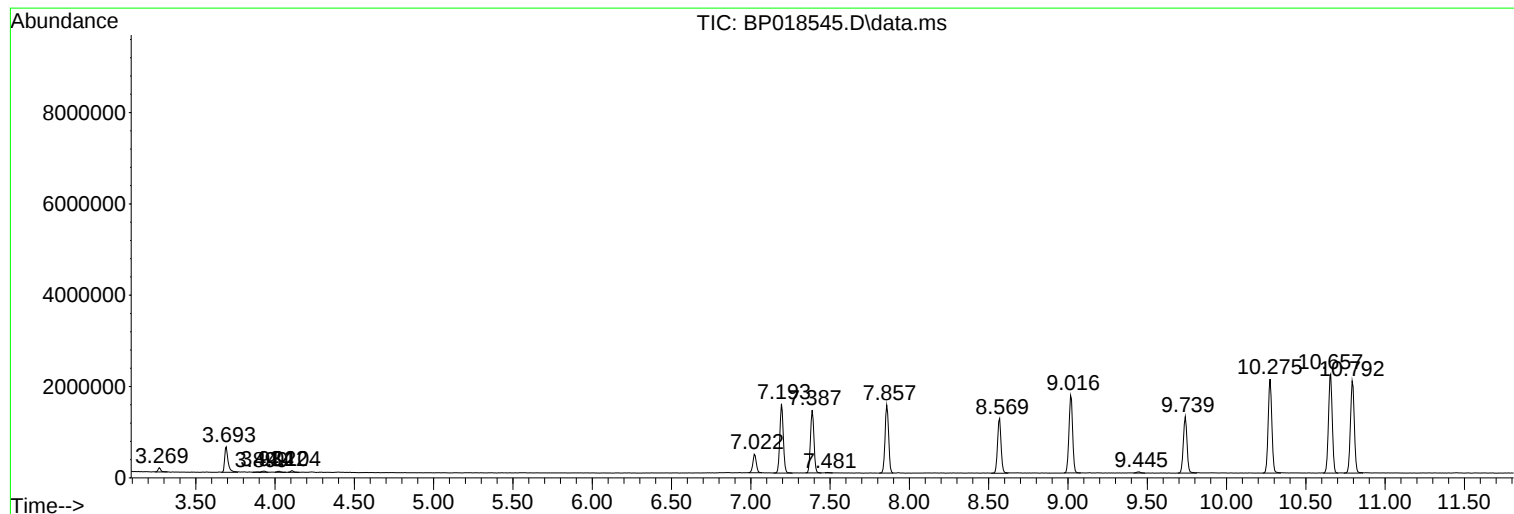

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018545.D
Acq On : 03 Dec 2023 08:28
Operator : MA/JU
Sample : 05341-03
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QK4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018545.D
Acq On : 03 Dec 2023 08:28
Operator : MA/JU
Sample : 05341-03
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QK4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc