

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018546.D
 Acq On : 03 Dec 2023 09:02
 Operator : MA/JU
 Sample : 05341-12
 Misc :
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QE9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018546.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	28	31	38	rVB	84573	106174	1.00%	0.112%
2	3.693	99	103	112	rBV	315147	440140	4.14%	0.465%
3	3.928	140	143	147	rVB2	20839	27736	0.26%	0.029%
4	4.022	155	159	164	rVB2	24920	37128	0.35%	0.039%
5	6.852	636	640	642	rBV3	8087	11896	0.11%	0.013%
6	7.022	663	669	679	rVB	379915	592446	5.58%	0.625%
7	7.193	690	698	709	rVB	1571038	2400002	22.59%	2.533%
8	7.387	723	731	739	rBV	1369087	2126825	20.02%	2.245%
9	7.857	803	811	819	rBV	1330913	2063350	19.42%	2.178%
10	7.928	819	823	829	rVB5	5316	10755	0.10%	0.011%
11	8.569	925	932	941	rBV	1096917	1763834	16.60%	1.862%
12	9.016	1001	1008	1017	rBV	1723468	2792541	26.28%	2.948%
13	9.434	1074	1079	1085	rVB5	9982	21163	0.20%	0.022%
14	9.740	1123	1131	1140	rBV	1255898	1998389	18.81%	2.109%
15	10.275	1213	1222	1235	rBV	2003496	3302299	31.08%	3.486%
16	10.651	1279	1286	1294	rBV	1821020	3072713	28.92%	3.243%
17	10.793	1303	1310	1320	rBV	1695150	2760824	25.98%	2.914%
18	12.240	1551	1556	1561	rVB	40853	61922	0.58%	0.065%
19	13.387	1747	1751	1756	rBV3	32863	52582	0.49%	0.056%
20	13.904	1830	1839	1845	rBV	3965966	5580733	52.53%	5.890%
21	14.181	1875	1886	1895	rBV	4507349	6624502	62.35%	6.992%
22	14.404	1920	1924	1927	rVB2	9649	10752	0.10%	0.011%
23	14.487	1930	1938	1948	rBV	2747621	4118082	38.76%	4.347%
24	14.681	1964	1971	1981	rBV	280785	446906	4.21%	0.472%
25	14.904	2005	2009	2014	rVB6	13785	22983	0.22%	0.024%
26	15.139	2043	2049	2052	rBV4	8742	16721	0.16%	0.018%
27	15.228	2061	2064	2071	rVB2	10265	14636	0.14%	0.015%
28	15.475	2100	2106	2114	rBV	5776862	8381786	78.89%	8.847%
29	15.592	2120	2126	2136	rBV	1446049	1966765	18.51%	2.076%
30	15.716	2139	2147	2155	rVB5	28752	74708	0.70%	0.079%
31	15.992	2191	2194	2198	rVB5	7753	12490	0.12%	0.013%
32	16.039	2200	2202	2207	rVB4	6877	11379	0.11%	0.012%
33	16.257	2237	2239	2244	rVB5	7949	12181	0.11%	0.013%
34	16.910	2348	2350	2356	rVB3	9100	11525	0.11%	0.012%
35	17.004	2361	2366	2369	rVV5	10359	20161	0.19%	0.021%
36	17.039	2369	2372	2376	rVB3	16196	20461	0.19%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018546.D
 Acq On : 03 Dec 2023 09:02
 Operator : MA/JU
 Sample : 05341-12
 Misc :
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QE9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	17.157	2389	2392	2396	rBV	8900	12115	0.11%	0.013%
38	17.233	2398	2405	2412	rVB	3081431	4329018	40.74%	4.569%
39	17.333	2415	2422	2438	rBV	6336745	9351093	88.01%	9.870%
40	17.528	2453	2455	2460	rVB	12997	15928	0.15%	0.017%
41	17.604	2467	2468	2474	rVB3	11207	13902	0.13%	0.015%
42	17.710	2482	2486	2493	rBV2	43220	67365	0.63%	0.071%
43	17.904	2517	2519	2523	rVB3	13591	14882	0.14%	0.016%
44	18.122	2552	2556	2565	rBV2	121114	163645	1.54%	0.173%
45	18.328	2588	2591	2595	rBV2	25488	29454	0.28%	0.031%
46	19.145	2725	2730	2735	rVB2	77455	111190	1.05%	0.117%
47	19.210	2737	2741	2746	rVV	76267	106014	1.00%	0.112%
48	19.357	2762	2766	2773	rBV3	118597	160258	1.51%	0.169%
49	19.569	2796	2802	2808	rBV	7528480	10023979	94.34%	10.580%
50	21.316	3094	3099	3107	rBV	3360812	4120059	38.78%	4.349%
51	23.539	3469	3477	3484	rBV2	5284367	10624839	100.00%	11.214%
52	23.692	3496	3503	3513	rVB	2414997	4608942	43.38%	4.865%




Sum of corrected areas: 94742173

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018546.D
Acq On : 03 Dec 2023 09:02
Operator : MA/JU
Sample : 05341-12
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QE9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

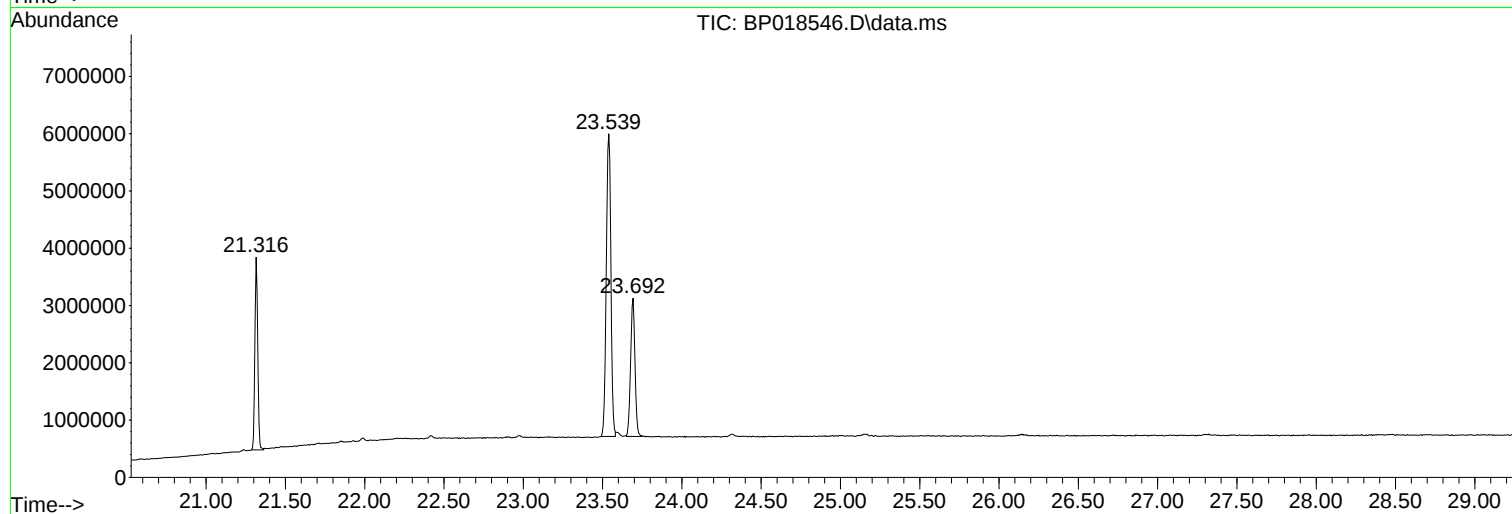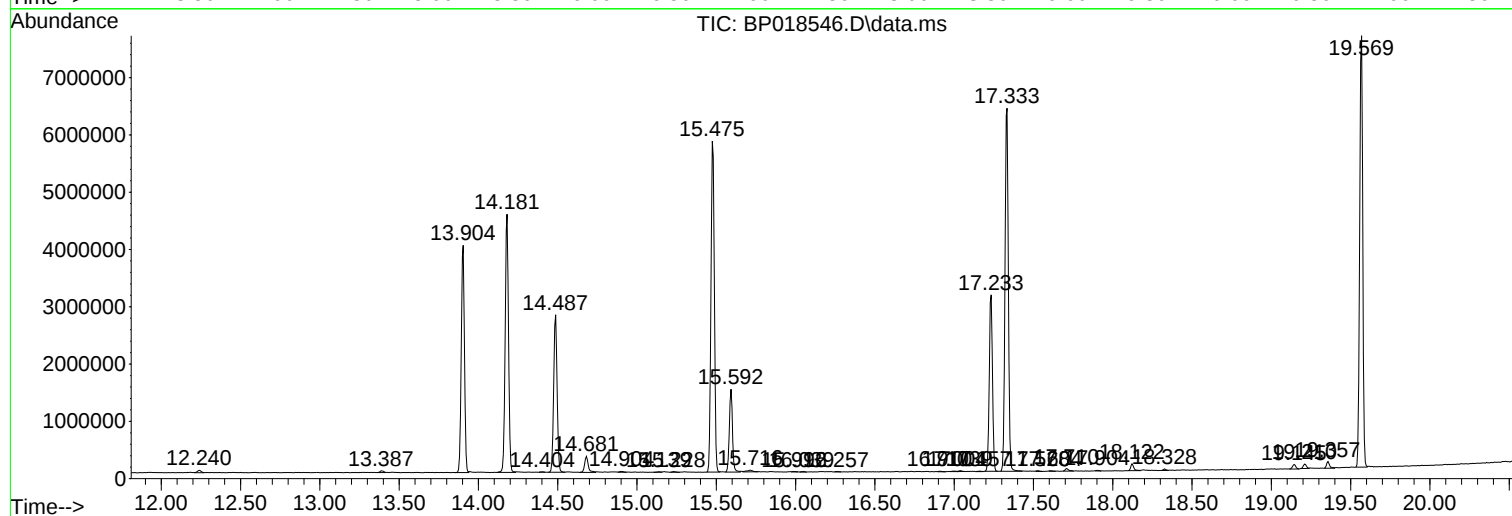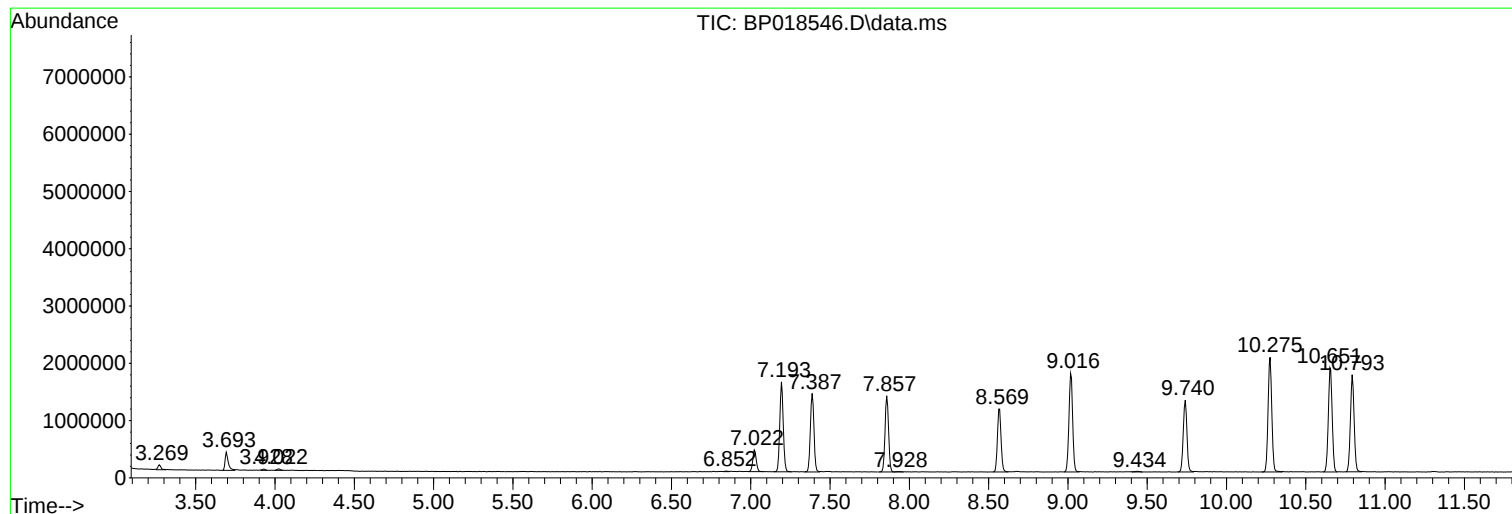

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018546.D
Acq On : 03 Dec 2023 09:02
Operator : MA/JU
Sample : 05341-12
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QE9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018546.D
Acq On : 03 Dec 2023 09:02
Operator : MA/JU
Sample : 05341-12
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QE9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc