

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018548.D
 Acq On : 03 Dec 2023 10:09
 Operator : MA/JU
 Sample : 05341-07
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QJ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018548.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	28	31	40	rVB	82994	110296	1.06%	0.115%
2	3.693	99	103	115	rBV	368846	545732	5.25%	0.569%
3	3.934	139	144	148	rVB2	22195	40544	0.39%	0.042%
4	4.023	156	159	163	rVB	24706	27097	0.26%	0.028%
5	7.022	664	669	677	rVB	336956	501712	4.83%	0.523%
6	7.193	690	698	709	rVB	1523973	2319542	22.32%	2.418%
7	7.387	722	731	742	rBV	1281415	1979377	19.04%	2.063%
8	7.858	801	811	821	rBV	1360205	2092210	20.13%	2.181%
9	8.569	924	932	945	rBV	1020652	1643161	15.81%	1.713%
10	9.016	1001	1008	1016	rBV	1693251	2731010	26.27%	2.846%
11	9.193	1031	1038	1043	rVB4	17207	32648	0.31%	0.034%
12	9.440	1076	1080	1084	rBV2	13668	19405	0.19%	0.020%
13	9.740	1123	1131	1145	rBV	1222240	1989688	19.14%	2.074%
14	10.275	1214	1222	1232	rBV	1999045	3252232	31.29%	3.390%
15	10.652	1278	1286	1299	rBV	1896385	3186096	30.65%	3.321%
16	10.793	1299	1310	1319	rBV	1859952	3112050	29.94%	3.244%
17	11.310	1393	1398	1405	rVB3	4840	13652	0.13%	0.014%
18	12.240	1550	1556	1562	rVB	44775	70538	0.68%	0.074%
19	13.275	1726	1732	1738	rBV5	4842	11394	0.11%	0.012%
20	13.393	1745	1752	1758	rBV2	36232	63494	0.61%	0.066%
21	13.463	1758	1764	1766	rBV3	10706	16870	0.16%	0.018%
22	13.904	1832	1839	1845	rBV	4407385	6108837	58.77%	6.367%
23	14.181	1876	1886	1898	rBV	4793787	7086102	68.17%	7.386%
24	14.487	1930	1938	1947	rBV	3089945	4559258	43.86%	4.752%
25	14.681	1965	1971	1977	rBV	248388	384419	3.70%	0.401%
26	14.898	2005	2008	2014	rVB6	19046	30156	0.29%	0.031%
27	15.481	2099	2107	2114	rBV	6443011	9283930	89.32%	9.676%
28	15.592	2120	2126	2140	rBV	1620633	2141665	20.60%	2.232%
29	15.716	2143	2147	2152	rVB4	36366	55575	0.53%	0.058%
30	16.045	2199	2203	2206	rVB4	9638	14146	0.14%	0.015%
31	17.016	2365	2368	2373	rVB4	8047	12114	0.12%	0.013%
32	17.234	2398	2405	2412	rBV	3637862	5086921	48.94%	5.302%
33	17.334	2415	2422	2433	rBV2	6919691	10138849	97.54%	10.567%
34	17.904	2517	2519	2524	rVB4	8136	11159	0.11%	0.012%
35	18.122	2551	2556	2562	rBV2	189826	251339	2.42%	0.262%
36	19.145	2725	2730	2734	rBV2	88384	123738	1.19%	0.129%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018548.D
Acq On : 03 Dec 2023 10:09
Operator : MA/JU
Sample : 05341-07
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QJ8

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	19.210	2737	2741	2745	rBV	90807	123763	1.19%	0.129%
38	19.357	2762	2766	2771	rBV2	157671	205014	1.97%	0.214%
39	19.504	2789	2791	2795	rVB4	30413	26913	0.26%	0.028%
40	19.569	2796	2802	2808	rVV	7690735	10394252	100.00%	10.833%
41	21.316	3094	3099	3107	rBV	3232962	3968370	38.18%	4.136%
42	23.539	3470	3477	3484	rBV2	4314858	8193848	78.83%	8.540%
43	23.692	3496	3503	3517	rVB	2053658	3986438	38.35%	4.155%




Sum of corrected areas: 95945554

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018548.D
Acq On : 03 Dec 2023 10:09
Operator : MA/JU
Sample : 05341-07
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QJ8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

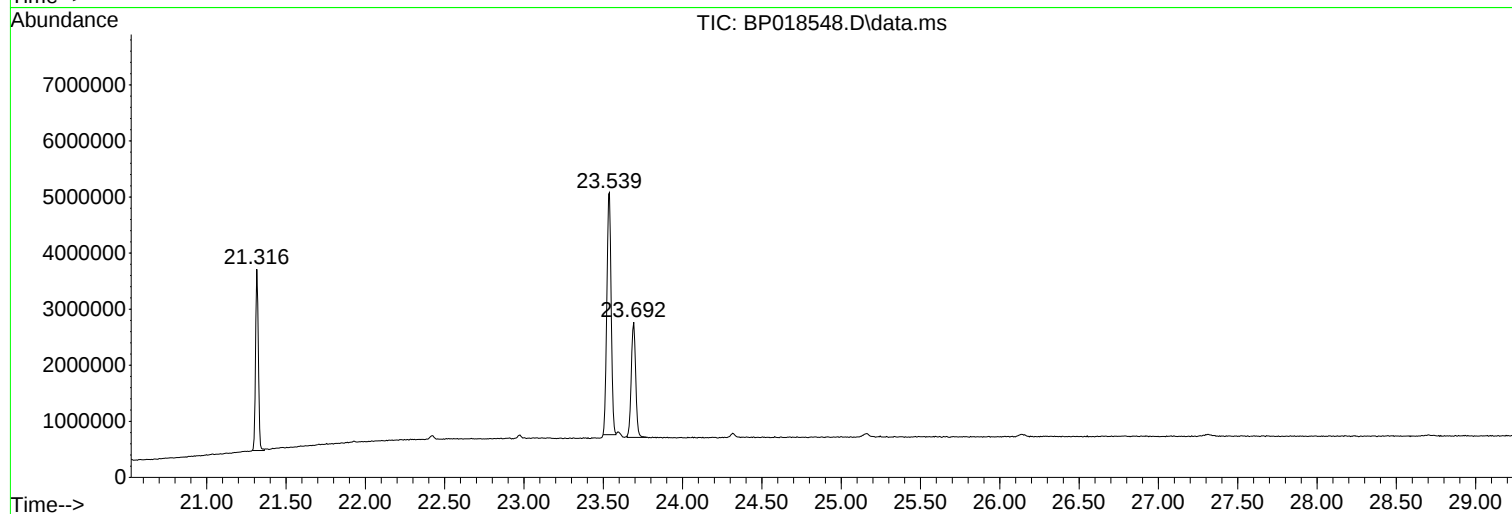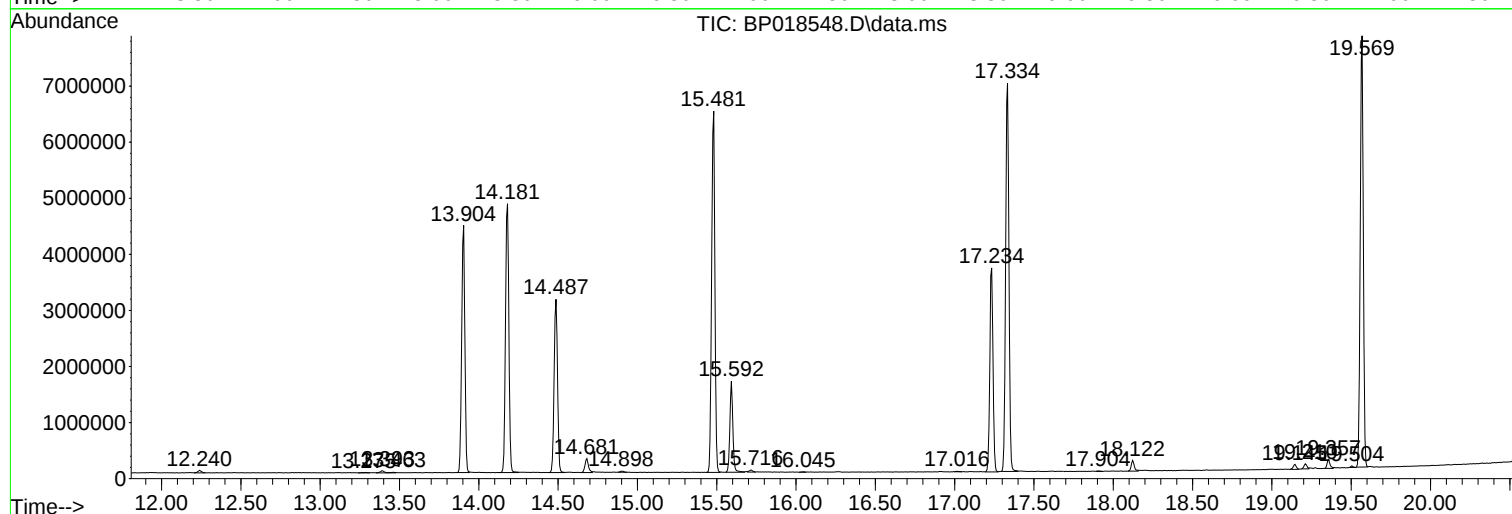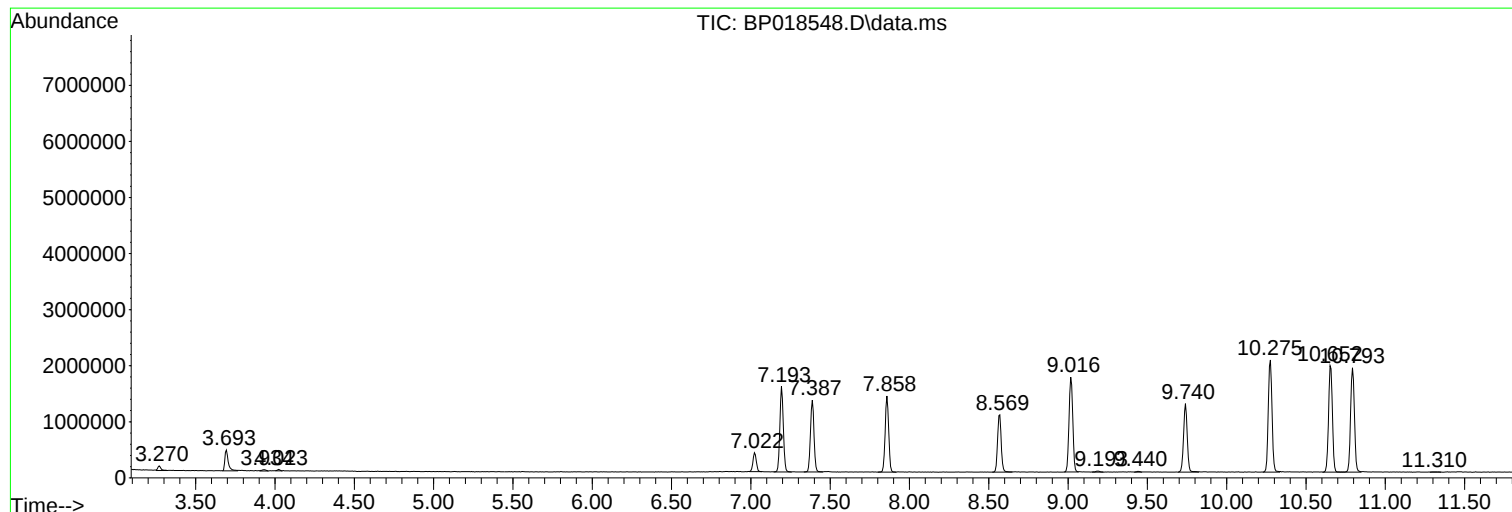

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018548.D
Acq On : 03 Dec 2023 10:09
Operator : MA/JU
Sample : 05341-07
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QJ8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018548.D
Acq On : 03 Dec 2023 10:09
Operator : MA/JU
Sample : 05341-07
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QJ8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------