

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
 Data File : BP018551.D
 Acq On : 03 Dec 2023 11:51
 Operator : MA/JU
 Sample : PB157194BL
 Misc :
 ALS Vial : 82 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK194

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018551.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	39	rVB	127513	163340	1.53%	0.148%
2	3.687	98	102	117	rBV	1704577	2391140	22.38%	2.160%
3	4.023	155	159	164	rVB2	41777	58359	0.55%	0.053%
4	7.022	663	669	681	rVB	1831705	2844457	26.62%	2.570%
5	7.193	692	698	706	rVB	1622502	2429189	22.73%	2.195%
6	7.387	723	731	741	rBV	1861831	2849333	26.67%	2.574%
7	7.858	804	811	818	rBV	1338219	2081236	19.48%	1.880%
8	8.569	924	932	942	rBV	2385085	3745221	35.05%	3.384%
9	9.016	1000	1008	1016	rBV	1811589	2909421	27.23%	2.629%
10	9.187	1034	1037	1041	rVB3	11027	16763	0.16%	0.015%
11	9.740	1120	1131	1141	rBV	1423450	2268848	21.23%	2.050%
12	10.275	1214	1222	1229	rBV	2388820	3870686	36.23%	3.497%
13	10.328	1229	1231	1236	rVB2	8259	11045	0.10%	0.010%
14	10.652	1278	1286	1294	rBV	1938629	3274799	30.65%	2.959%
15	10.793	1302	1310	1322	rBV	2535994	4164599	38.98%	3.763%
16	12.240	1551	1556	1565	rVB2	47220	78096	0.73%	0.071%
17	13.393	1748	1752	1758	rVB2	50605	75936	0.71%	0.069%
18	13.457	1758	1763	1768	rVB4	8900	17254	0.16%	0.016%
19	13.904	1830	1839	1846	rBV	4672681	6441376	60.28%	5.819%
20	14.181	1879	1886	1895	rBV	5219210	7599075	71.12%	6.865%
21	14.487	1931	1938	1947	rBV	3377101	4860716	45.49%	4.391%
22	14.681	1965	1971	1985	rBV	1943469	2785962	26.07%	2.517%
23	14.904	2006	2009	2014	rVB4	13619	18127	0.17%	0.016%
24	15.481	2100	2107	2115	rBV	6623395	9577081	89.63%	8.652%
25	15.592	2119	2126	2138	rBV	1610567	2187726	20.47%	1.977%
26	15.716	2143	2147	2153	rVB2	32873	54658	0.51%	0.049%
27	16.040	2198	2202	2209	rVB2	8362	12670	0.12%	0.011%
28	16.257	2236	2239	2245	rVB4	9222	14242	0.13%	0.013%
29	16.910	2347	2350	2356	rVB5	10518	14539	0.14%	0.013%
30	17.022	2366	2369	2375	rVB6	11248	16663	0.16%	0.015%
31	17.234	2398	2405	2412	rVB	4137879	5695809	53.31%	5.146%
32	17.334	2415	2422	2437	rVV	7093294	10037367	93.94%	9.068%
33	18.122	2553	2556	2561	rBV6	18314	26794	0.25%	0.024%
34	19.145	2726	2730	2735	rBV2	87208	112772	1.06%	0.102%
35	19.210	2737	2741	2747	rBV	76213	112015	1.05%	0.101%
36	19.569	2796	2802	2808	rBV	7947196	10684909	100.00%	9.653%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018551.D
Acq On : 03 Dec 2023 11:51
Operator : MA/JU
Sample : PB157194BL
Misc :
ALS Vial : 82 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK194

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	21.316	3094	3099	3106	rBV	3694291	4656187	43.58%	4.207%
38	23.533	3469	3476	3484	rBV2	4190781	8191550	76.66%	7.401%
39	23.686	3496	3502	3513	rVB	2189190	4336705	40.59%	3.918%




Sum of corrected areas: 110686665

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018551.D
Acq On : 03 Dec 2023 11:51
Operator : MA/JU
Sample : PB157194BL
Misc :
ALS Vial : 82 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK194

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

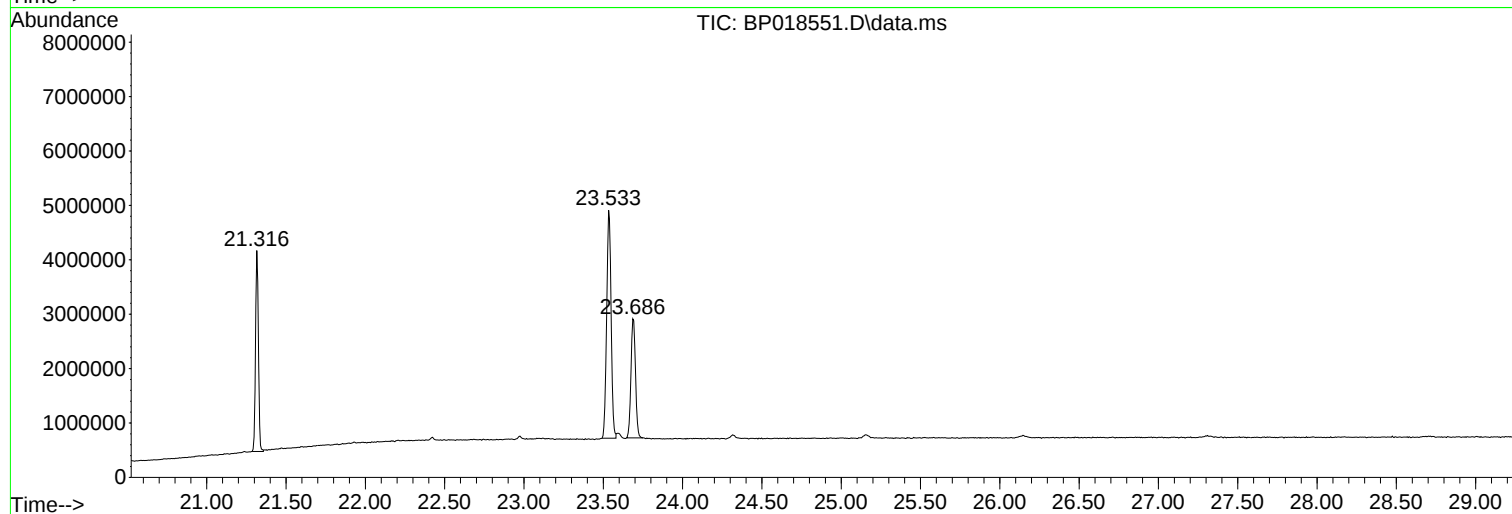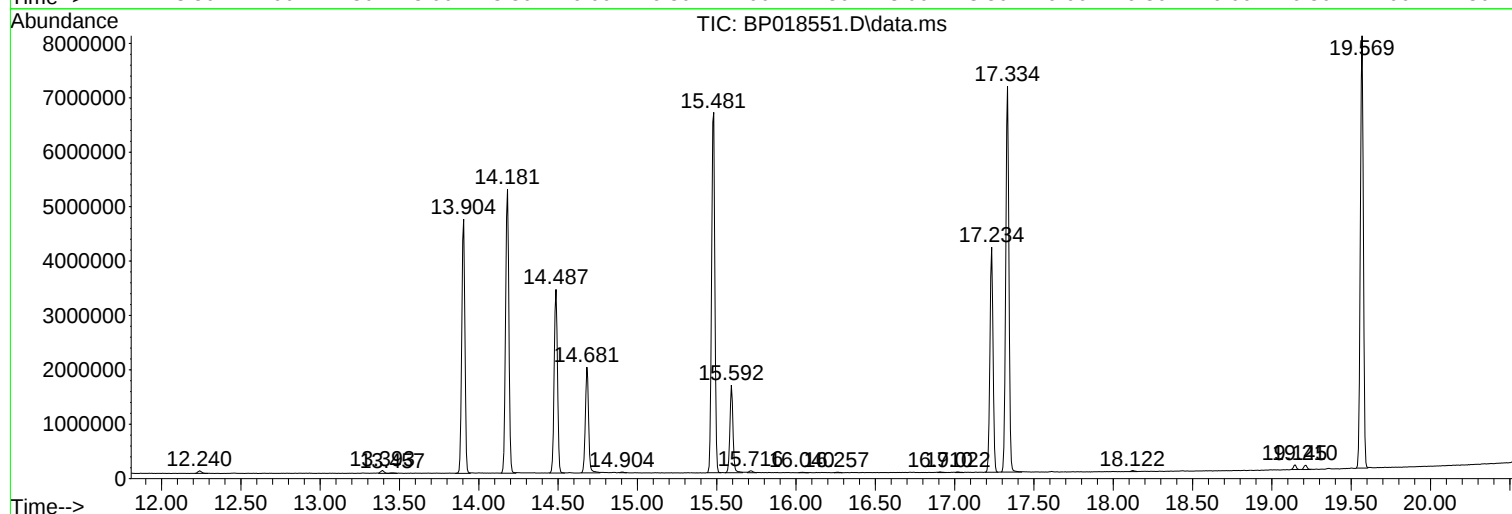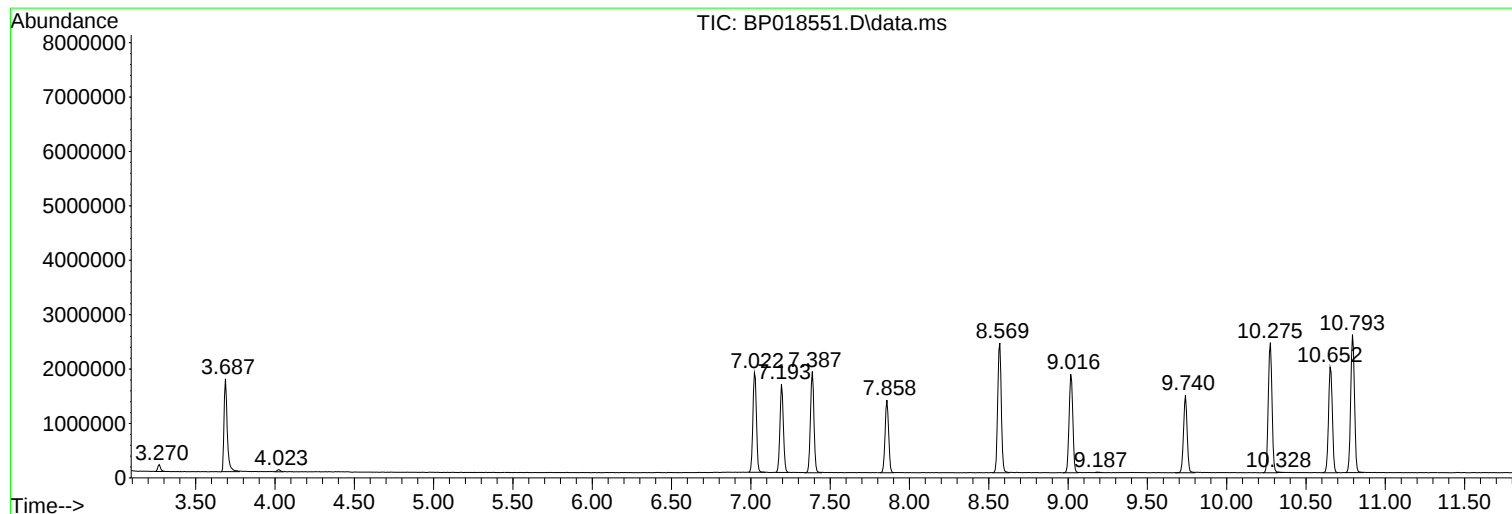

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018551.D
Acq On : 03 Dec 2023 11:51
Operator : MA/JU
Sample : PB157194BL
Misc :
ALS Vial : 82 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK194

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120123\
Data File : BP018551.D
Acq On : 03 Dec 2023 11:51
Operator : MA/JU
Sample : PB157194BL
Misc :
ALS Vial : 82 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK194

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------