

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120125\
 Data File : BP026205.D
 Acq On : 01 Dec 2025 20:43
 Operator : RC/JU
 Sample : Q3716-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 MW3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP026205.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.825	315	321	332	rVB	395325	554659	3.58%	0.955%
2	5.284	391	399	408	rBV	2072752	3114050	20.09%	5.364%
3	6.837	656	663	682	rBV	1071954	1903257	12.28%	3.278%
4	7.655	793	802	811	rBV	797026	1221637	7.88%	2.104%
5	8.796	987	996	1008	rBV	2531313	4350919	28.07%	7.494%
6	10.419	1265	1272	1280	rBV	915501	1600006	10.32%	2.756%
7	12.896	1685	1693	1703	rBV	6001901	10198634	65.80%	17.566%
8	14.290	1922	1930	1940	rBV	1279574	2099368	13.54%	3.616%
9	15.678	2159	2166	2171	rBV	335617	487819	3.15%	0.840%
10	15.801	2180	2187	2205	rBV	5173012	7728807	49.86%	13.312%
11	17.089	2400	2406	2415	rBV2	1572771	2455302	15.84%	4.229%
12	18.042	2563	2568	2577	rBV2	117774	221957	1.43%	0.382%
13	19.830	2866	2872	2878	rBV	11151941	15499485	100.00%	26.696%
14	21.530	3155	3161	3174	rBV	1982336	3146326	20.30%	5.419%
15	24.807	3710	3718	3736	rVB	1222009	3476148	22.43%	5.987%




Sum of corrected areas: 58058374

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120125\
Data File : BP026205.D
Acq On : 01 Dec 2025 20:43
Operator : RC/JU
Sample : Q3716-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
MW3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

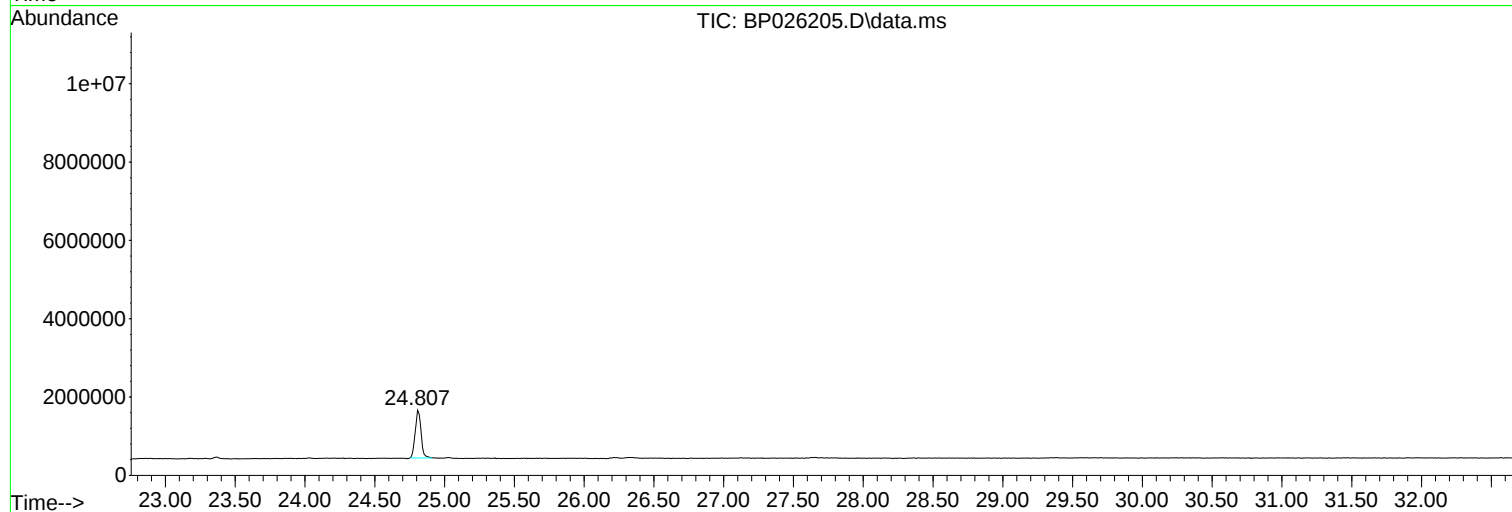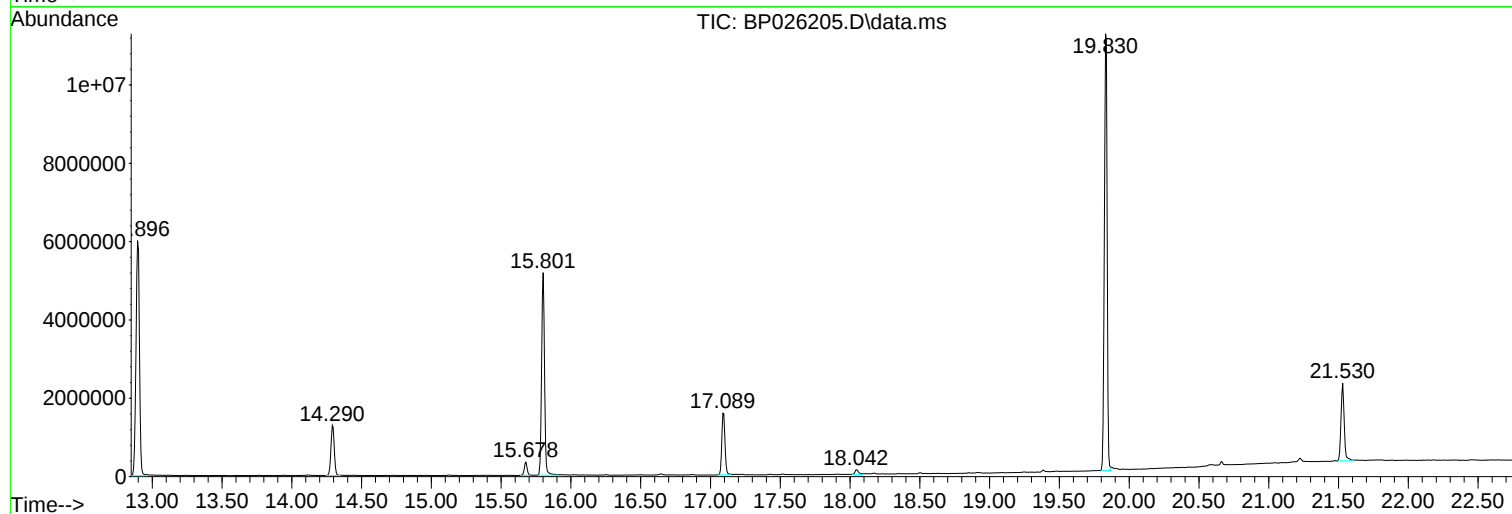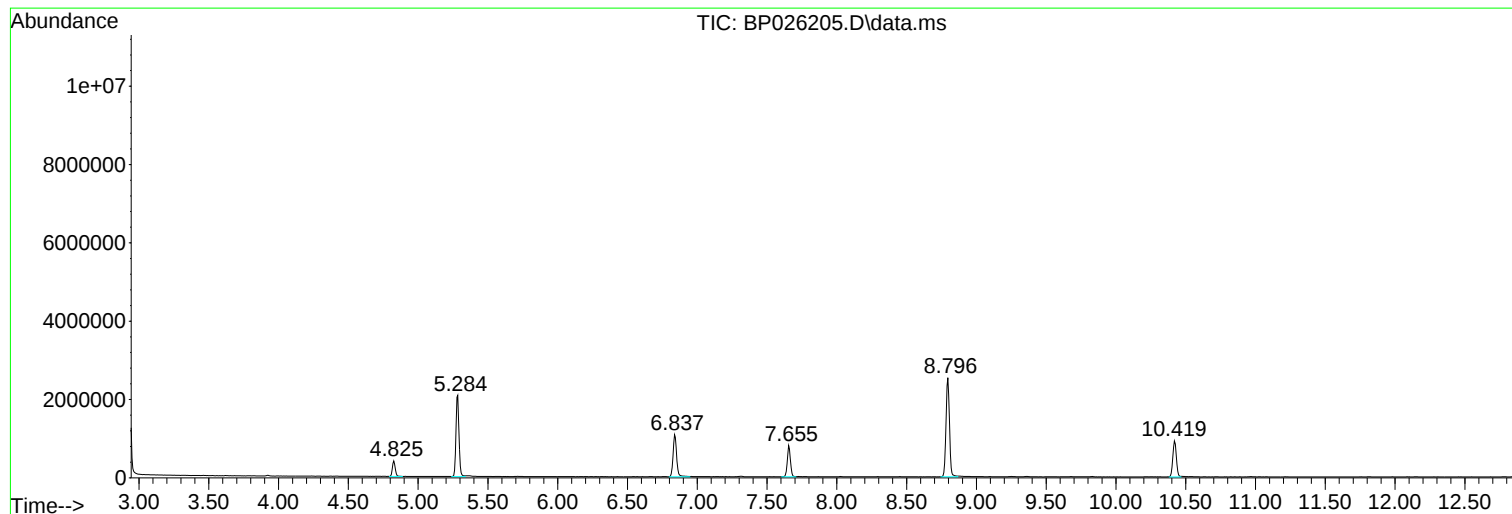

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120125\
Data File : BP026205.D
Acq On : 01 Dec 2025 20:43
Operator : RC/JU
Sample : Q3716-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
MW3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Benzophenone Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.678	4.65 ng	487819	Acenaphthene-d10	14.290

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	96
2			1,2,4,5-Tetroxane, 3,3,6,6-tetra...	396	C26H20O4	016204-36-7	64
3			Azobenzene	182	C12H10N2	000103-33-3	50
4			1,2,4-Trioxolane, 3,3,5-triphenyl-	304	C20H16O3	023246-12-0	50
5			Benzenamine, N-(3-pyridinylmethy...	182	C12H10N2	029722-97-2	45

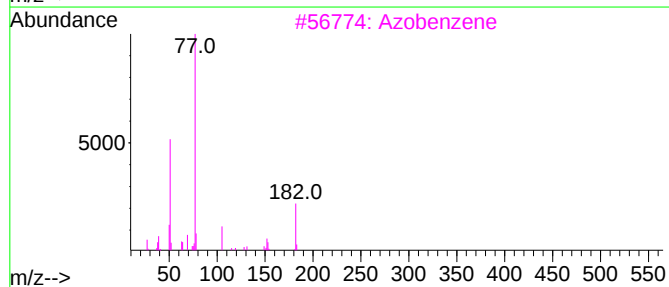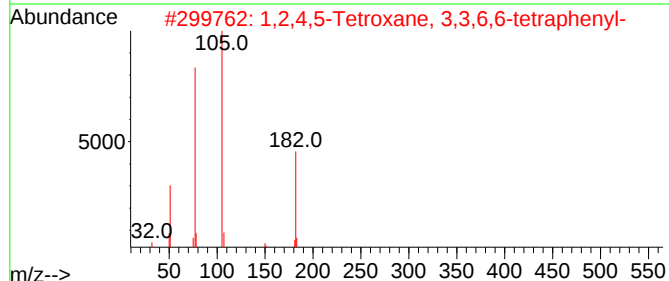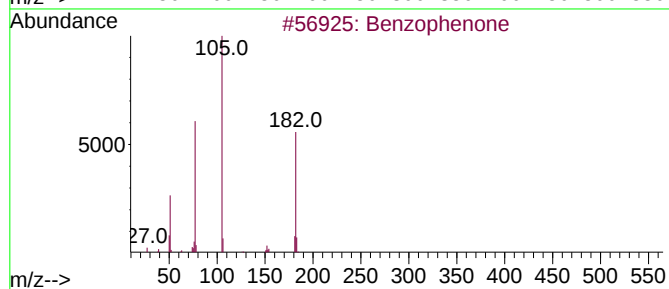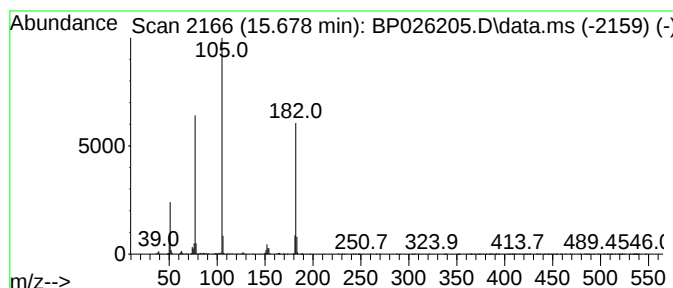

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120125\
Data File : BP026205.D
Acq On : 01 Dec 2025 20:43
Operator : RC/JU
Sample : Q3716-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
MW3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	15.678	4.7	ng	487819	3	14.290	2099370	20.0