
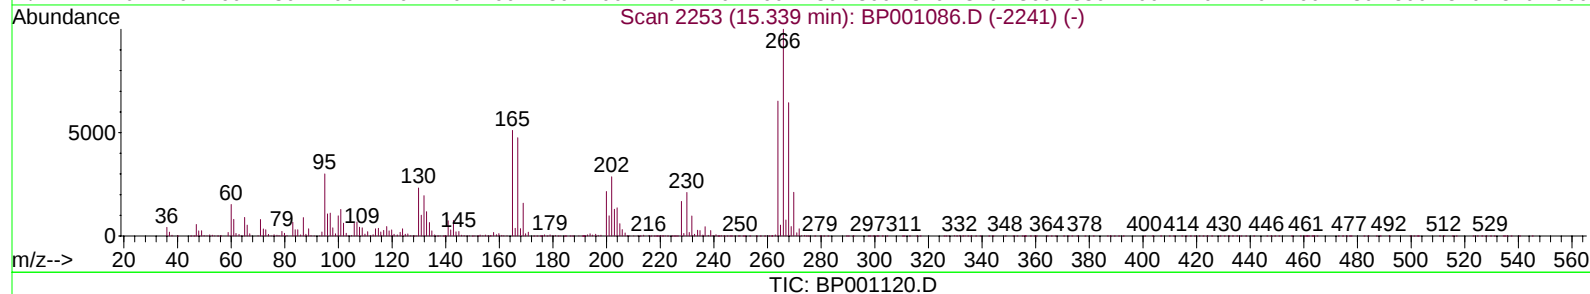
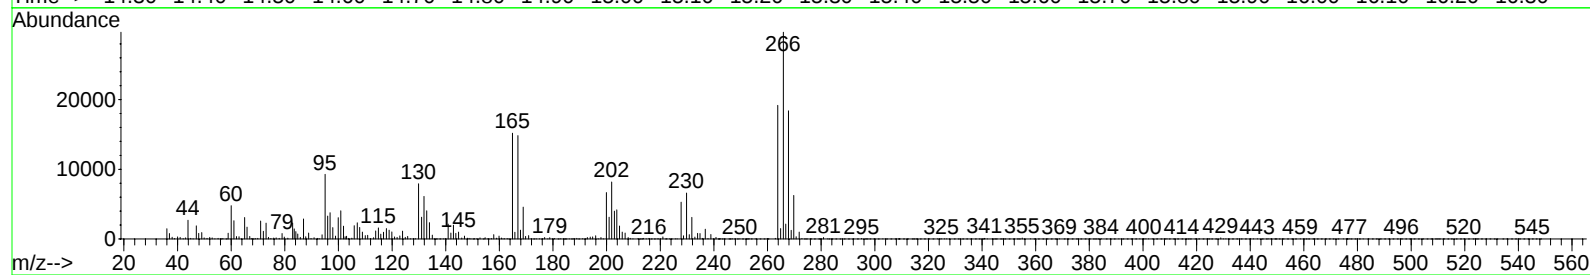


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP120219\
Data File : BP001120.D
Acq On : 02 Dec 2019 11:45
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 02 16:59:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP112719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 27 17:38:46 2019
Response via : Initial Calibration

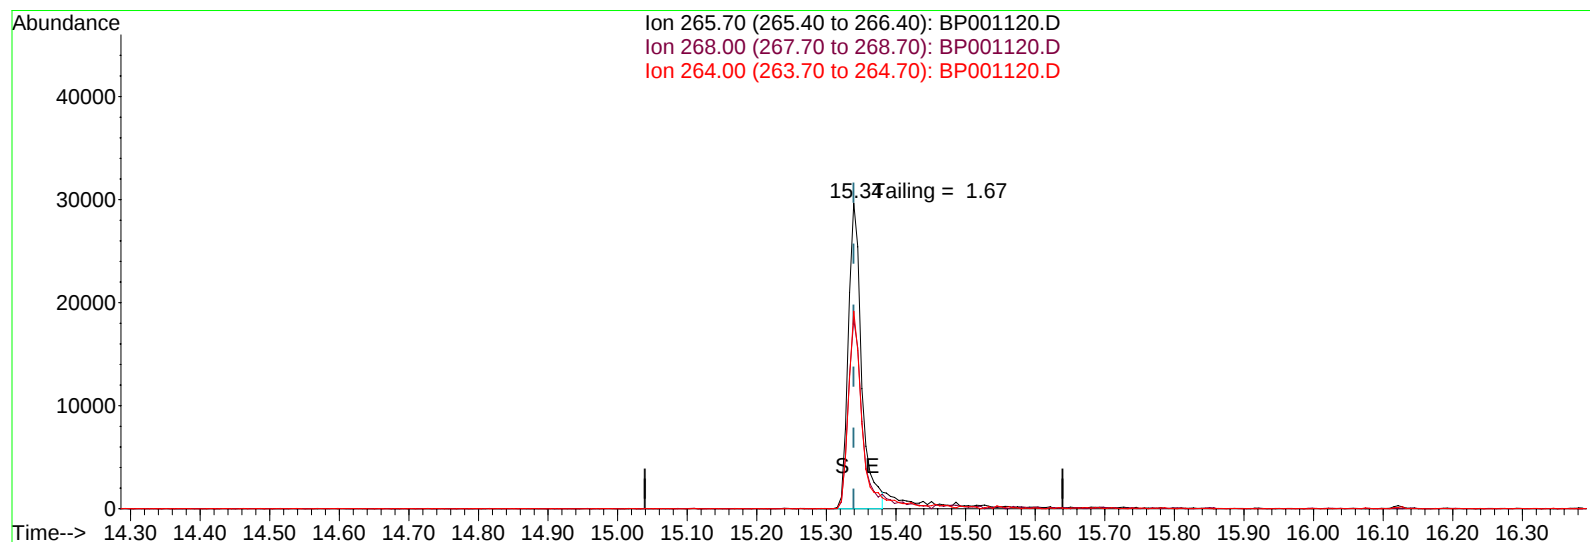

(70) Pentachlorophenol (C)




15.339min (-0.000) 304729.65ng

response 34122

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	62.01
264.00	65.30	64.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP120219\
Data File : BP001120.D
Acq On : 02 Dec 2019 11:45
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 02 16:59:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP112719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 27 17:38:46 2019
Response via : Initial Calibration

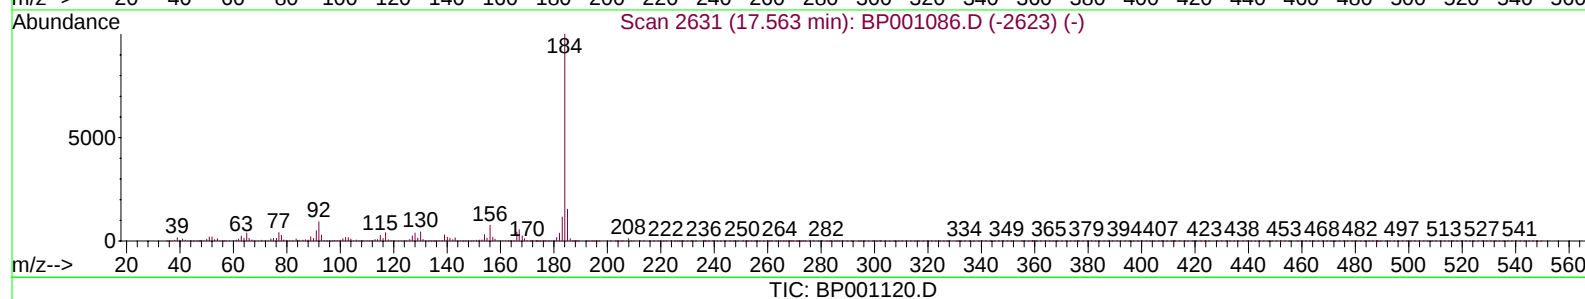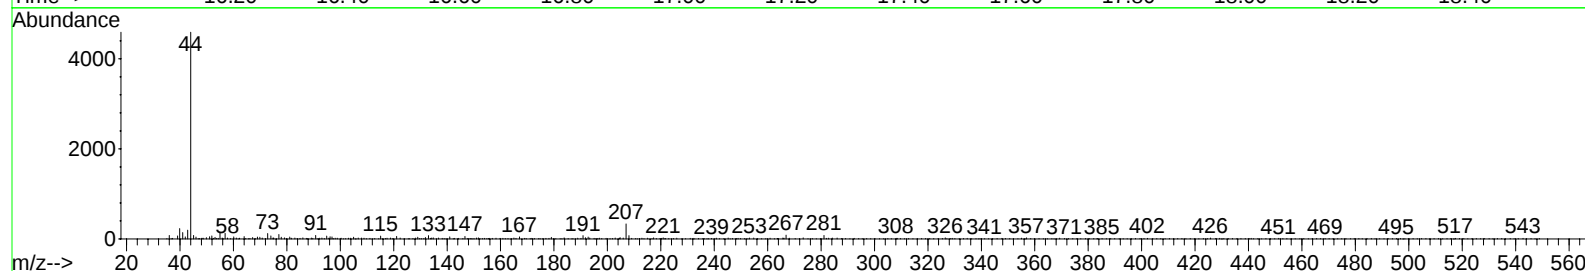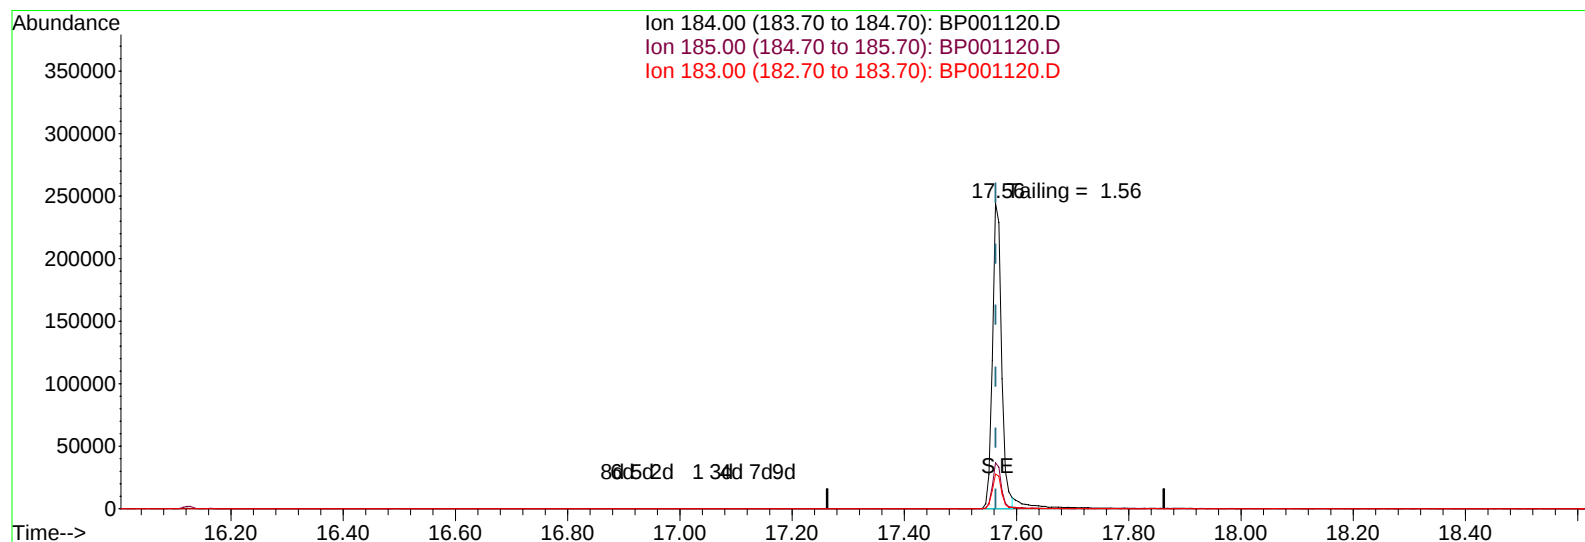

(77) Benzidine

17.033min (-0.529) 0.36ng

response 25

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	34.62#
183.00	11.60	23.08#
0.00	0.00	0.00