


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP120219\
 Data File : BP001120.D
 Acq On : 02 Dec 2019 11:45
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP112719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 27 17:38:46 2019

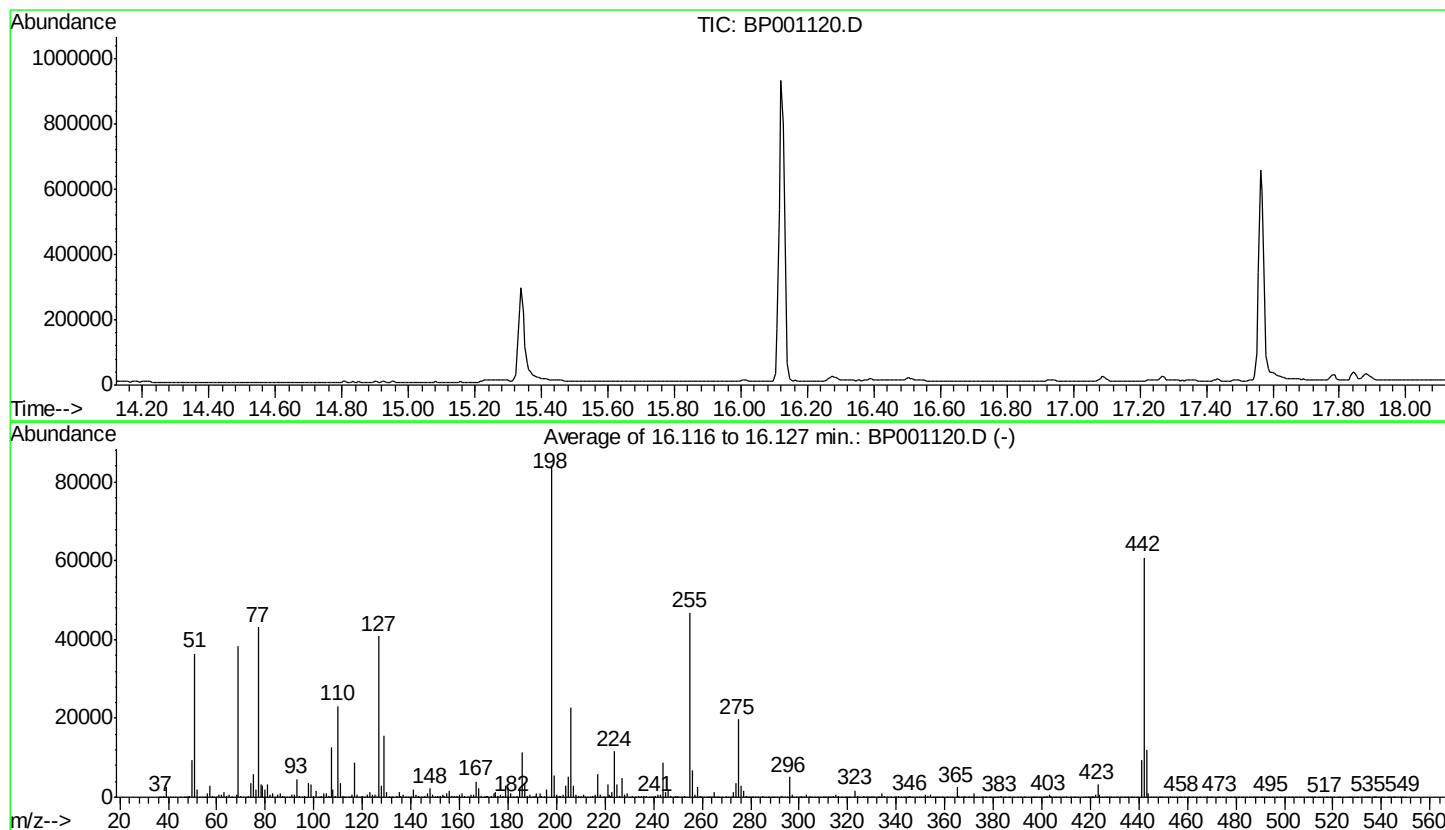

AutoFind: Scans 2385, 2386, 2387; Background Corrected with Scan 2378

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.3	36390	PASS
68	69	0.00	2	2.0	756	PASS
69	198	0.00	100	45.7	38416	PASS
70	69	0.00	2	0.6	238	PASS
127	198	10	80	48.5	40808	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	84136	PASS
199	198	5	9	6.5	5467	PASS
275	198	10	60	23.4	19690	PASS
365	198	1	100	2.9	2450	PASS
441	198	0.01	100	11.3	9537	PASS
442	198	50	100	72.4	60901	PASS
443	442	15	24	19.6	11944	PASS