


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP120219\
 Data File : BP001143.D
 Acq On : 03 Dec 2019 01:16
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP112719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 27 17:38:46 2019

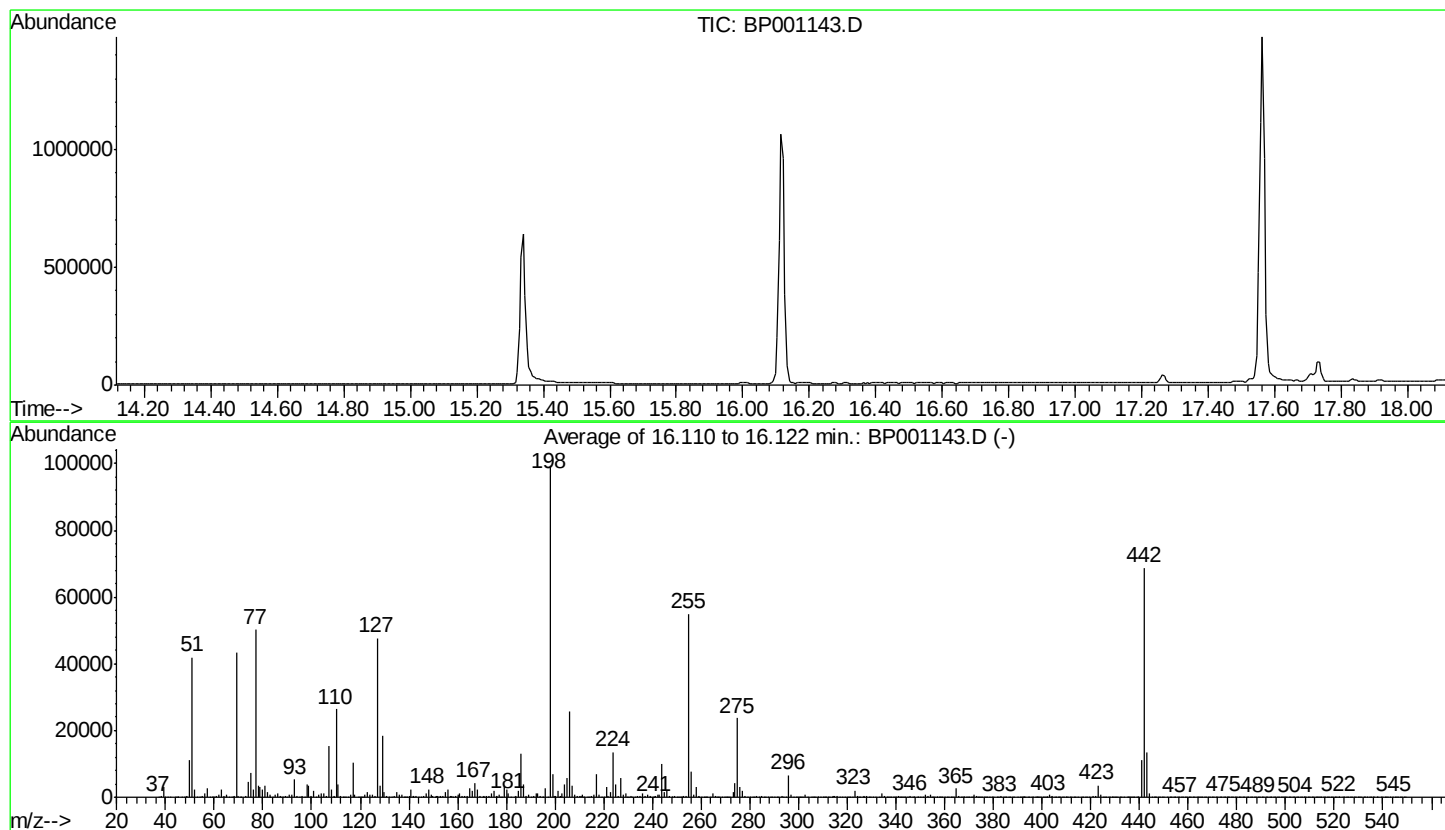

AutoFind: Scans 2384, 2385, 2386; Background Corrected with Scan 2376

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.2	41908	PASS
68	69	0.00	2	1.2	512	PASS
69	198	0.00	100	43.8	43546	PASS
70	69	0.00	2	0.6	255	PASS
127	198	10	80	48.0	47728	PASS
197	198	0.00	2	0.1	138	PASS
198	198	100	100	100.0	99386	PASS
199	198	5	9	7.0	6998	PASS
275	198	10	60	23.8	23690	PASS
365	198	1	100	2.7	2684	PASS
441	198	0.01	100	11.1	11073	PASS
442	198	50	100	69.2	68800	PASS
443	442	15	24	19.8	13608	PASS