
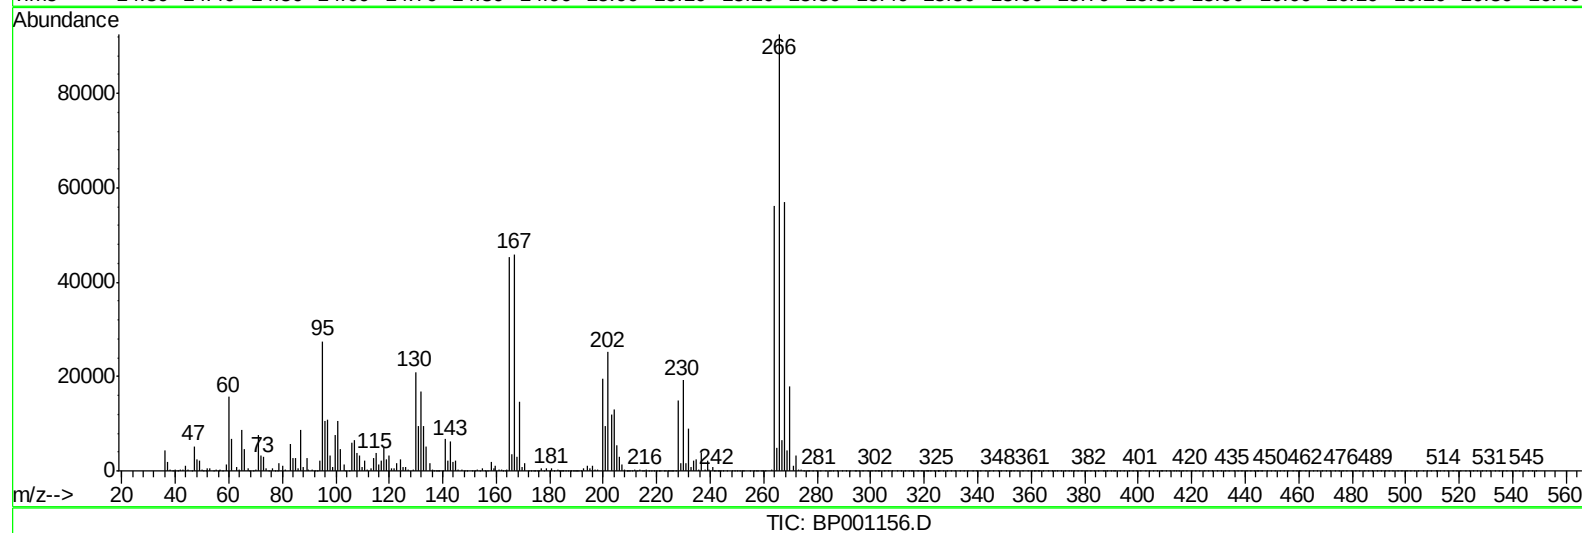


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP120319\
Data File : BP001156.D
Acq On : 03 Dec 2019 15:41
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 04 04:02:35 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP112719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 27 17:38:46 2019
Response via : Initial Calibration

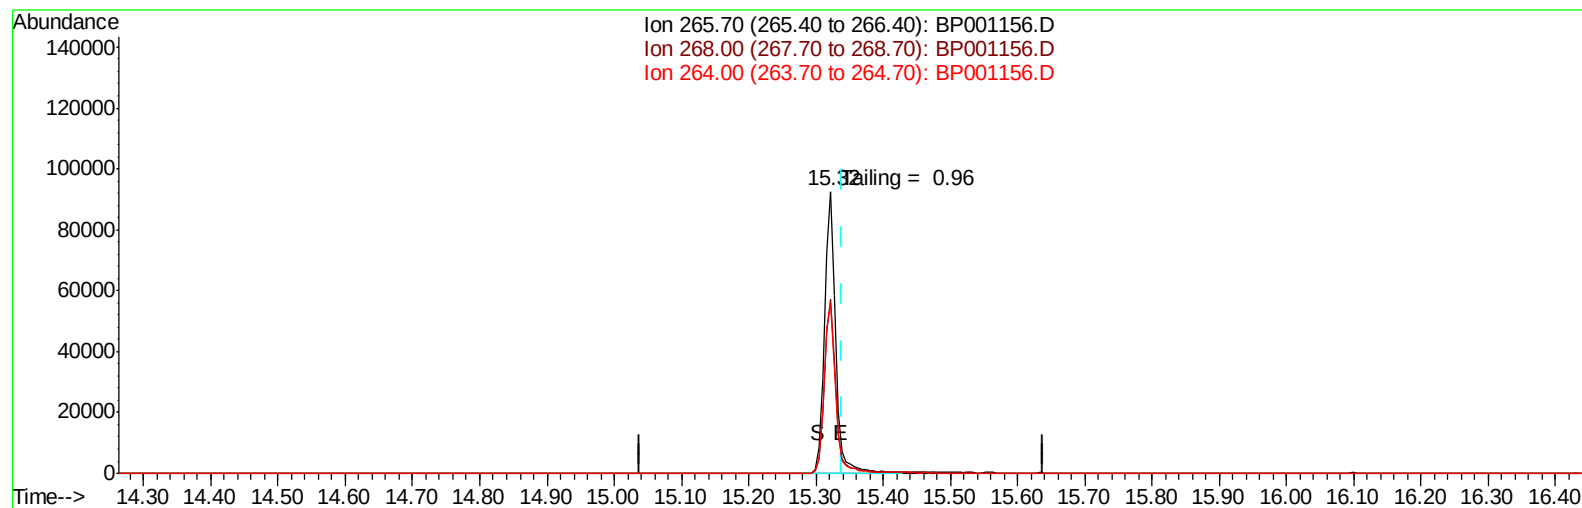

TIC: BP001156.D

(70) Pentachlorophenol (C)



15.322min (-0.017) 840029.33ng

response 109739

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	61.69
264.00	65.30	60.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP120319\
 Data File : BP001156.D
 Acq On : 03 Dec 2019 15:41
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 04 04:02:35 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP112719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 27 17:38:46 2019
 Response via : Initial Calibration

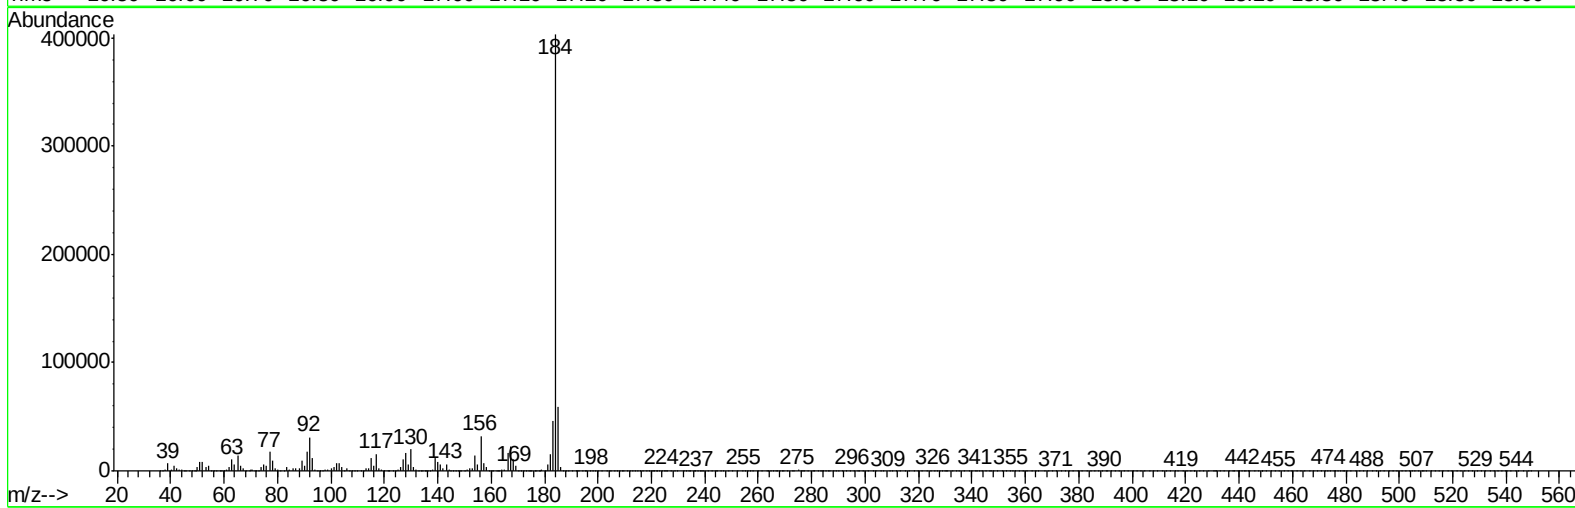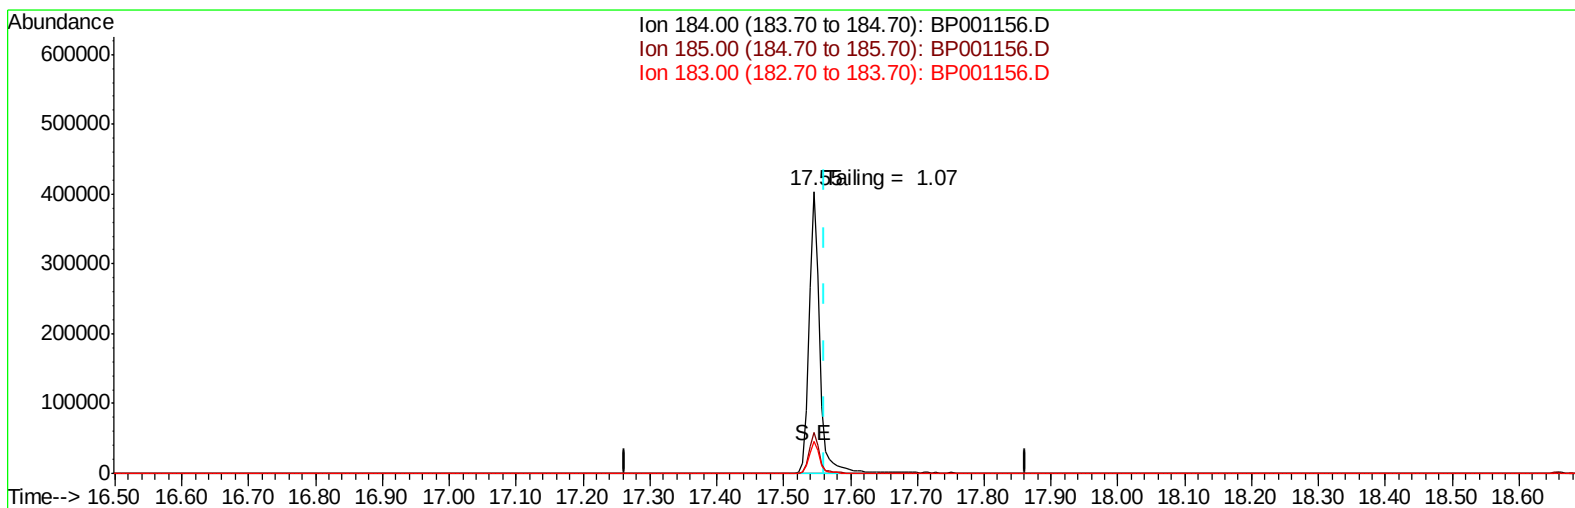

TIC: BP001156.D

(77) Benzidine

17.545min (-0.017) 88230.17ng

response 453329

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	14.57
183.00	11.60	11.53
0.00	0.00	0.00