


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP120319\
 Data File : BP001156.D
 Acq On : 03 Dec 2019 15:41
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP112719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 27 17:38:46 2019

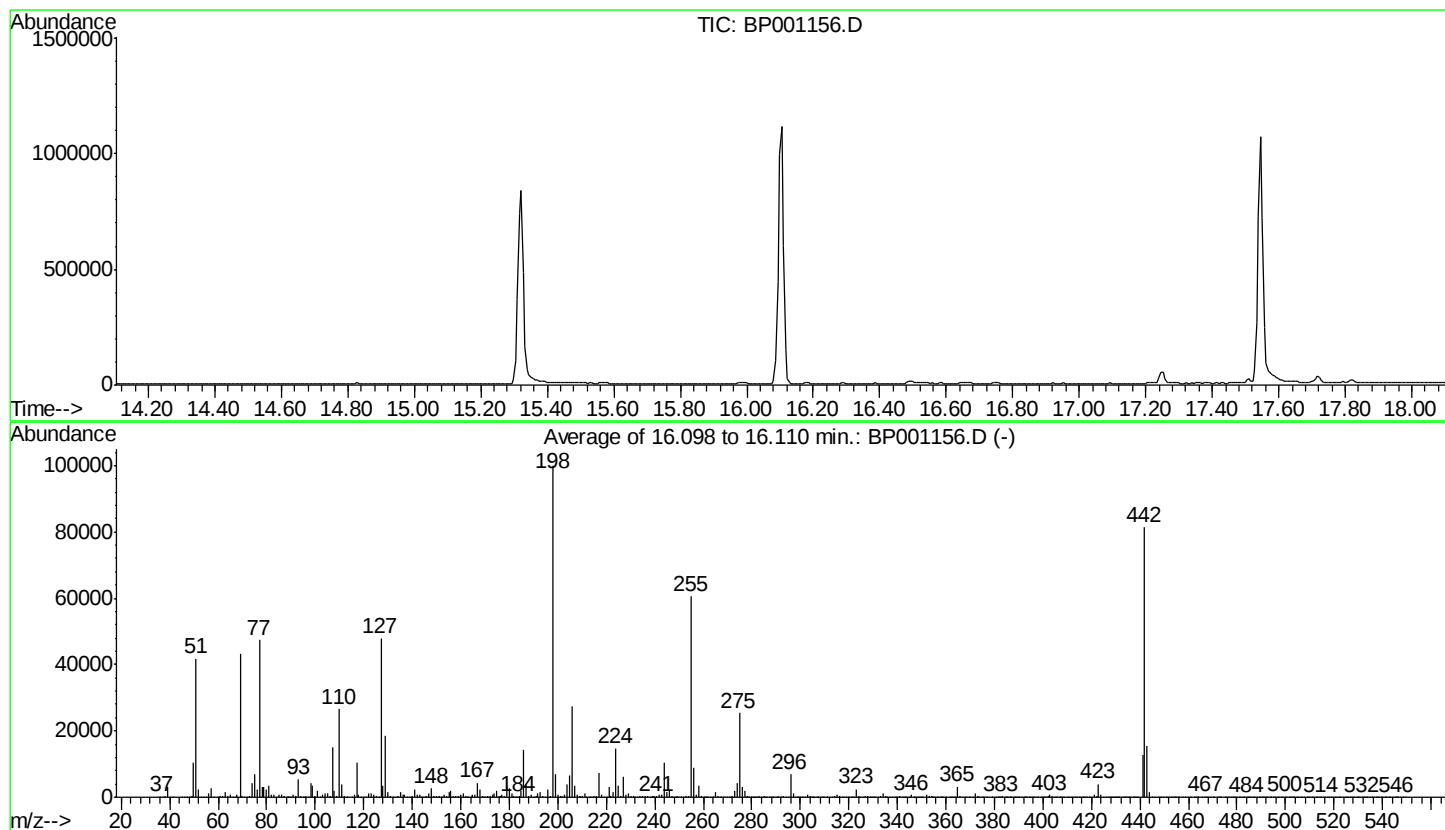

AutoFind: Scans 2382, 2383, 2384; Background Corrected with Scan 2373

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.7	41739	PASS
68	69	0.00	2	1.5	650	PASS
69	198	0.00	100	43.3	43266	PASS
70	69	0.00	2	0.5	222	PASS
127	198	10	80	47.9	47845	PASS
197	198	0.00	2	0.2	221	PASS
198	198	100	100	100.0	99986	PASS
199	198	5	9	6.8	6803	PASS
275	198	10	60	25.3	25338	PASS
365	198	1	100	3.2	3156	PASS
441	198	0.01	100	12.8	12797	PASS
442	198	50	100	81.4	81421	PASS
443	442	15	24	18.8	15275	PASS