

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120320\
 Data File : BP004143.D
 Acq On : 03 Dec 2020 23:07
 Operator : CG/JU
 Sample : L4917-01 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CL-02-12220

Quant Time: Dec 04 00:15:11 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 02 11:39:42 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.193	152	135470	20.00	ng	0.00
21) Naphthalene-d8	11.022	136	469664	20.00	ng	# 0.00
39) Acenaphthene-d10	14.822	164	268229	20.00	ng	0.00
64) Phenanthrene-d10	17.563	188	560321	20.00	ng	# 0.00
76) Chrysene-d12	21.604	240	547369	20.00	ng	0.00
86) Perylene-d12	24.045	264	581988	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.740	112	105326	12.98	ng	0.00
7) Phenol-d6	7.381	99	125354	10.76	ng	0.00
23) Nitrobenzene-d5	9.357	82	75027	7.82	ng	0.00
42) 2,4,6-Tribromophenol	16.310	330	35204	10.49	ng	0.00
45) 2-Fluorobiphenyl	13.445	172	157384	8.20	ng	0.00
79) Terphenyl-d14	20.063	244	200406	7.07	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120320\
Data File : BP004143.D
Acq On : 03 Dec 2020 23:07
Operator : CG/JU
Sample : L4917-01 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CL-02-12220

Quant Time: Dec 04 00:15:11 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 02 11:39:42 2020
Response via : Initial Calibration




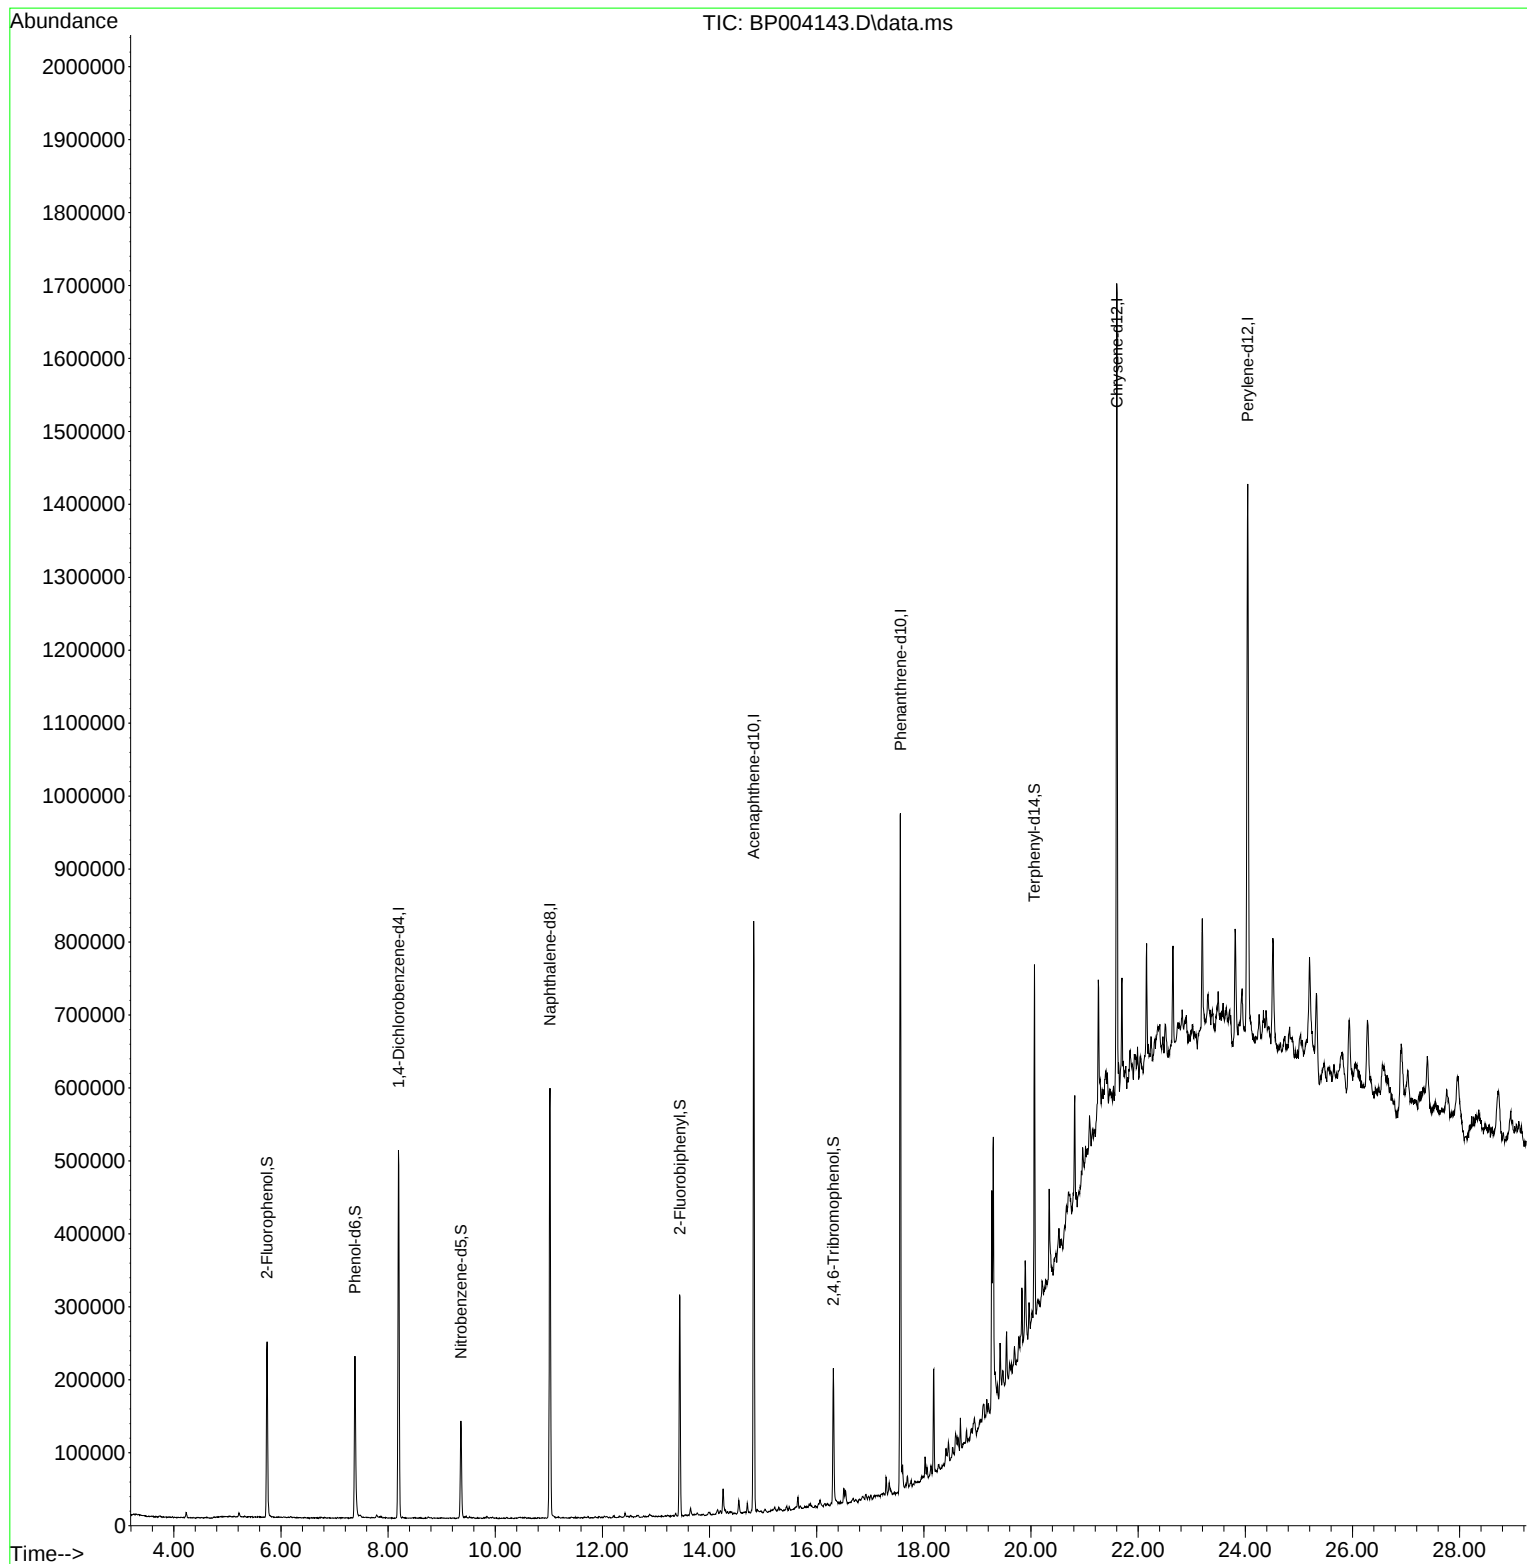




#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.193 min Scan# 851
Delta R.T. -0.000 min
Lab File: BP004143.D
Acq: 03 Dec 2020 23:07




Instrument :
BNA_P
ClientSampleId :
CL-02-12220

Tgt Ion:152 Resp: 135470
Ion Ratio Lower Upper
152 100
150 153.6 123.8 185.6
115 60.7 43.8 65.6

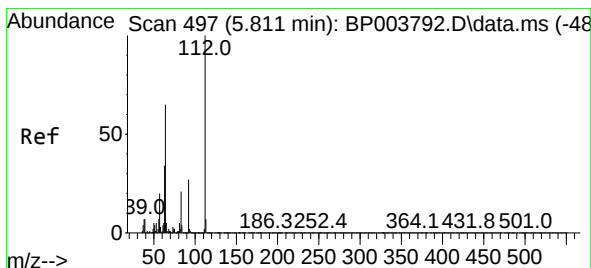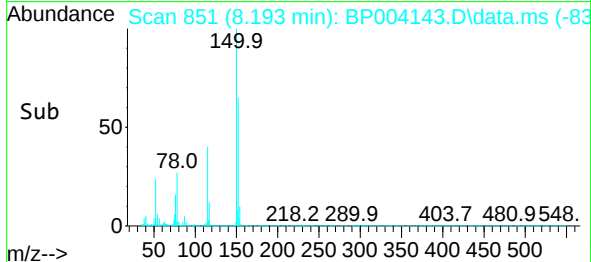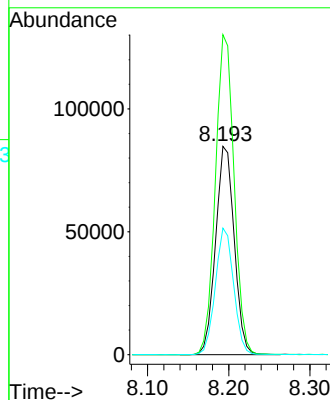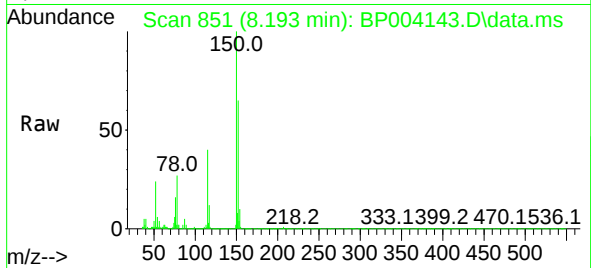

#5
2-Fluorophenol
Concen: 12.98 ng
RT: 5.740 min Scan# 434
Delta R.T. 0.006 min
Lab File: BP004143.D
Acq: 03 Dec 2020 23:07

Tgt Ion:112 Resp: 105326
Ion Ratio Lower Upper
112 100
64 65.7 32.8 49.2#
63 33.4 17.0 25.4#


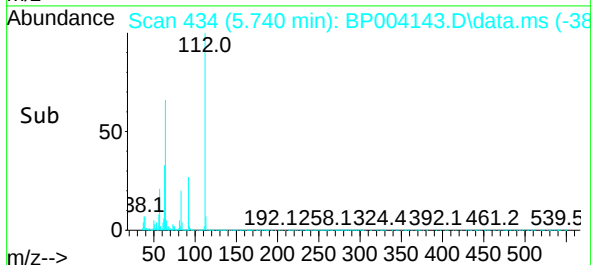
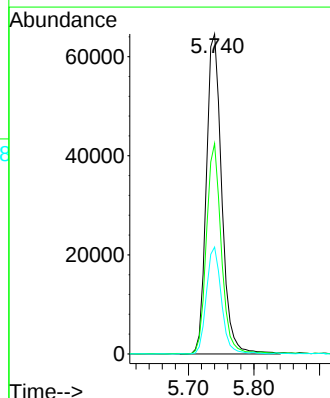
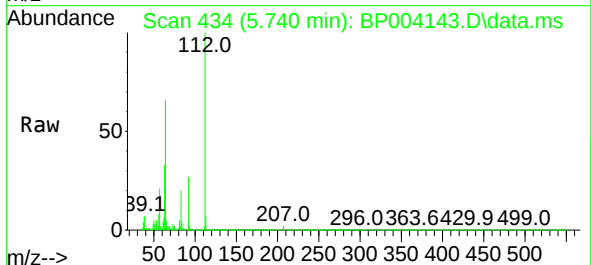




#7
Phenol-d6
Concen: 10.76 ng
RT: 7.381 min Scan# 713
Delta R.T. -0.000 min
Lab File: BP004143.D
Acq: 03 Dec 2020 23:07




Instrument :
BNA_P
ClientSampleId :
CL-02-12220


Tgt Ion: 99 Resp: 125354
Ion Ratio Lower Upper
99 100
42 18.7 8.6 13.0#
71 34.8 23.4 35.2

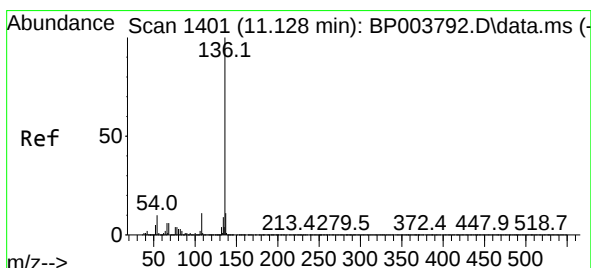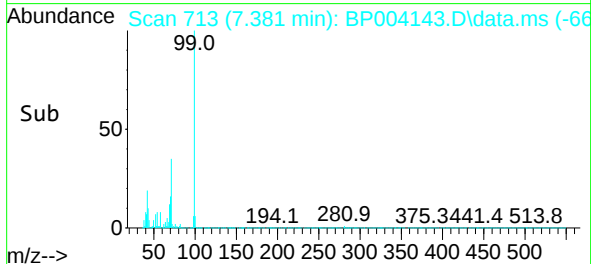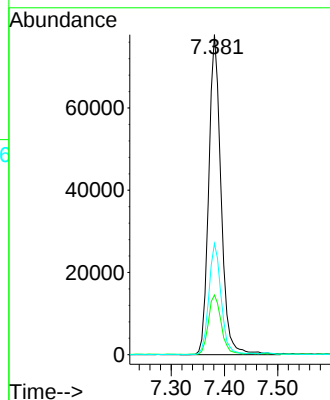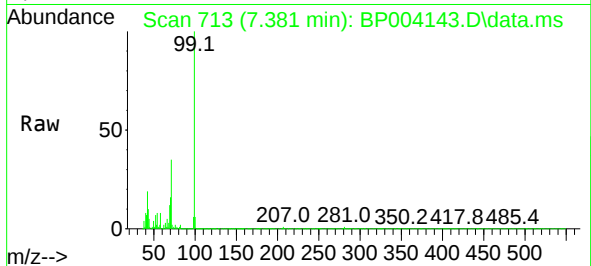

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 11.022 min Scan# 1332
Delta R.T. -0.000 min
Lab File: BP004143.D
Acq: 03 Dec 2020 23:07

Tgt Ion: 136 Resp: 469664
Ion Ratio Lower Upper
136 100
137 10.5 8.6 13.0
54 9.3 3.6 5.4#
68 5.6 3.3 4.9#


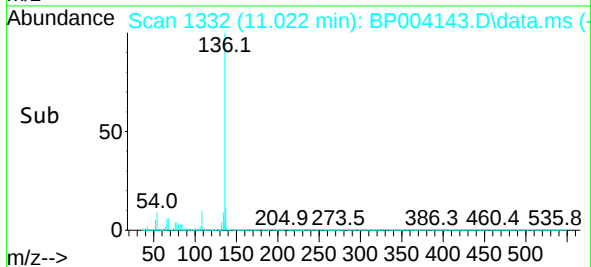
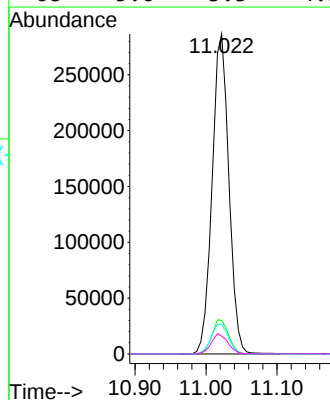
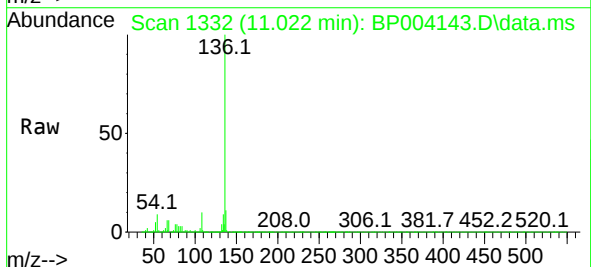


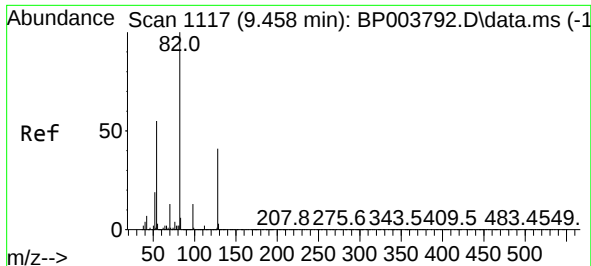

#23
Nitrobenzene-d5
Concen: 7.82 ng
RT: 9.357 min Scan# 1049
Delta R.T. -0.000 min
Lab File: BP004143.D
Acq: 03 Dec 2020 23:07




Instrument :
BNA_P
ClientSampleId :
CL-02-12220


Tgt Ion: 82 Resp: 75027
Ion Ratio Lower Upper
82 100
128 40.5 45.6 68.4#
54 53.3 30.1 45.1#

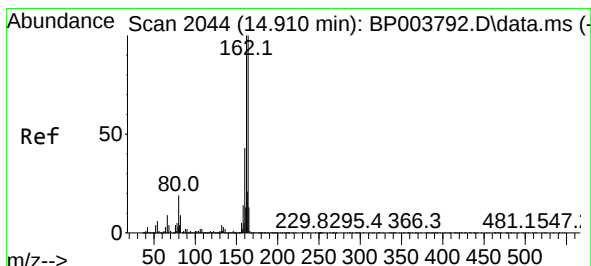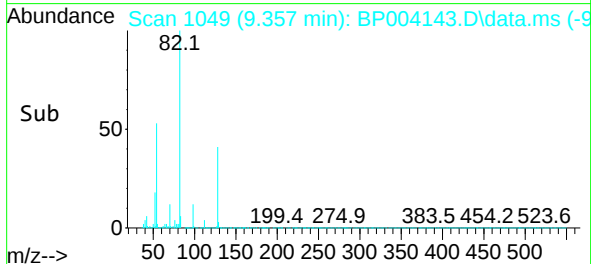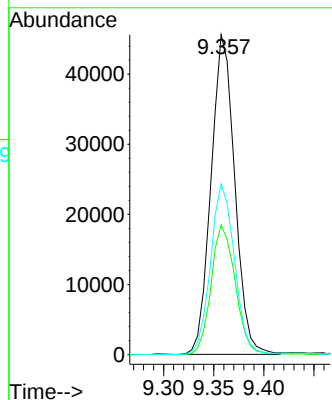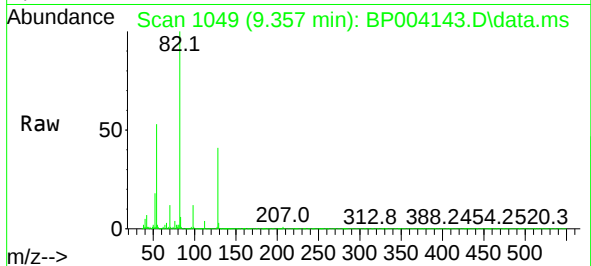

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.822 min Scan# 1978
Delta R.T. -0.006 min
Lab File: BP004143.D
Acq: 03 Dec 2020 23:07

Tgt Ion: 164 Resp: 268229
Ion Ratio Lower Upper
164 100
162 100.5 79.4 119.2
160 42.5 36.1 54.1


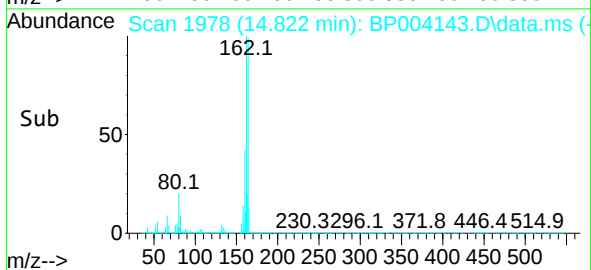
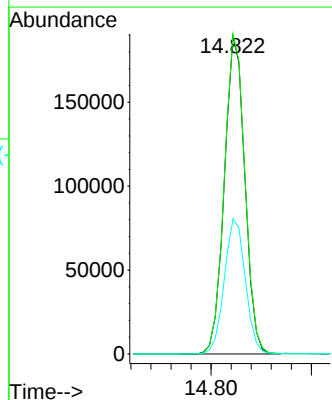
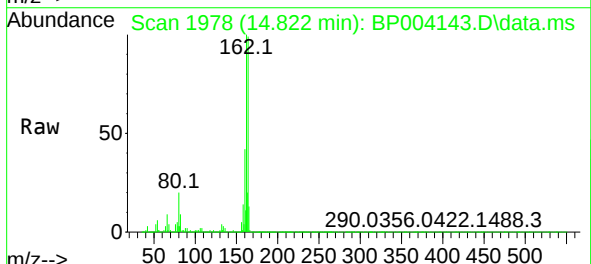


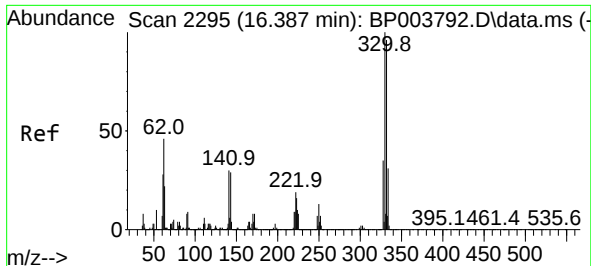

#42
2,4,6-Tribromophenol
Concen: 10.49 ng
RT: 16.310 min Scan# 2231
Delta R.T. -0.000 min
Lab File: BP004143.D
Acq: 03 Dec 2020 23:07




Instrument :
BNA_P
ClientSampleId :
CL-02-12220


Tgt Ion: 330 Resp: 35204
Ion Ratio Lower Upper
330 100
332 97.3 77.1 115.7
141 33.9 23.4 35.2

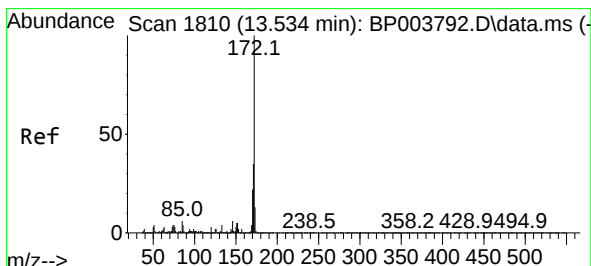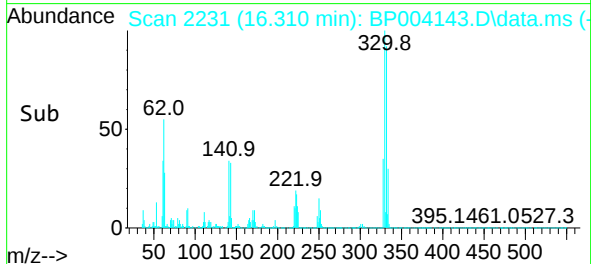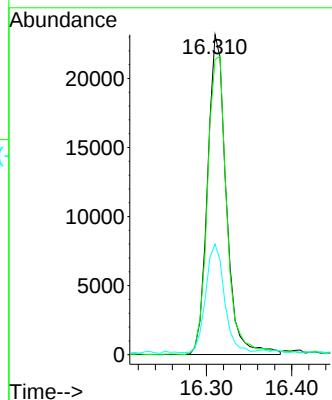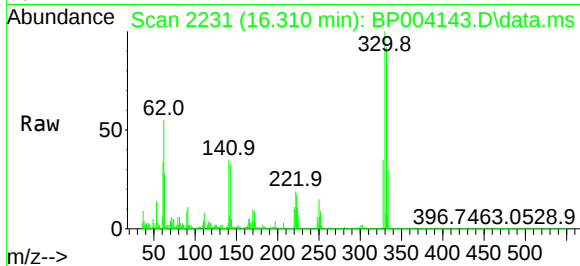

#45
2-Fluorobiphenyl
Concen: 8.20 ng
RT: 13.445 min Scan# 1744
Delta R.T. -0.000 min
Lab File: BP004143.D
Acq: 03 Dec 2020 23:07

Tgt Ion: 172 Resp: 157384
Ion Ratio Lower Upper
172 100
171 35.2 28.5 42.7
170 22.5 19.2 28.8


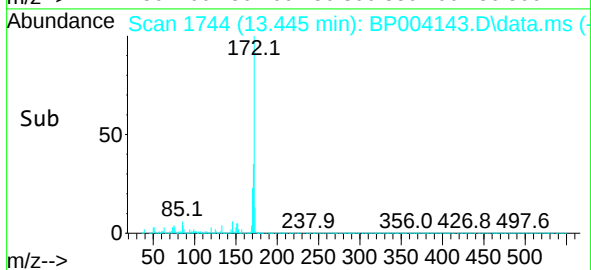
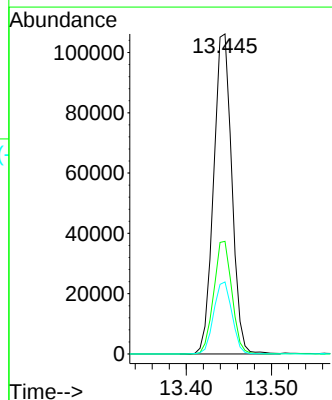
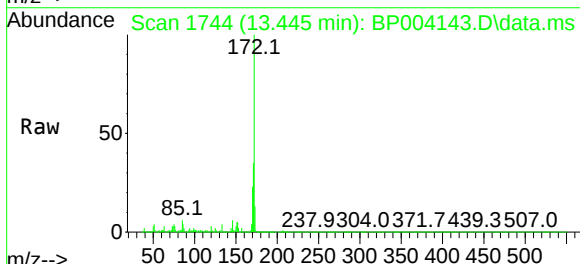


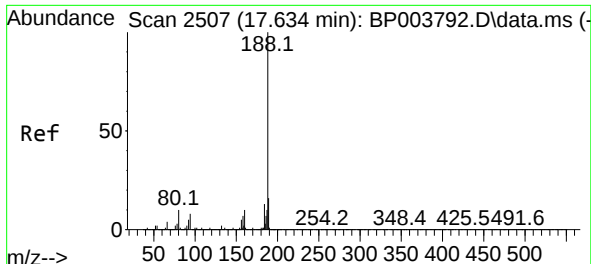

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.563 min Scan# 2444
Delta R.T. -0.000 min
Lab File: BP004143.D
Acq: 03 Dec 2020 23:07




Instrument :
BNA_P
ClientSampleId :
CL-02-12220


Tgt Ion:188 Resp: 560321
Ion Ratio Lower Upper
188 100
94 8.2 6.2 9.2
80 9.3 6.2 9.2#

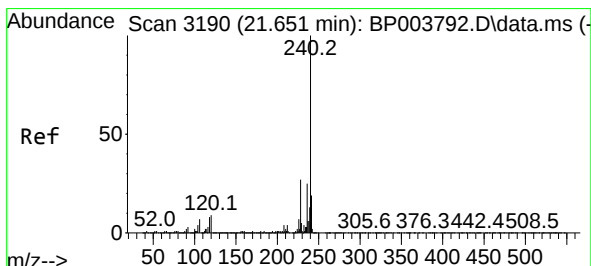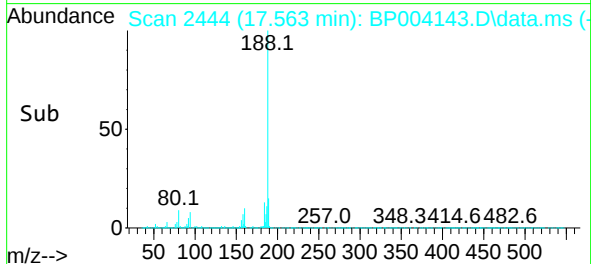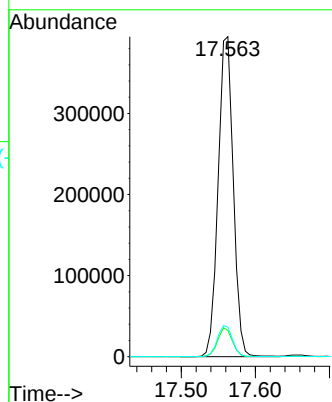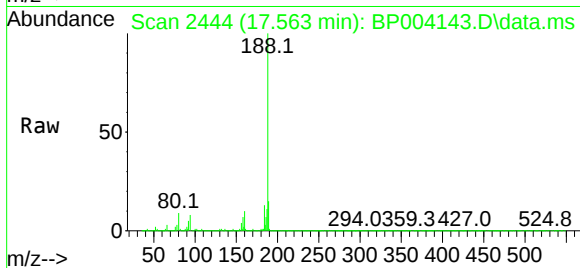

#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.604 min Scan# 3131
Delta R.T. 0.006 min
Lab File: BP004143.D
Acq: 03 Dec 2020 23:07

Tgt Ion:240 Resp: 547369
Ion Ratio Lower Upper
240 100
120 9.3 7.8 11.6
236 25.5 20.8 31.2


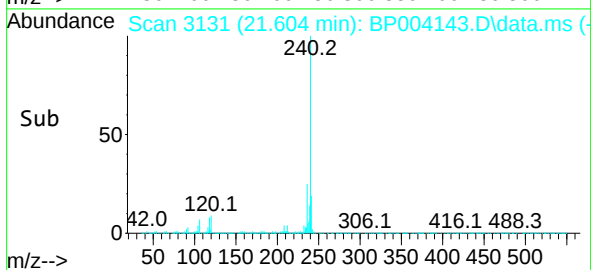
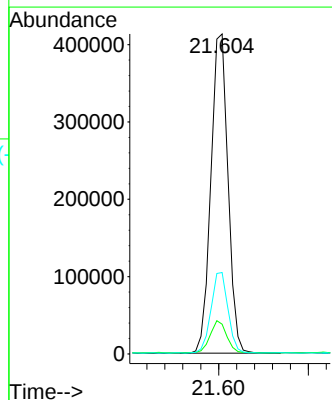
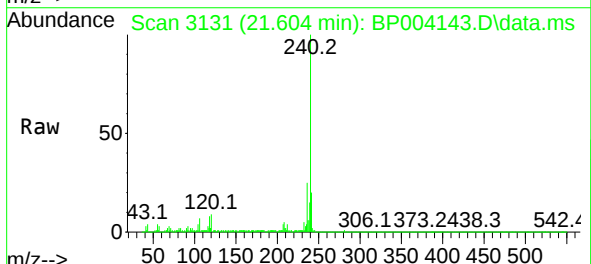


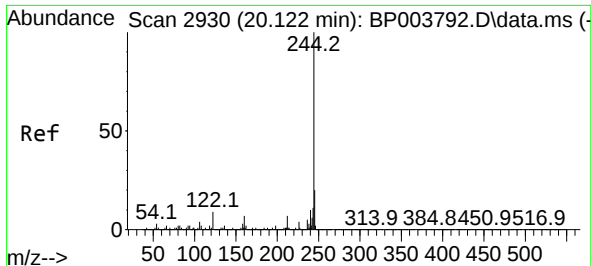

#79
Terphenyl-d14
Concen: 7.07 ng
RT: 20.063 min Scan# 2869
Delta R.T. -0.006 min
Lab File: BP004143.D
Acq: 03 Dec 2020 23:07

Instrument :
BNA_P
ClientSampleId :
CL-02-12220

Tgt Ion:244 Resp: 200406
Ion Ratio Lower Upper
244 100
212 7.5 5.8 8.6
122 10.2 7.8 11.8

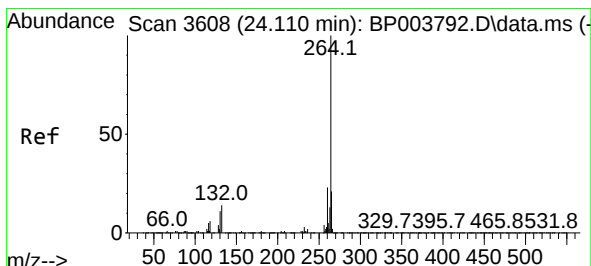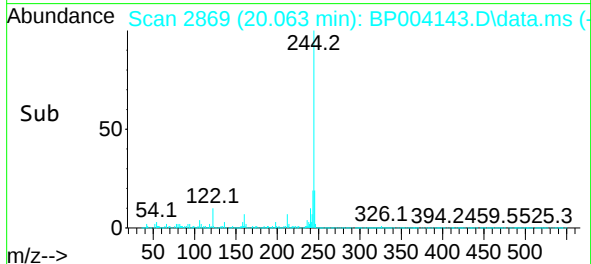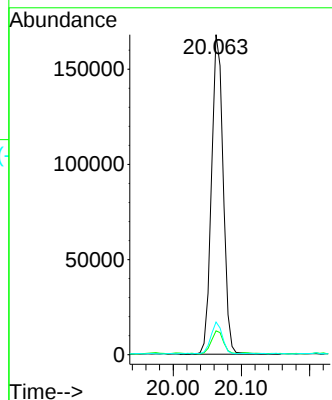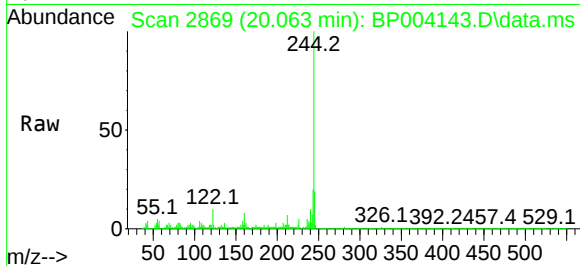

#86
Perylene-d12
Concen: 20.00 ng
RT: 24.045 min Scan# 3546
Delta R.T. 0.006 min
Lab File: BP004143.D
Acq: 03 Dec 2020 23:07

Tgt Ion:264 Resp: 581988
Ion Ratio Lower Upper
264 100
260 22.9 18.8 28.2
265 21.9 17.4 26.2

