

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120320\
 Data File : BP004142.D
 Acq On : 03 Dec 2020 22:33
 Operator : CG/JU
 Sample : L4916-01 2X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 OK-01-12220

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP004142.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.228	173	177	183	rBV	13714	20260	1.00%	0.110%
2	5.211	340	344	350	rBV	21521	33205	1.65%	0.180%
3	5.734	426	433	452	rBV	907016	1390553	68.96%	7.549%
4	7.381	706	713	727	rVB	801973	1328004	65.86%	7.210%
5	7.775	774	780	788	rBV	36655	61854	3.07%	0.336%
6	8.193	844	851	859	rVB	585087	903925	44.83%	4.907%
7	9.357	1033	1049	1059	rBV	511619	862524	42.77%	4.683%
8	11.016	1323	1331	1340	rBV	648435	1104828	54.79%	5.998%
9	13.440	1737	1743	1751	rBV	1085376	1579169	78.31%	8.573%
10	13.710	1783	1789	1795	rBV	225911	331355	16.43%	1.799%
11	14.251	1876	1881	1887	rBV	108774	166115	8.24%	0.902%
12	14.545	1925	1931	1943	rBV	59925	96303	4.78%	0.523%
13	14.822	1971	1978	1985	rBV	904342	1294411	64.19%	7.027%
14	15.928	2162	2166	2172	rBV2	18413	29072	1.44%	0.158%
15	16.310	2225	2231	2245	rBV	731589	1078707	53.50%	5.856%
16	16.533	2266	2269	2275	rVB4	20335	31195	1.55%	0.169%
17	17.351	2404	2408	2412	rBV2	15934	23541	1.17%	0.128%
18	17.557	2437	2443	2448	rBV	1035318	1479004	73.35%	8.029%
19	17.598	2448	2450	2457	rVB	58900	81202	4.03%	0.441%
20	17.692	2462	2466	2471	rVB	42947	60299	2.99%	0.327%
21	18.410	2585	2588	2591	rBV	21794	27245	1.35%	0.148%
22	18.457	2593	2596	2601	rVB2	31827	44454	2.20%	0.241%
23	18.598	2616	2620	2624	rBV2	28160	54187	2.69%	0.294%
24	19.286	2733	2737	2742	rBV2	48643	74596	3.70%	0.405%
25	19.539	2776	2780	2786	rVB	265511	355302	17.62%	1.929%
26	19.686	2803	2805	2810	rVB	39359	39322	1.95%	0.213%
27	19.892	2836	2840	2847	rVB	312606	419378	20.80%	2.277%
28	20.063	2864	2869	2875	rBV	1729724	2004109	99.39%	10.880%
29	21.598	3124	3130	3134	rBV2	1323936	2016455	100.00%	10.947%
30	24.045	3540	3546	3553	rBV	749492	1429385	70.89%	7.760%




Sum of corrected areas: 18419959

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120320\
Data File : BP004142.D
Acq On : 03 Dec 2020 22:33
Operator : CG/JU
Sample : L4916-01 2X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OK-01-12220

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

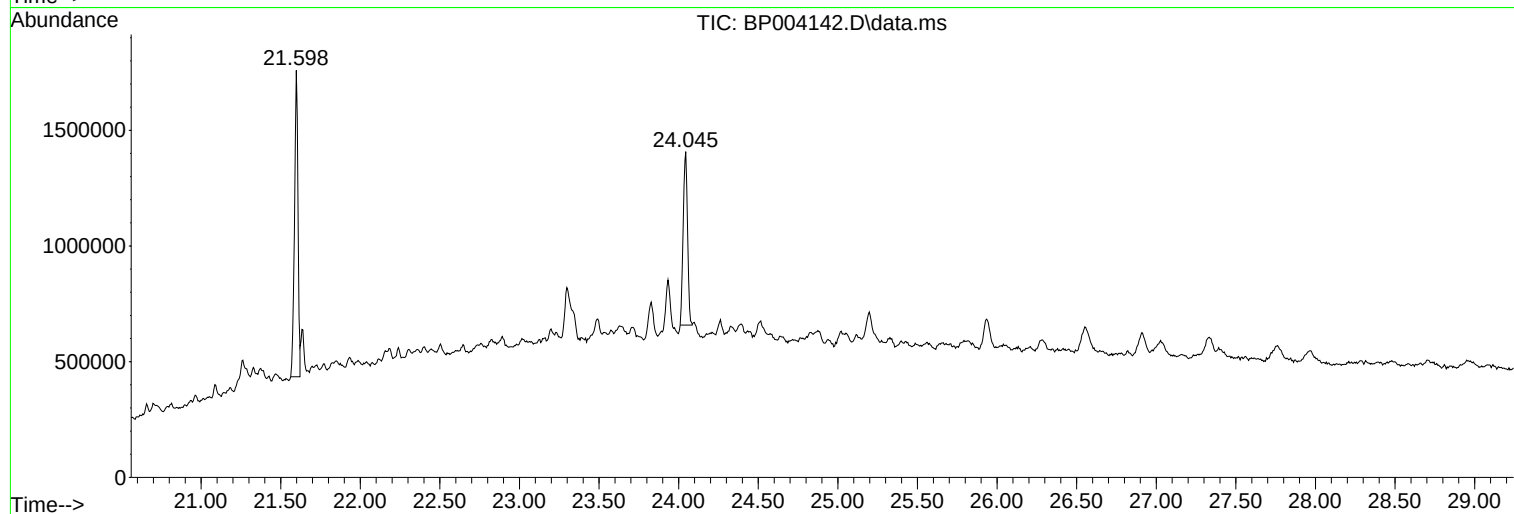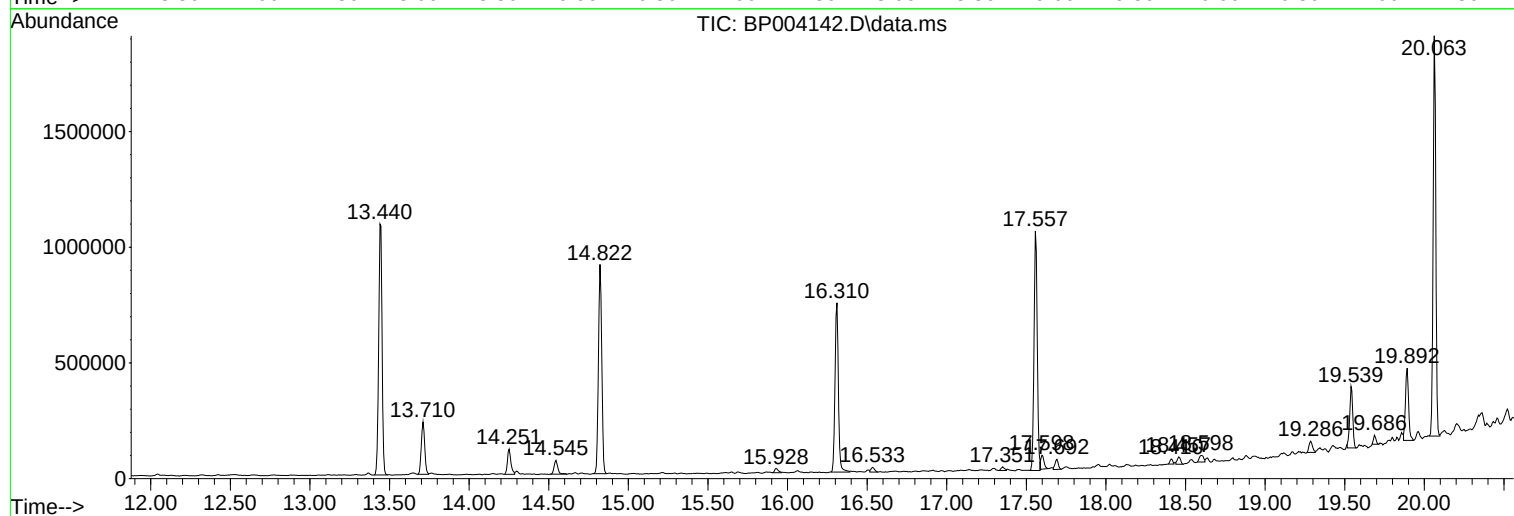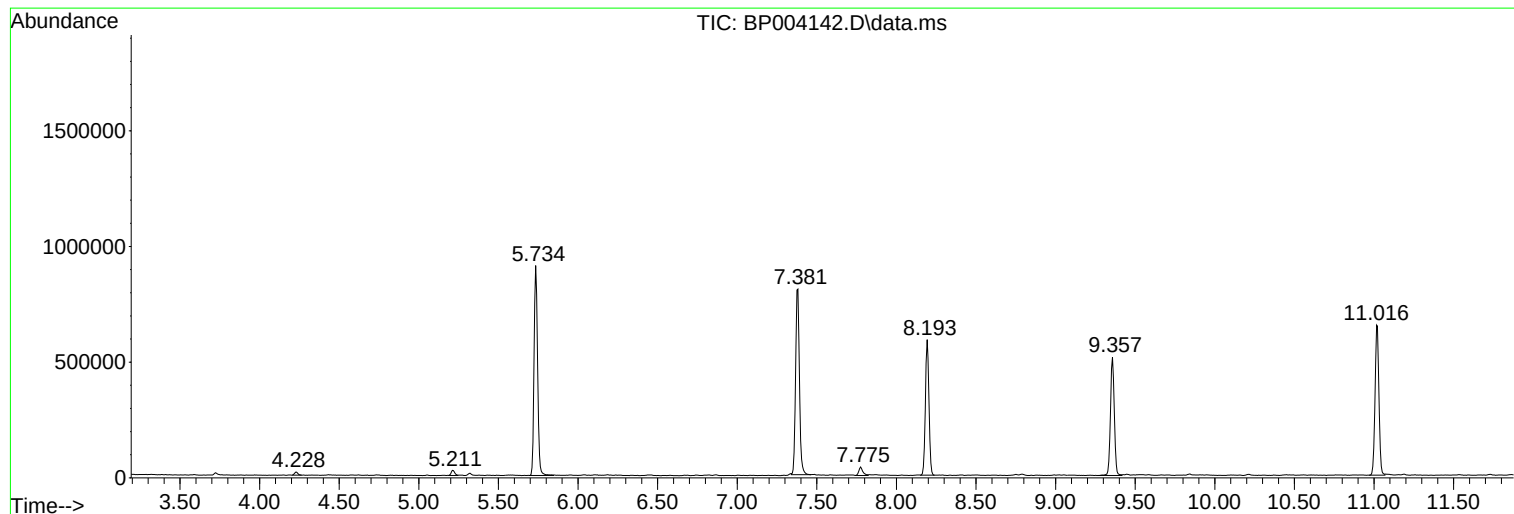

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120320\
Data File : BP004142.D
Acq On : 03 Dec 2020 22:33
Operator : CG/JU
Sample : L4916-01 2X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OK-01-12220










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2,4,7,9-Tetramethyl-5-decyn... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.710	5.12 ng	331355	Acenaphthene-d10	14.822

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2,4,7,9-Tetramethyl-5-decyn-4,7-...	226	C14H26O2	000126-86-3	90		
2	m-Isopropoxyaniline	151	C9H13NO	041406-00-2	50		
3	Butanamide, N-acetyl-N-(4-hydrox...	221	C12H15NO3	1000107-08-7	33		
4	Pyridine, 3-butyl-, 1-oxide	151	C9H13NO	031396-33-5	33		
5	Cyclohexanol, 3,3,5-trimethyl-, ...	142	C9H18O	000767-54-4	32		

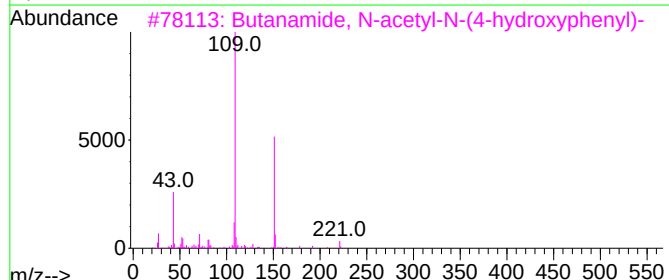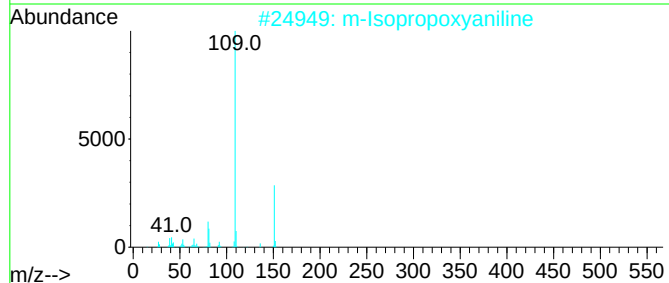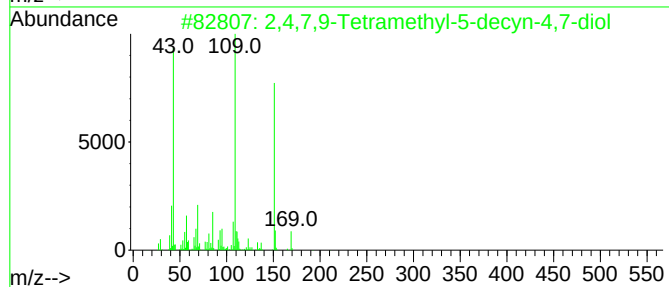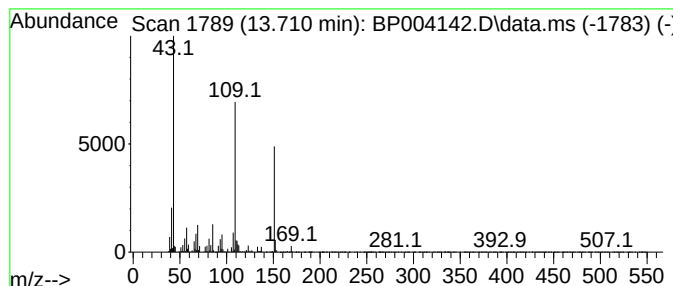

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120320\
Data File : BP004142.D
Acq On : 03 Dec 2020 22:33
Operator : CG/JU
Sample : L4916-01 2X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OK-01-12220

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2,4,7,9-Tetrame...	13.710	5.1	ng	331355	3	14.822	1294410	20.0