
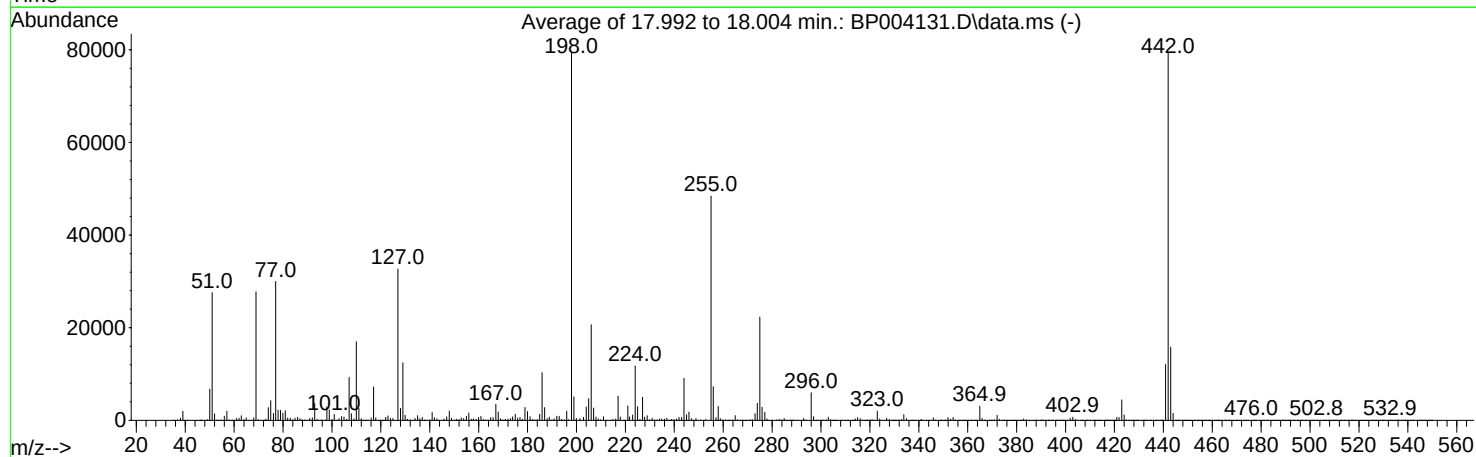


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120320\
Data File : BP004131.D
Acq On : 03 Dec 2020 16:14
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270E-BP110320.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Dec 02 11:39:42 2020

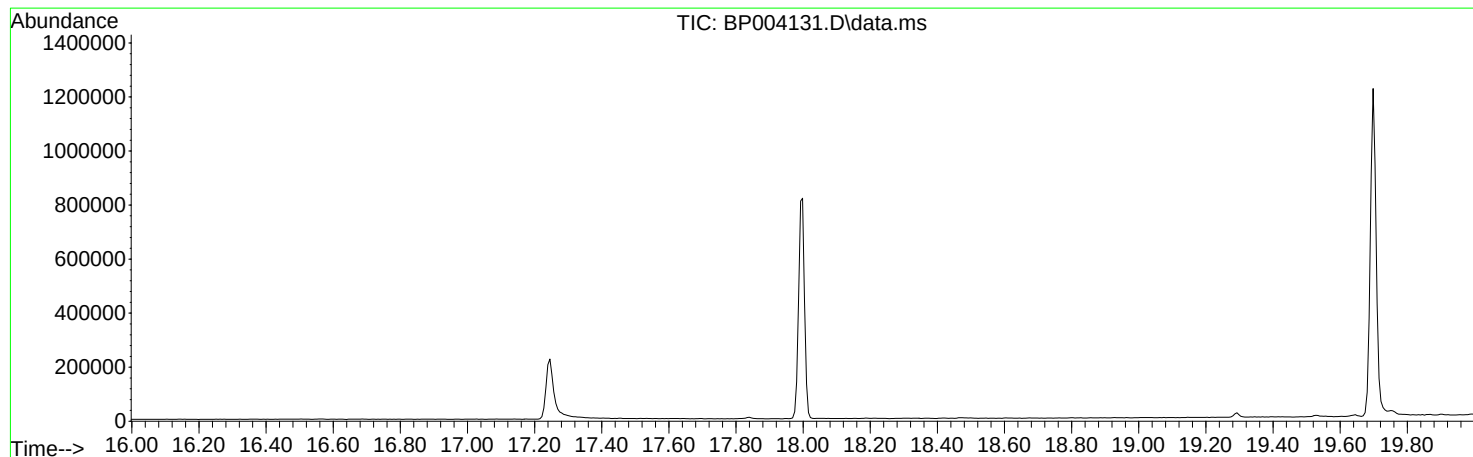

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2509

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	27606	PASS
68	69	0.00	2	1.9	519	PASS
69	198	0.00	100	35.0	27786	PASS
70	69	0.00	2	0.5	140	PASS
127	198	10	80	41.2	32673	PASS
197	198	0.00	2	0.2	125	PASS
198	198	100	100	100.0	79310	PASS
199	198	5	9	6.4	5075	PASS
275	198	10	60	28.1	22272	PASS
365	198	1	100	3.8	3045	PASS
441	198	0.01	100	15.2	12075	PASS
442	442	100	100	100.0	79421	PASS
443	442	15	24	19.9	15828	PASS