


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120321\
 Data File : BP008202.D
 Acq On : 03 Dec 2021 12:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 03 14:39:24 2021

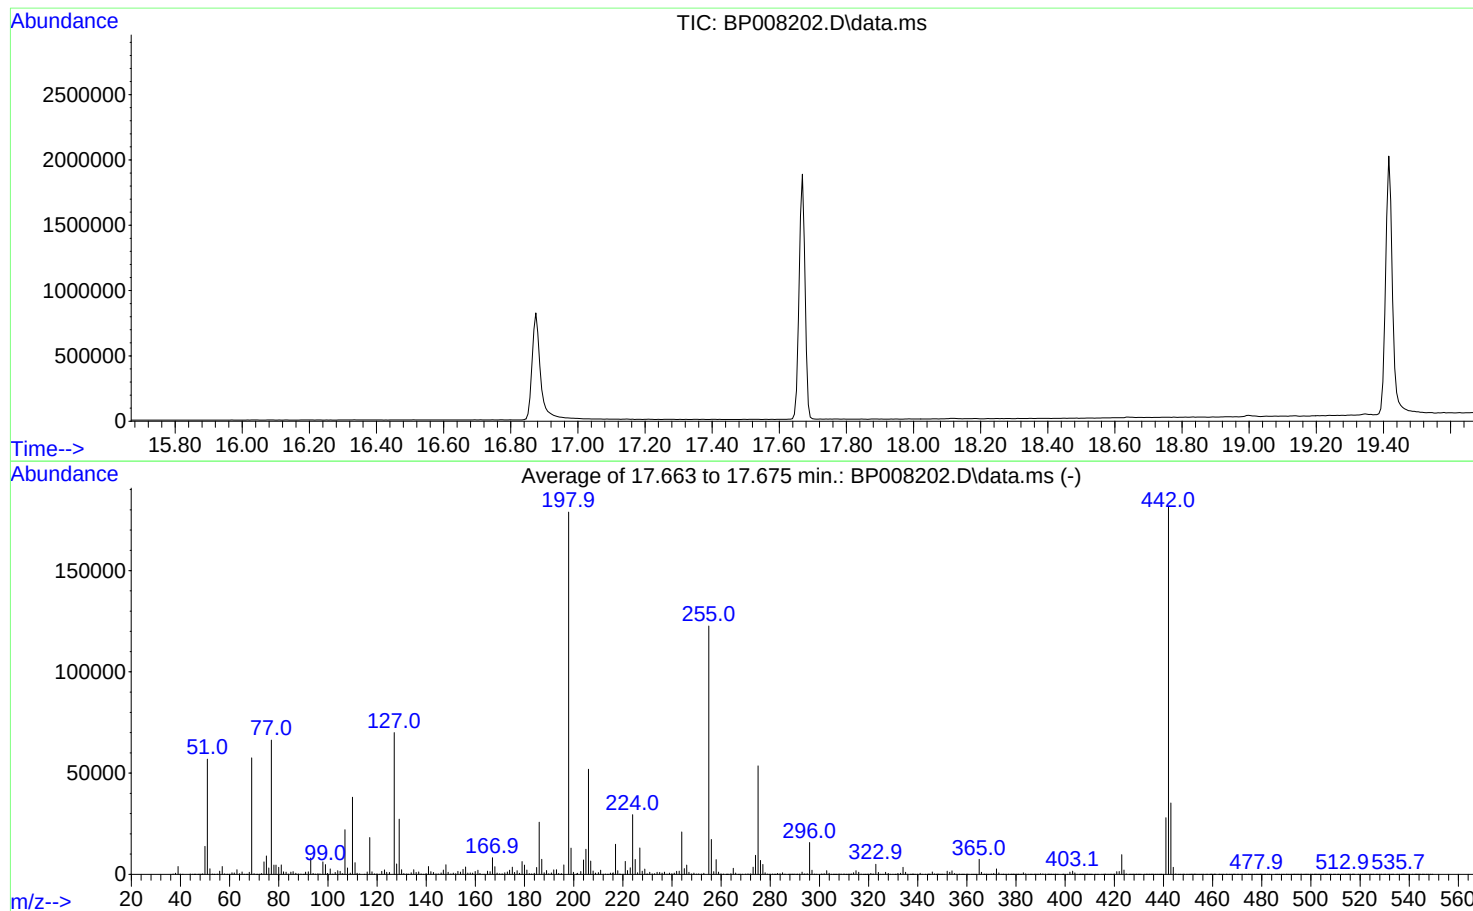


AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.8	56863	PASS
68	69	0.00	2	1.8	1027	PASS
69	198	0.00	100	32.1	57488	PASS
70	69	0.00	2	0.5	308	PASS
127	198	10	80	39.1	70020	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	178923	PASS
199	198	5	9	7.3	12996	PASS
275	198	10	60	29.9	53568	PASS
365	198	1	100	4.1	7397	PASS
441	198	0.01	100	15.6	27972	PASS
442	442	100	100	100.0	181653	PASS
443	442	15	24	19.4	35224	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120321\
Data File : BP008202.D
Acq On : 03 Dec 2021 12:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Dec 03 13:22:18 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 01 12:06:05 2021
Response via : Initial Calibration

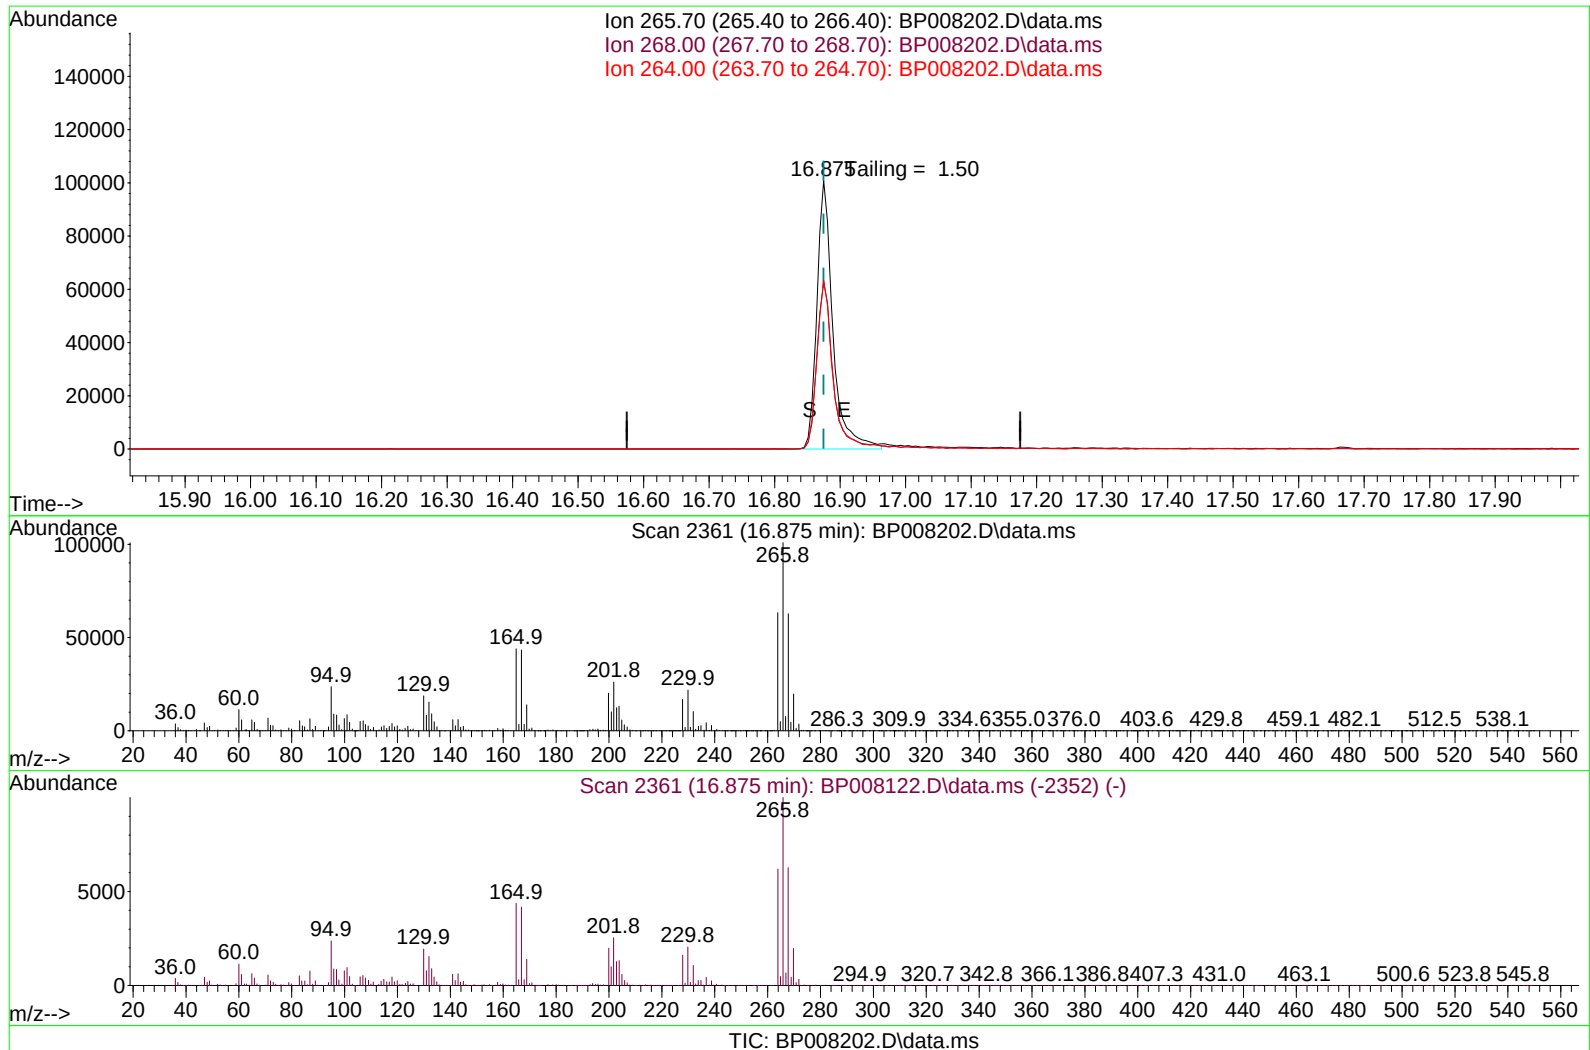

(70) Pentachlorophenol (C)

16.875min (-0.000) 382935.49 ng




response 175930

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	62.19
264.00	61.90	62.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120321\
 Data File : BP008202.D
 Acq On : 03 Dec 2021 12:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Dec 03 13:22:18 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP112521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 01 12:06:05 2021
 Response via : Initial Calibration

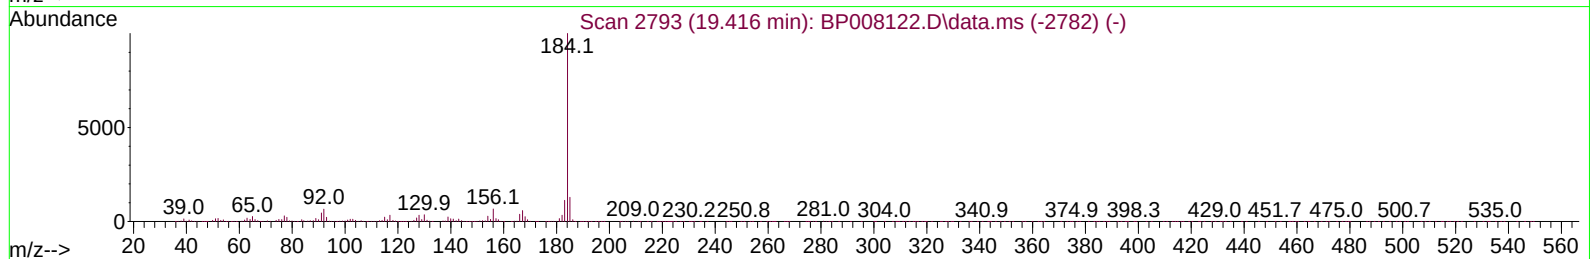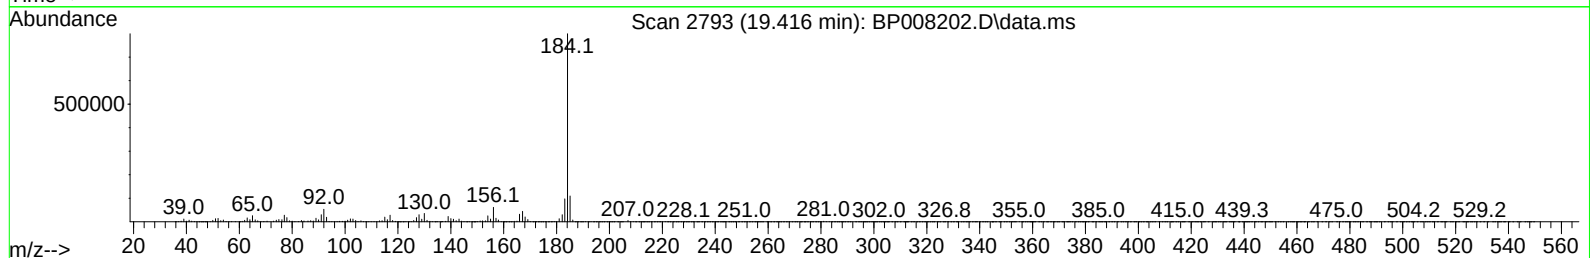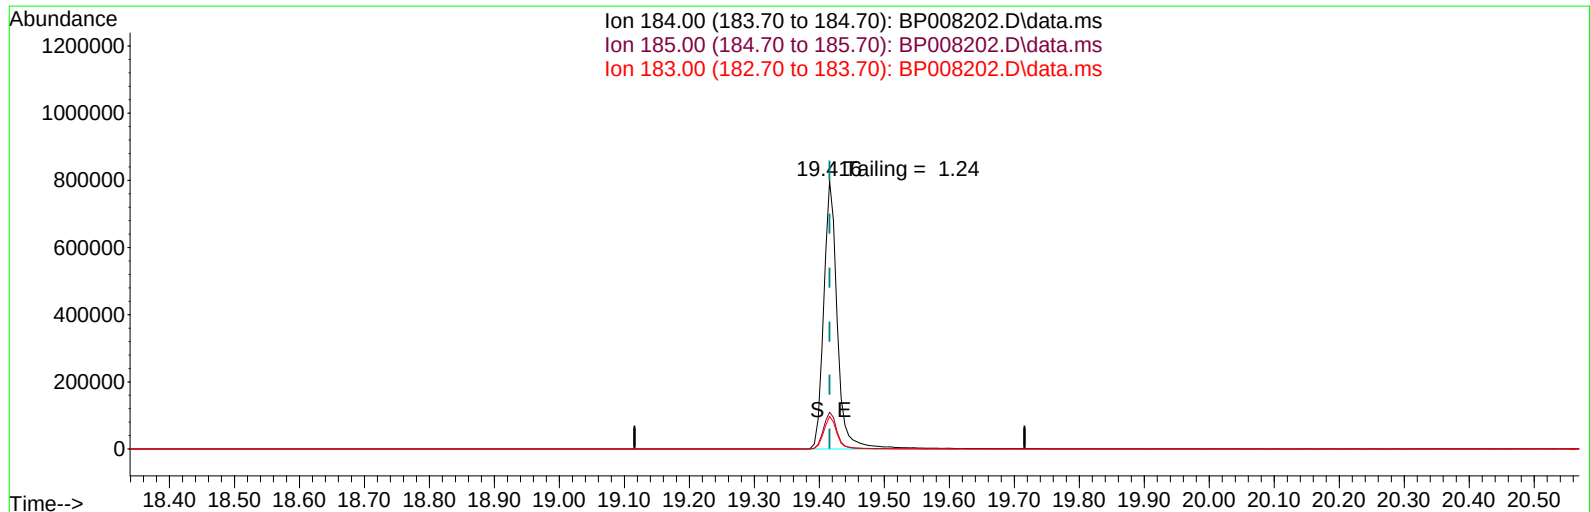

TIC: BP008202.D\data.ms

(77) Benzidine

19.416min (-0.000) 43819.33 ng

response 1158280

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	12.90	13.71
183.00	11.40	12.15
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/3/2021	BNA_P	BP008202.D
Compound Name	Response	Retention Time
DDT	649116	20.62
DDD	7100	20.19
DDE	1355	19.69
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8455	657571	1.29

Instrument :
BNA_P
ClientSampleId :
DFTPP