

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120325\
 Data File : BP026234.D
 Acq On : 03 Dec 2025 19:43
 Operator : RC/JU
 Sample : Q3753-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 MOO-25-334-337

Quant Time: Dec 04 00:05:58 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 19 01:25:31 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.661	152	309190	20.000	ng	-0.01
21) Naphthalene-d8	10.419	136	1111564	20.000	ng	-0.03
39) Acenaphthene-d10	14.295	164	591827	20.000	ng	-0.03
64) Phenanthrene-d10	17.107	188	1013215	20.000	ng	#-0.02
76) Chrysene-d12	21.542	240	1371417	20.000	ng	-0.03
86) Perylene-d12	24.824	264	1647362	20.000	ng	-0.08
System Monitoring Compounds						
5) 2-Fluorophenol	5.284	112	1410953	73.246	ng	0.00
7) Phenol-d6	6.843	99	1690136	68.919	ng	-0.01
23) Nitrobenzene-d5	8.796	82	1004228	51.317	ng	-0.02
42) 2,4,6-Tribromophenol	15.813	330	635737	82.806	ng	-0.02
45) 2-Fluorobiphenyl	12.890	172	2325727	57.594	ng	-0.04
79) Terphenyl-d14	19.842	244	3481594	51.765	ng	-0.03
Target Compounds						
						Qvalue
32) Benzoic acid	9.690	122	112321	7.385	ng	95
75) Fluoranthene	19.248	202	291967	4.210	ng	# 62
78) Pyrene	19.625	202	257921	2.868	ng	# 64
83) Chrysene	21.589	228	180142	2.029	ng	# 91
88) Benzo(b)fluoranthene	23.783	252	260524	2.597	ng	# 80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120325\
Data File : BP026234.D
Acq On : 03 Dec 2025 19:43
Operator : RC/JU
Sample : Q3753-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
MOO-25-334-337

Quant Time: Dec 04 00:05:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP111825.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 19 01:25:31 2025
Response via : Initial Calibration




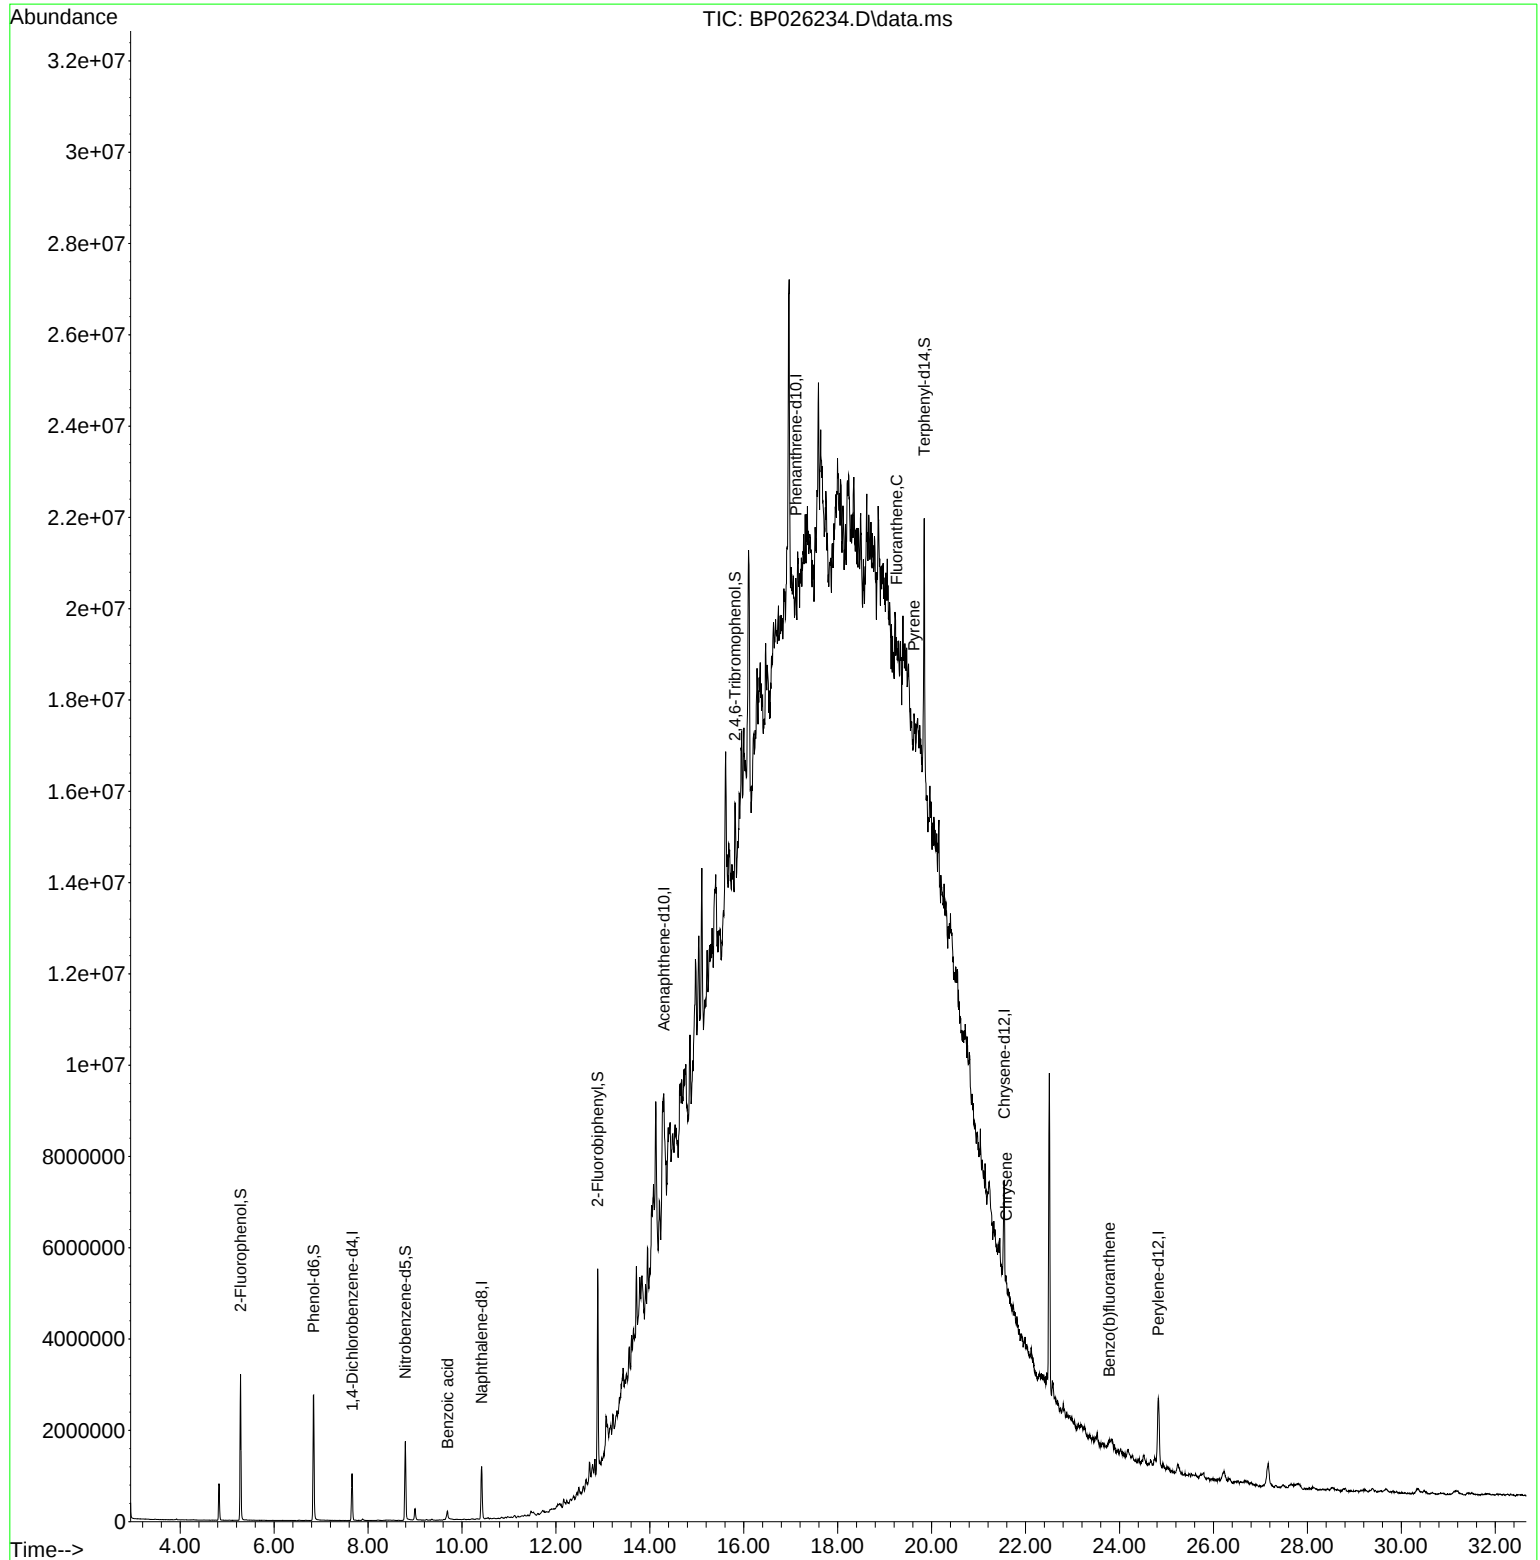




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.661 min Scan# 807
Delta R.T. -0.011 min
Lab File: BP026234.D
Acq: 03 Dec 2025 19:43




Instrument :
BNA_P
ClientSampleId :
MOO-25-334-337

Tgt Ion:152 Resp: 309190
Ion Ratio Lower Upper
152 100
150 157.1 123.0 184.6
115 58.1 46.3 69.5

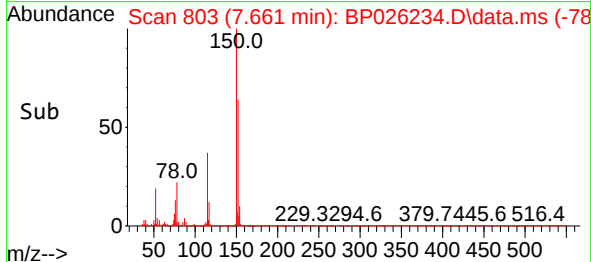

#5
2-Fluorophenol
Concen: 73.246 ng
RT: 5.284 min Scan# 399
Delta R.T. -0.006 min
Lab File: BP026234.D
Acq: 03 Dec 2025 19:43

Tgt Ion:112 Resp: 1410953
Ion Ratio Lower Upper
112 100
64 56.6 45.8 68.6
63 29.4 23.5 35.3


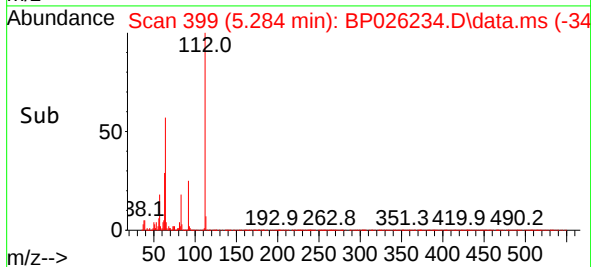

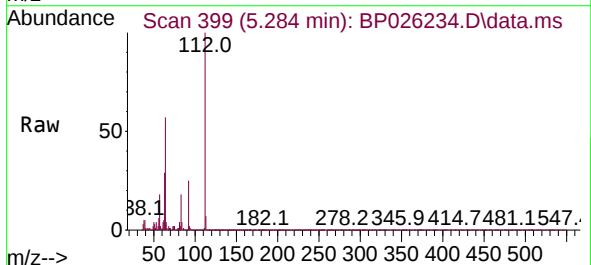




#7
Phenol-d6
Concen: 68.919 ng
RT: 6.843 min Scan# 60
Delta R.T. -0.012 min
Lab File: BP026234.D
Acq: 03 Dec 2025 19:43




Instrument :
BNA_P
ClientSampleId :
MOO-25-334-337


Tgt Ion: 99 Resp: 1690136
Ion Ratio Lower Upper
99 100
42 16.1 12.9 19.3
71 32.1 24.8 37.2

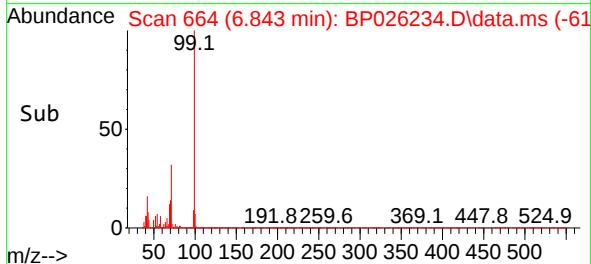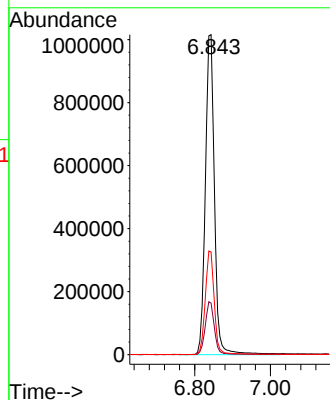

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.419 min Scan# 1272
Delta R.T. -0.029 min
Lab File: BP026234.D
Acq: 03 Dec 2025 19:43

Tgt Ion: 136 Resp: 1111564
Ion Ratio Lower Upper
136 100
137 11.0 8.7 13.1
54 8.0 6.4 9.6
68 5.5 4.9 7.3


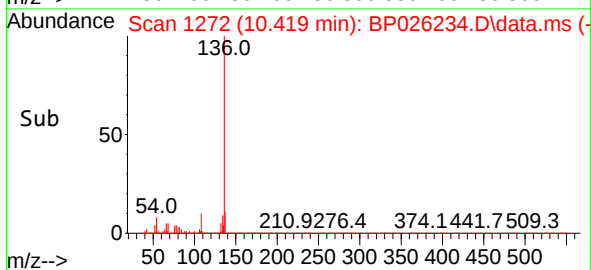
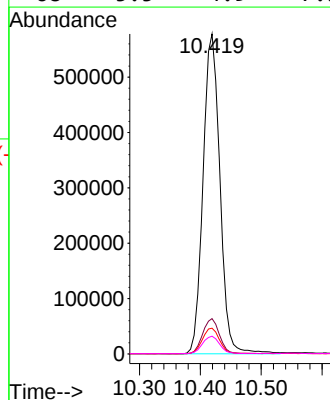
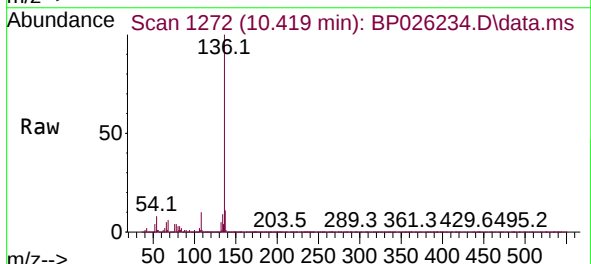




#23
Nitrobenzene-d5
Concen: 51.317 ng
RT: 8.796 min Scan# 99
Delta R.T. -0.017 min
Lab File: BP026234.D
Acq: 03 Dec 2025 19:43




Instrument :
BNA_P
ClientSampleId :
MOO-25-334-337


Tgt Ion: 82 Resp: 1004228
Ion Ratio Lower Upper
82 100
128 47.4 37.4 56.0
54 50.9 41.6 62.4

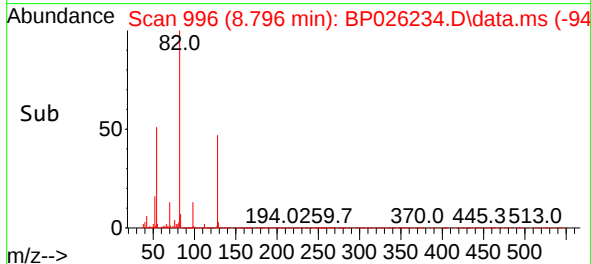

#32
Benzoic acid
Concen: 7.385 ng
RT: 9.690 min Scan# 1148
Delta R.T. -0.076 min
Lab File: BP026234.D
Acq: 03 Dec 2025 19:43

Tgt Ion: 122 Resp: 112321
Ion Ratio Lower Upper
122 100
105 124.9 100.1 140.1
77 91.5 66.7 106.7

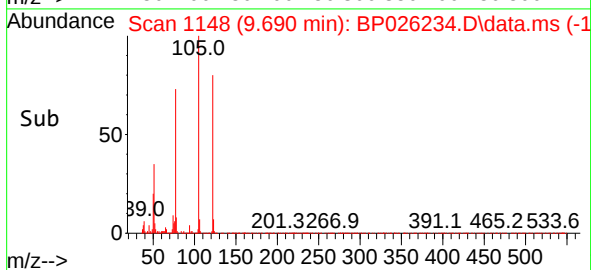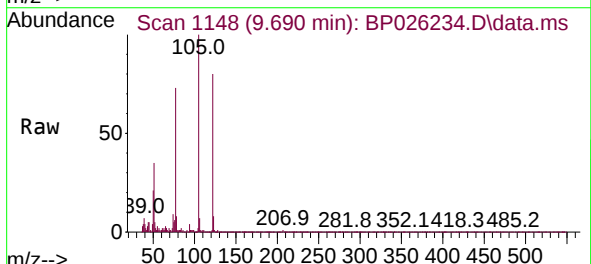



#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.295 min Scan# 19

Delta R.T. -0.029 min

Lab File: BP026234.D

Acq: 03 Dec 2025 19:43

Instrument :

BNA_P

ClientSampleId :

MOO-25-334-337





Tgt Ion:164 Resp: 591827

Ion Ratio Lower Upper

164 100

162 95.7 80.3 120.5

160 42.6 35.2 52.8

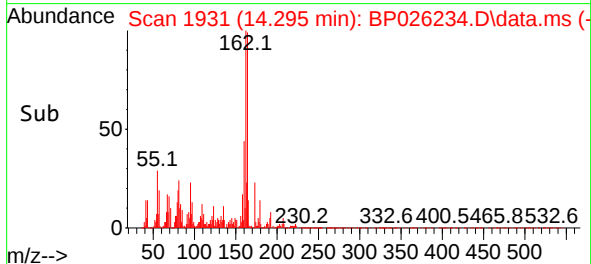

#42

2,4,6-Tribromophenol

Concen: 82.806 ng

RT: 15.813 min Scan# 2189

Delta R.T. -0.023 min

Lab File: BP026234.D

Acq: 03 Dec 2025 19:43




Tgt Ion:330 Resp: 635737


Ion Ratio Lower Upper

330 100

332 97.0 78.0 117.0

141 23.1 26.8 40.2#

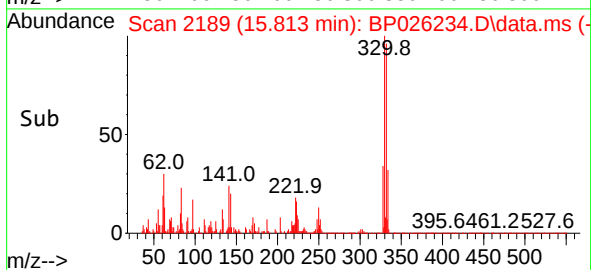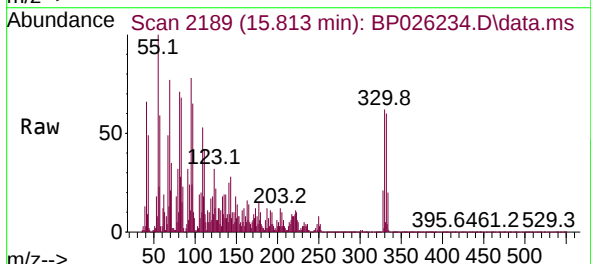



#45

2-Fluorobiphenyl

Concen: 57.594 ng

RT: 12.890 min Scan# 1

Delta R.T. -0.041 min

Lab File: BP026234.D

Acq: 03 Dec 2025 19:43

Instrument :

BNA_P

ClientSampleId :

MOO-25-334-337





Tgt Ion:172 Resp: 2325727

Ion Ratio Lower Upper

172 100

171 35.3 28.2 42.4

170 23.5 18.7 28.1

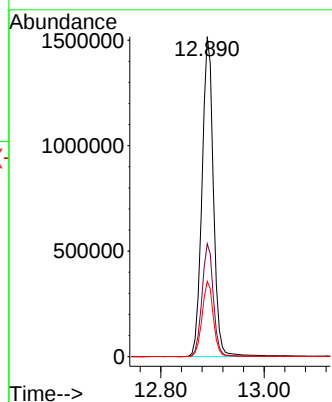

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.107 min Scan# 2409

Delta R.T. -0.023 min

Lab File: BP026234.D

Acq: 03 Dec 2025 19:43




Tgt Ion:188 Resp: 1013215


Ion Ratio Lower Upper

188 100

94 20.3 7.8 11.6#

80 18.0 8.2 12.2#


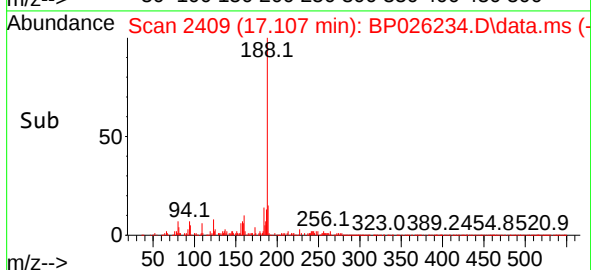






#75
Fluoranthene
Concen: 4.210 ng
RT: 19.248 min Scan# 21
Delta R.T. -0.017 min
Lab File: BP026234.D
Acq: 03 Dec 2025 19:43




Instrument :
BNA_P
ClientSampleId :
MOO-25-334-337


Tgt Ion:202 Resp: 291967
Ion Ratio Lower Upper
202 100
101 8.7 0.0 31.2
203 43.2 0.0 37.7#

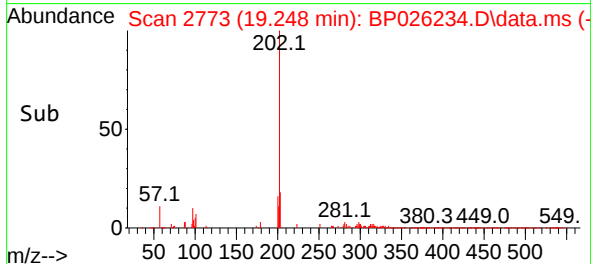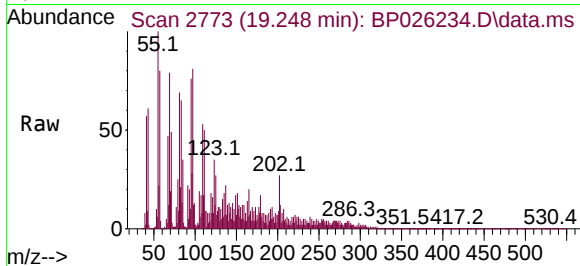

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.542 min Scan# 3163
Delta R.T. -0.029 min
Lab File: BP026234.D
Acq: 03 Dec 2025 19:43

Tgt Ion:240 Resp: 1371417
Ion Ratio Lower Upper
240 100
120 10.8 9.0 13.4
236 26.3 20.4 30.6

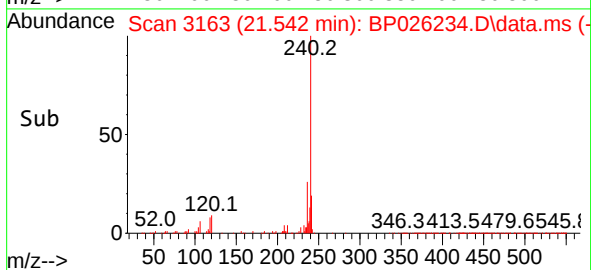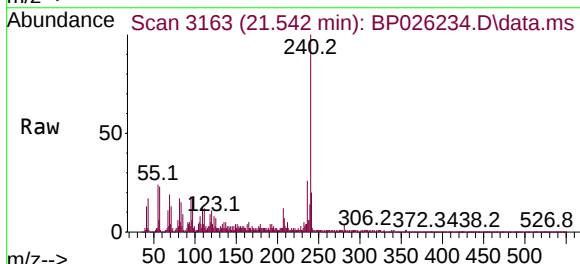



#78

Pyrene

Concen: 2.868 ng

RT: 19.625 min Scan# 2837

Delta R.T. -0.017 min

Lab File: BP026234.D

Acq: 03 Dec 2025 19:43

Instrument :

BNA_P

ClientSampleId :

MOO-25-334-337





Tgt Ion:202 Resp: 257921

Ion Ratio Lower Upper

202 100

200 27.0 16.9 25.3#

203 45.3 13.8 20.8#

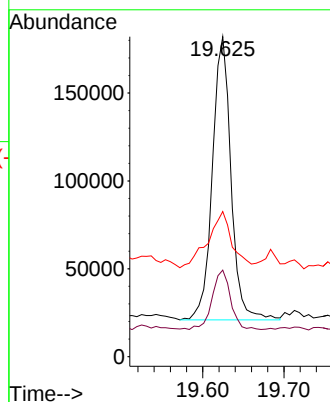

#79

Terphenyl-d14

Concen: 51.765 ng

RT: 19.842 min Scan# 2874

Delta R.T. -0.029 min

Lab File: BP026234.D

Acq: 03 Dec 2025 19:43




Tgt Ion:244 Resp: 3481594


Ion Ratio Lower Upper

244 100

212 7.4 5.8 8.8

122 8.8 8.2 12.2

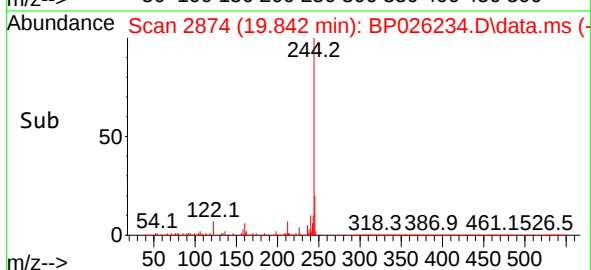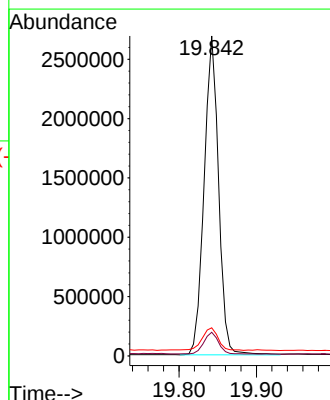



#83

Chrysene

Concen: 2.029 ng

RT: 21.589 min Scan# 3178

Delta R.T. -0.029 min

Lab File: BP026234.D

Acq: 03 Dec 2025 19:43

Instrument :

BNA_P

ClientSampleId :

MOO-25-334-337





Tgt Ion:228 Resp: 180142

Ion Ratio Lower Upper

228 100

226 32.3 23.9 35.9

229 27.5 15.9 23.9#

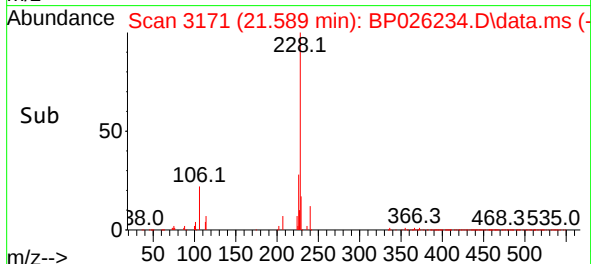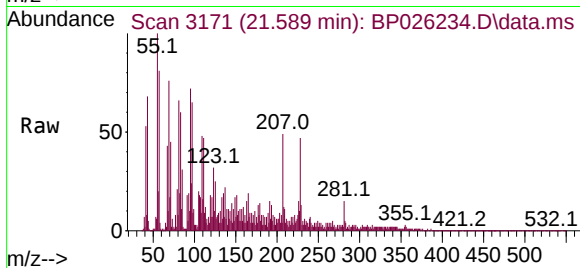

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.824 min Scan# 3721

Delta R.T. -0.082 min

Lab File: BP026234.D

Acq: 03 Dec 2025 19:43




Tgt Ion:264 Resp: 1647362


Ion Ratio Lower Upper

264 100

260 23.8 18.7 28.1


265 22.0 17.5 26.3

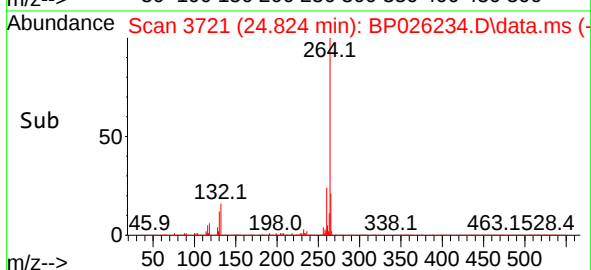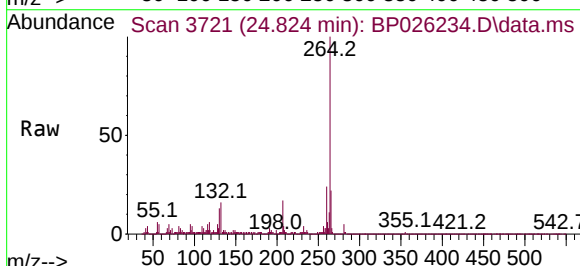



#88
 Benzo(b)fluoranthene
 Concen: 2.597 ng
 RT: 23.783 min Scan# 31
 Delta R.T. -0.082 min
 Lab File: BP026234.D
 Acq: 03 Dec 2025 19:43

Instrument :
 BNA_P
 ClientSampleId :
 MOO-25-334-337



Tgt Ion:252 Resp: 260524
 Ion Ratio Lower Upper
 252 100
 253 26.4 17.6 26.4#
 125 26.1 8.2 12.4#

