




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018575.D
 Acq On : 04 Dec 2023 21:42
 Operator : MA/JU
 Sample : 05441-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG6

Manual IntegrationsAPPROVED

Quant Time: Dec 04 22:28:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 04 21:39:40 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/05/2023
 Supervised By :mohammad ahmed 12/08/2023

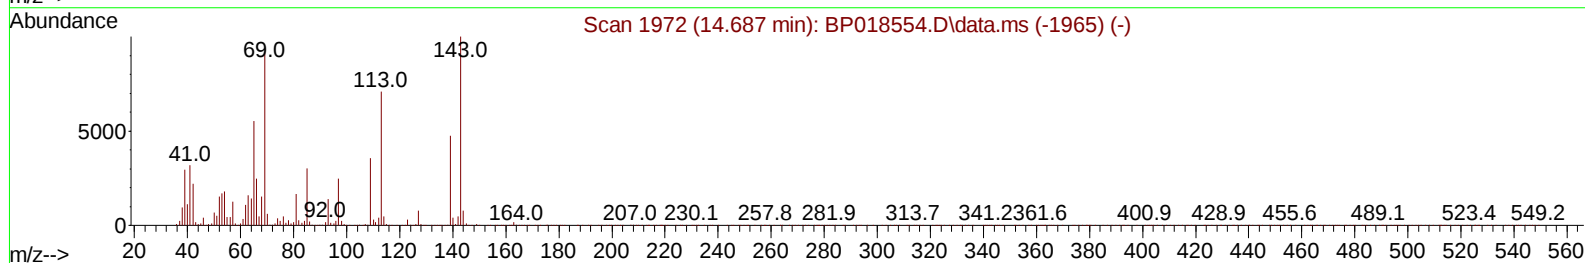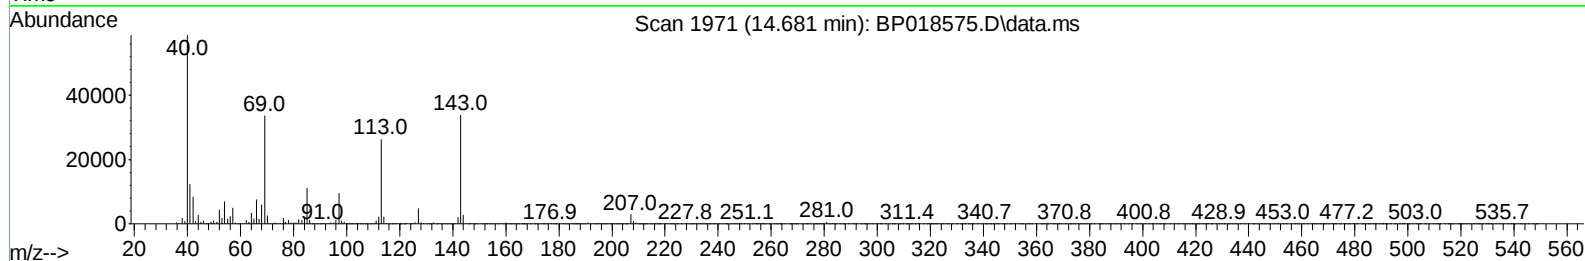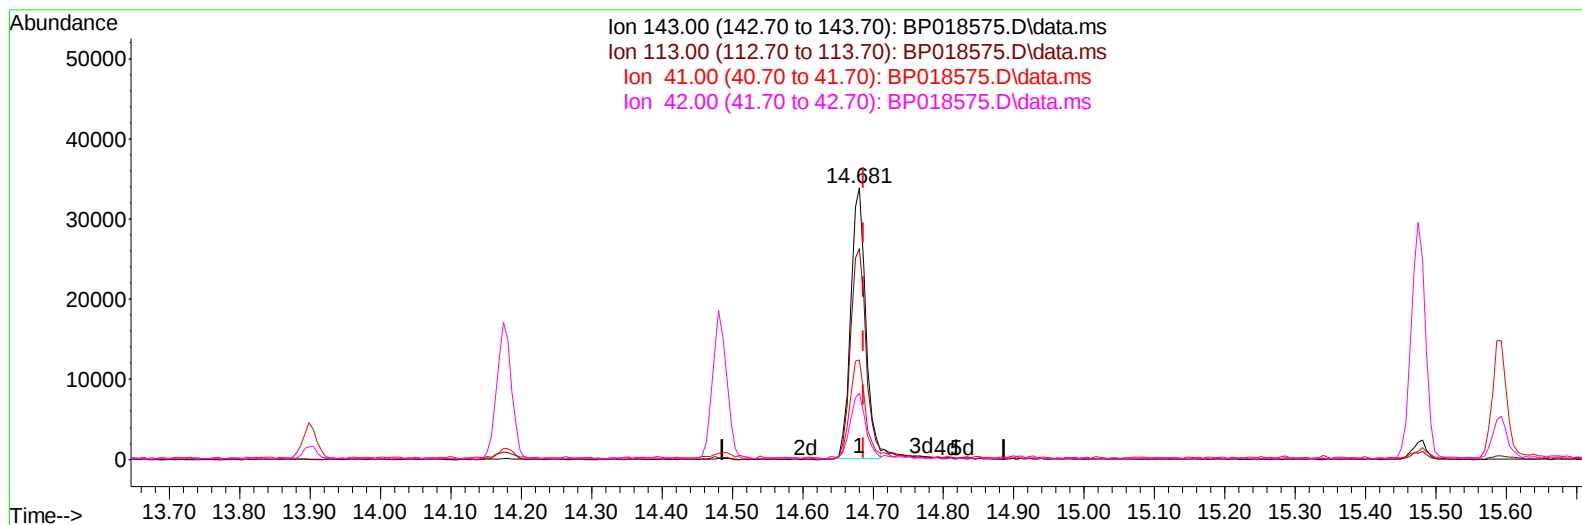

TIC: BP018575.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.681min (-0.006) 3.49 ng/u1

response 49377

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	70.80	77.80
41.00	34.60	36.71
42.00	23.00	24.43




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018575.D
 Acq On : 04 Dec 2023 21:42
 Operator : MA/JU
 Sample : 05441-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG6

Manual IntegrationsAPPROVED

Quant Time: Dec 04 22:28:30 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 04 21:39:40 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/05/2023
 Supervised By :mohammad ahmed 12/08/2023

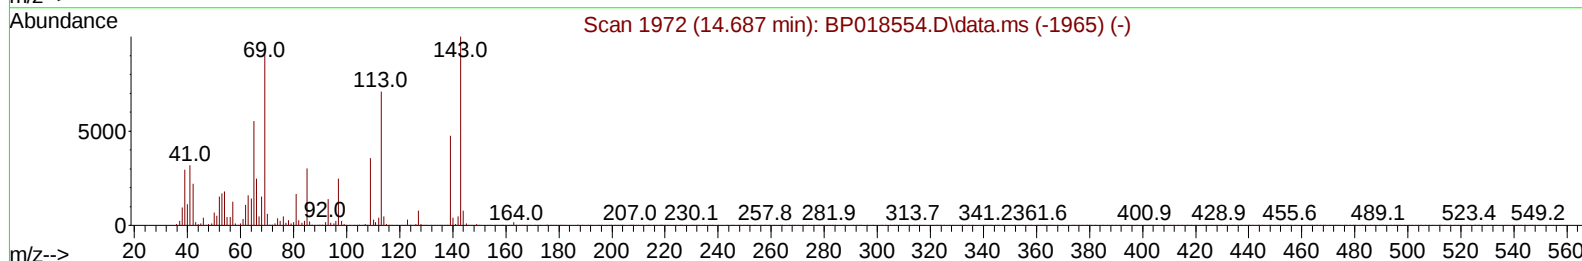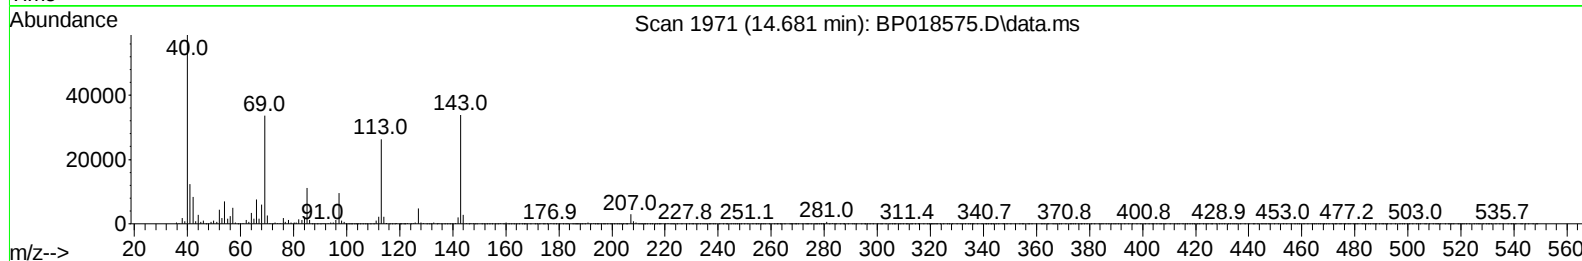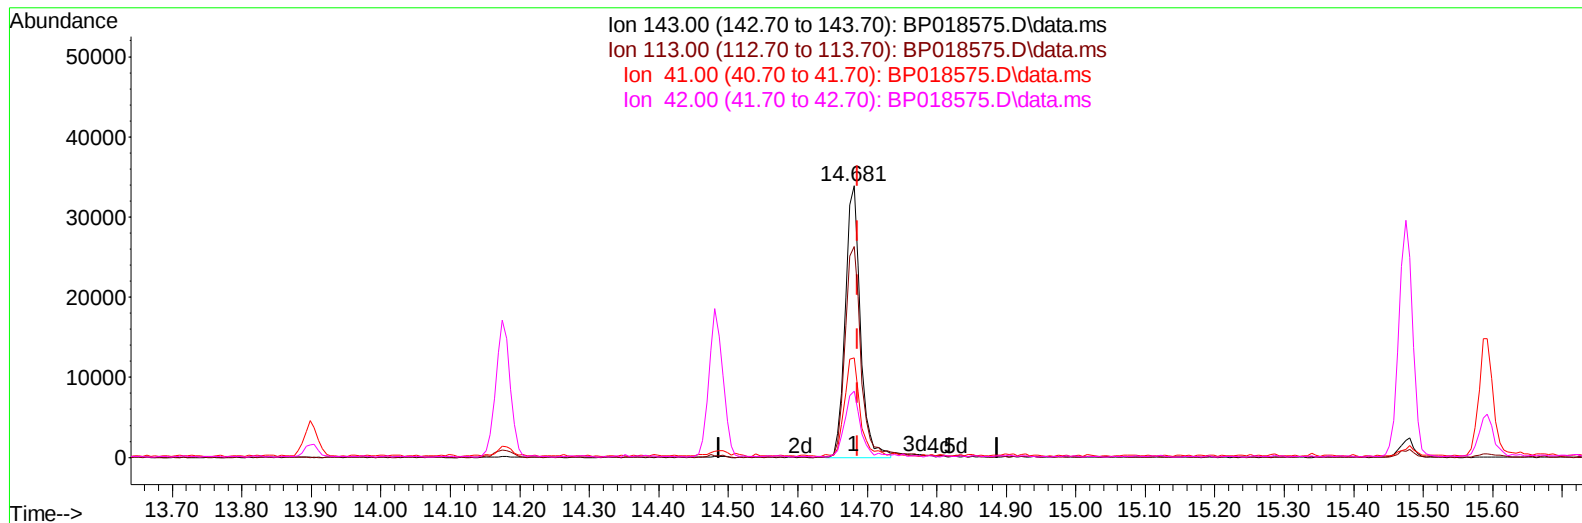

TIC: BP018575.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.681min (-0.006) 3.62 ng/ul m

response 51174

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	70.80	77.80
41.00	34.60	36.71
42.00	23.00	24.43

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018575.D
 Acq On : 04 Dec 2023 21:42
 Operator : MA/JU
 Sample : 05441-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG6

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/05/2023
 Supervised By :mohammad ahmed 12/08/2023

Quant Time: Dec 04 22:29:11 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 04 21:39:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.857	152	321403	20.000	ng/ul	0.00
20) Naphthalene-d8	10.651	136	1388068	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.481	164	966070	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.233	188	2200583	20.000	ng/ul	0.00
79) Chrysene-d12	21.316	240	2224402	20.000	ng/ul	0.00
88) Perylene-d12	23.692	264	2060716	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	35980	3.815	ng/uL	0.00
4) Pyridine-d5	3.687	84	256195	10.141	ng/ul	0.00
7) Phenol-d5	7.022	99	181726	5.634	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.193	67	634863	33.210	ng/ul	0.00
11) 2-Chlorophenol-d4	7.387	132	505988	20.105	ng/ul	0.00
15) 4-Methylphenol-d8	8.563	113	274705	10.524	ng/ul	0.00
21) Nitrobenzene-d5	9.016	128	287480	23.270	ng/ul	0.00
24) 2-Nitrophenol-d4	9.734	143	279654	21.833	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.269	165	530459	20.254	ng/ul	0.00
31) 4-Chloroaniline-d4	10.793	131	733628	21.433	ng/ul	0.00
46) Dimethylphthalate-d6	13.898	166	2223782	25.791	ng/ul	0.00
49) Acenaphthylene-d8	14.175	160	2319544	24.431	ng/ul	0.00
54) 4-Nitrophenol-d4	14.681	143	51174m	3.616	ng/ul	0.00
60) Fluorene-d10	15.475	176	1962128	27.111	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.592	200	307492	23.304	ng/ul	0.00
73) Anthracene-d10	17.328	188	3440465	29.739	ng/ul	0.00
81) Pyrene-d10	19.569	212	5011023	28.940	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.539	264	3615301	30.089	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018575.D
Acq On : 04 Dec 2023 21:42
Operator : MA/JU
Sample : 05441-11
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG6

Manual IntegrationsAPPROVED

Quant Time: Dec 04 22:29:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 04 21:39:40 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/05/2023
Supervised By :mohammad ahmed 12/08/2023

