

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018595.D
 Acq On : 05 Dec 2023 10:37
 Operator : MA/JU
 Sample : 05441-14
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QH4

Quant Time: Dec 05 11:27:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 04 21:39:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.852	152	355465	20.000	ng/u1	0.00
20) Naphthalene-d8	10.651	136	1574983	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.481	164	1069782	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.228	188	2341939	20.000	ng/u1	0.00
79) Chrysene-d12	21.316	240	1732910	20.000	ng/u1	0.00
88) Perylene-d12	23.686	264	1791162	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	39231	3.761	ng/uL	0.00
4) Pyridine-d5	3.693	84	122457	4.383	ng/u1	0.00
7) Phenol-d5	7.022	99	207070	5.805	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.187	67	698985	33.061	ng/u1	0.00
11) 2-Chlorophenol-d4	7.381	132	623440	22.398	ng/u1	0.00
15) 4-Methylphenol-d8	8.563	113	413759	14.332	ng/u1	0.00
21) Nitrobenzene-d5	9.016	128	432825	30.877	ng/u1	0.00
24) 2-Nitrophenol-d4	9.734	143	424432	29.204	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.269	165	789920	26.581	ng/u1	0.00
31) 4-Chloroaniline-d4	10.787	131	857475	22.079	ng/u1	0.00
46) Dimethylphthalate-d6	13.898	166	3320674	34.779	ng/u1	0.00
49) Acenaphthylene-d8	14.175	160	3419078	32.521	ng/u1	0.00
54) 4-Nitrophenol-d4	14.675	143	71695	4.575	ng/u1	-0.01
60) Fluorene-d10	15.475	176	2835926	35.385	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.592	200	407642	29.030	ng/u1	0.00
73) Anthracene-d10	17.328	188	4661058	37.858	ng/u1	0.00
81) Pyrene-d10	19.569	212	5054710	37.472	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.533	264	4077371	39.041	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.305	88	11576	1.012 ng/uL	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018595.D
Acq On : 05 Dec 2023 10:37
Operator : MA/JU
Sample : 05441-14
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QH4


Quant Time: Dec 05 11:27:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 04 21:39:40 2023
Response via : Initial Calibration

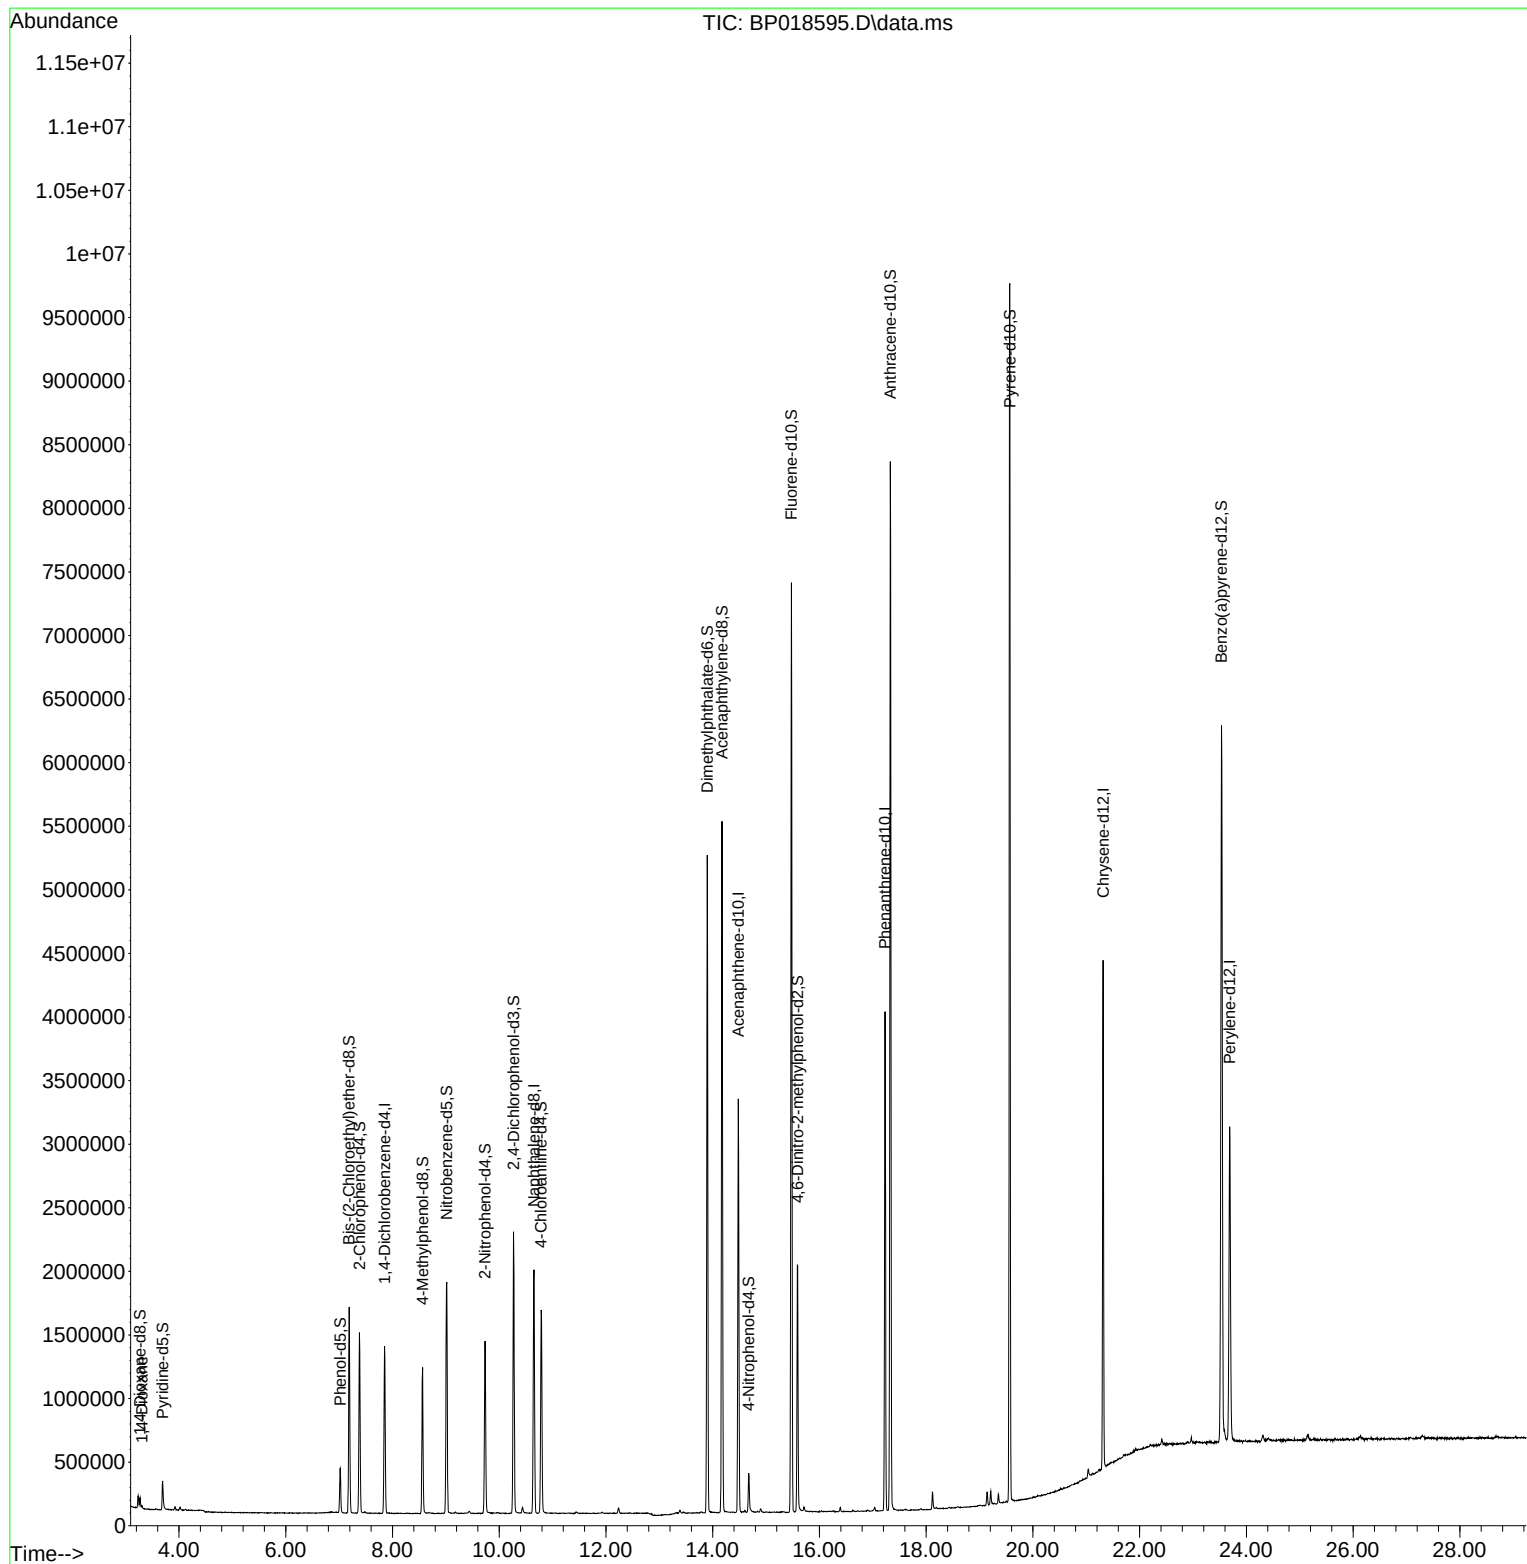

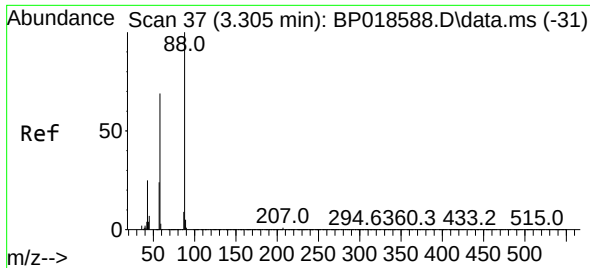

#2
 1,4-Dioxane
 Concen: 1.012 ng/uL
 RT: 3.305 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: BP018595.D
 Acq: 05 Dec 2023 10:37

Instrument :
 BNA_P
 ClientSampleId :
 C0QH4

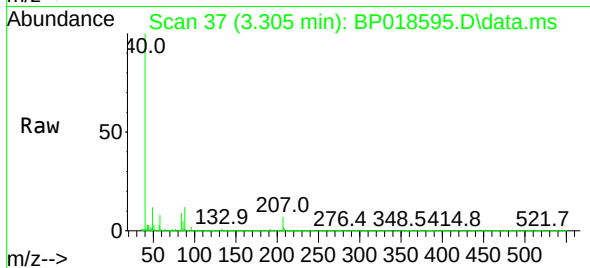

Tgt Ion: 88 Resp: 11576
 Ion Ratio Lower Upper
 88 100
 43 22.1 21.8 32.6
 58 66.9 56.5 84.7

