

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018600.D
 Acq On : 05 Dec 2023 13:26
 Operator : MA/JU
 Sample : 05441-19
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QL1

Quant Time: Dec 05 14:06:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 04 21:39:40 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.852	152	322483	20.000	ng/u1	0.00
20) Naphthalene-d8	10.652	136	1440574	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.481	164	994445	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.228	188	2307453	20.000	ng/u1	0.00
79) Chrysene-d12	21.316	240	1900028	20.000	ng/u1	0.00
88) Perylene-d12	23.686	264	1819623	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	36924	3.902	ng/uL	0.00
4) Pyridine-d5	3.687	84	224043	8.839	ng/u1	0.00
7) Phenol-d5	7.017	99	176657	5.459	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.187	67	660856	34.454	ng/u1	0.00
11) 2-Chlorophenol-d4	7.381	132	576426	22.827	ng/u1	0.00
15) 4-Methylphenol-d8	8.564	113	381342	14.560	ng/u1	0.00
21) Nitrobenzene-d5	9.011	128	403698	31.486	ng/u1	0.00
24) 2-Nitrophenol-d4	9.734	143	381493	28.699	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.269	165	735942	27.075	ng/u1	0.00
31) 4-Chloroaniline-d4	10.787	131	1060419	29.852	ng/u1	0.00
46) Dimethylphthalate-d6	13.899	166	2991232	33.702	ng/u1	0.00
49) Acenaphthylene-d8	14.175	160	3255117	33.307	ng/u1	0.00
54) 4-Nitrophenol-d4	14.675	143	64889	4.454	ng/u1	-0.01
60) Fluorene-d10	15.475	176	2650237	35.573	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.587	200	364815	26.368	ng/u1	0.00
73) Anthracene-d10	17.328	188	4458736	36.756	ng/u1	0.00
81) Pyrene-d10	19.563	212	5141219	34.761	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.533	264	3964504	37.367	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.305	88	10978	1.058	ng/uL	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018600.D
Acq On : 05 Dec 2023 13:26
Operator : MA/JU
Sample : 05441-19
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QL1


Quant Time: Dec 05 14:06:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 04 21:39:40 2023
Response via : Initial Calibration

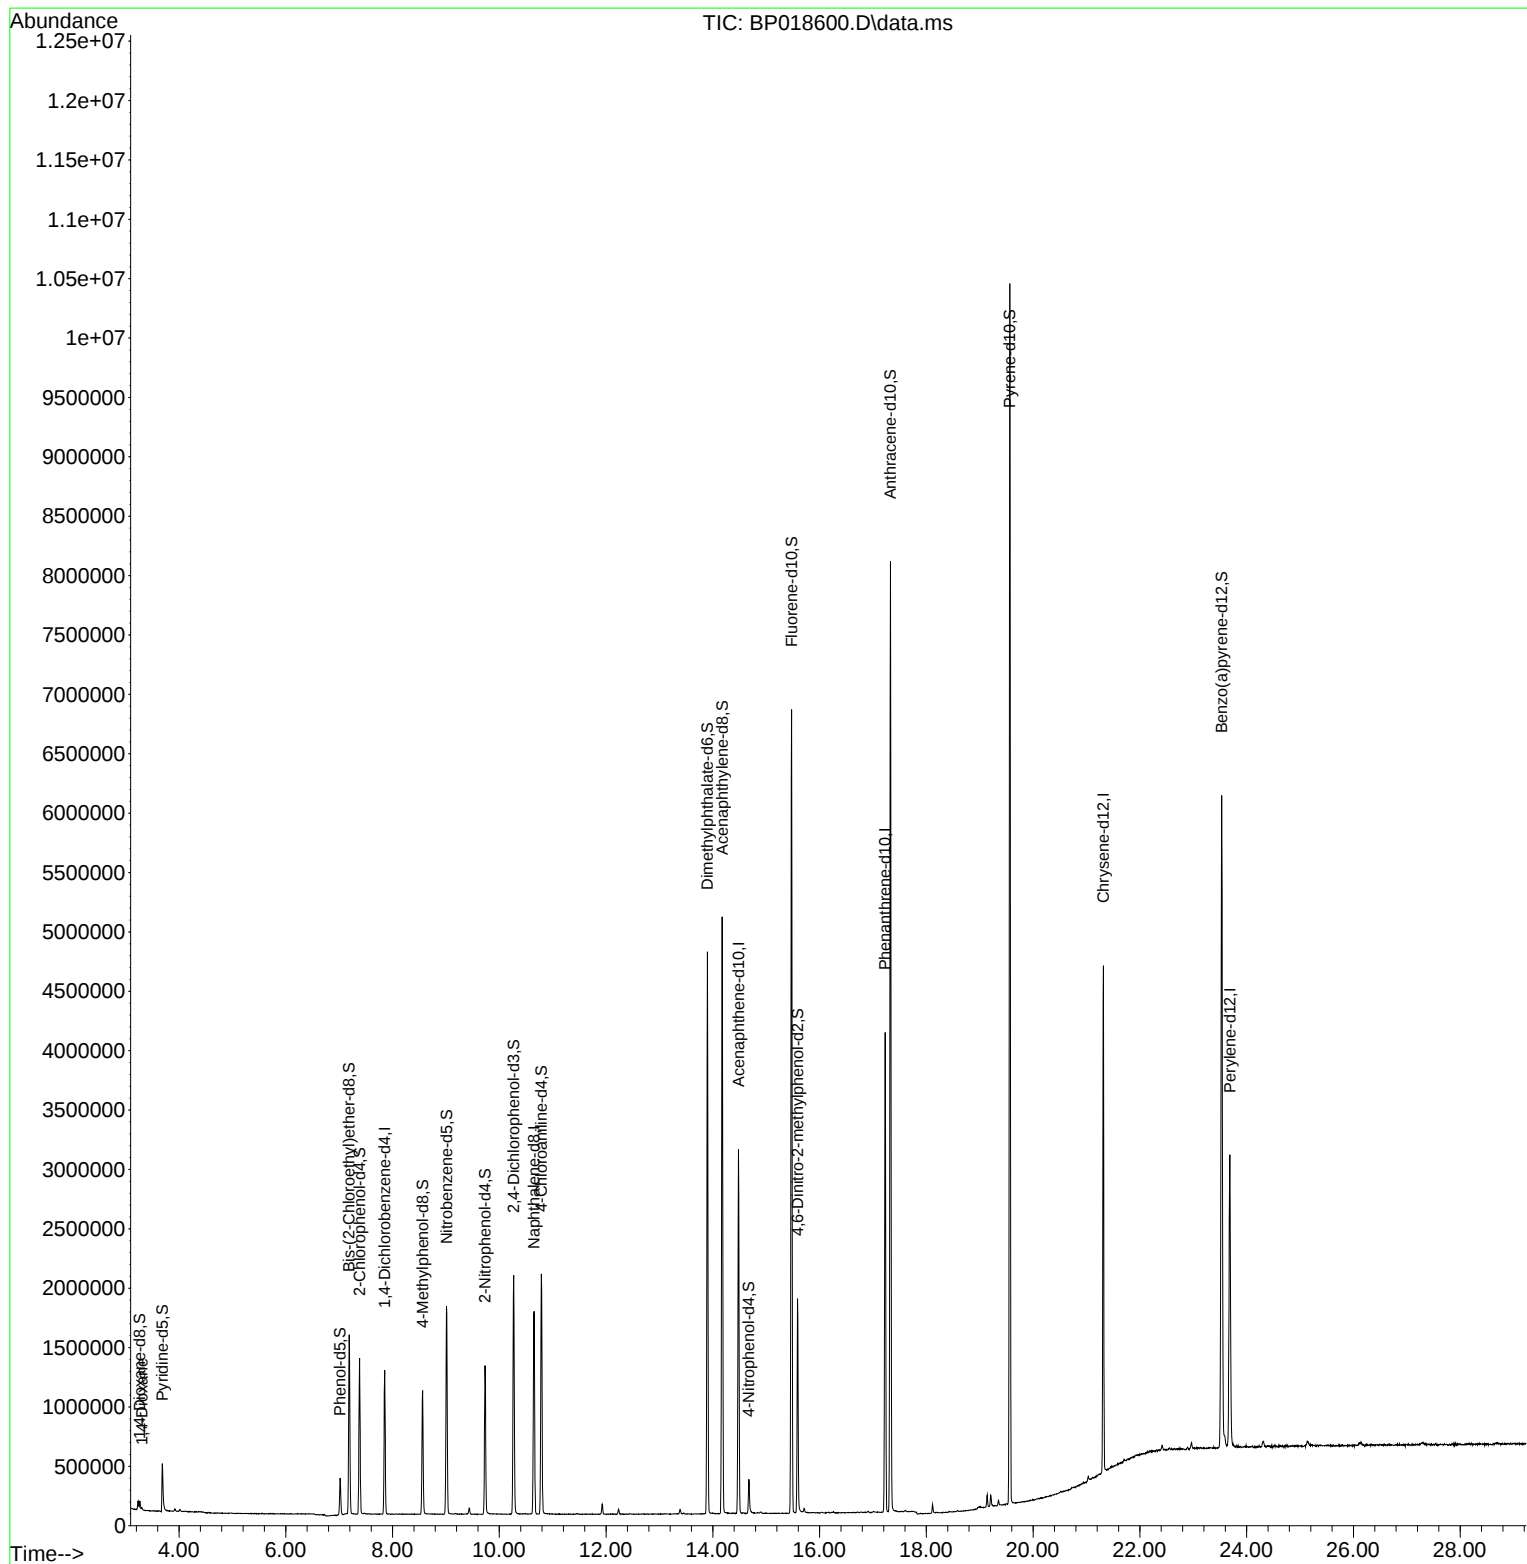

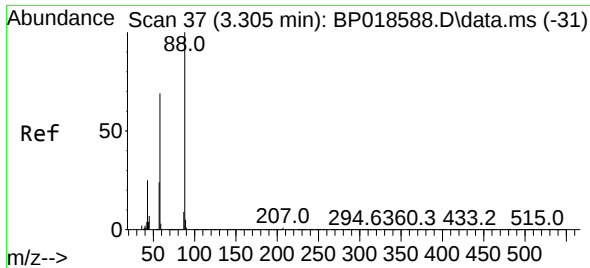

#2
 1,4-Dioxane
 Concen: 1.058 ng/uL
 RT: 3.305 min Scan# 31
 Delta R.T. 0.000 min
 Lab File: BP018600.D
 Acq: 05 Dec 2023 13:26

Instrument :
 BNA_P
 ClientSampleId :
 C0QL1

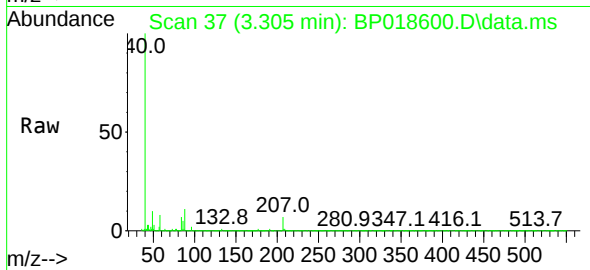

Tgt Ion	Ratio	Lower	Upper
88	100		
43	29.5	21.8	32.6
58	71.8	56.5	84.7

