

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018618.D
 Acq On : 05 Dec 2023 23:38
 Operator : MA/JU
 Sample : 05424-03
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YCGB7

Quant Time: Dec 06 00:07:10 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 04 21:39:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.852	152	334806	20.000	ng/u1	0.00
20) Naphthalene-d8	10.646	136	1491130	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.481	164	1026526	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.228	188	2255833	20.000	ng/u1	0.00
79) Chrysene-d12	21.310	240	1745643	20.000	ng/u1	0.00
88) Perylene-d12	23.680	264	1646112	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	37925	3.860	ng/uL	0.00
4) Pyridine-d5	3.687	84	276892	10.522	ng/u1	0.00
7) Phenol-d5	7.016	99	242981	7.232	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.187	67	612044	30.735	ng/u1	0.00
11) 2-Chlorophenol-d4	7.381	132	573382	21.870	ng/u1	0.00
15) 4-Methylphenol-d8	8.563	113	512749	18.857	ng/u1	0.00
21) Nitrobenzene-d5	9.010	128	401364	30.242	ng/u1	0.00
24) 2-Nitrophenol-d4	9.734	143	405960	29.504	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.269	165	793443	28.201	ng/u1	0.00
31) 4-Chloroaniline-d4	10.787	131	889192	24.183	ng/u1	0.00
46) Dimethylphthalate-d6	13.898	166	3118672	34.040	ng/u1	0.00
49) Acenaphthylene-d8	14.175	160	3200623	31.726	ng/u1	0.00
54) 4-Nitrophenol-d4	14.681	143	77489	5.153	ng/u1	0.00
60) Fluorene-d10	15.475	176	2619078	34.056	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.586	200	404896	29.935	ng/u1	0.00
73) Anthracene-d10	17.328	188	4215427	35.545	ng/u1	0.00
81) Pyrene-d10	19.563	212	4780034	35.177	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.527	264	3500805	36.474	ng/u1	0.00


Target Compounds					Qvalue
13) 2-Methylphenol	8.299	108	25638	1.016 ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018618.D
Acq On : 05 Dec 2023 23:38
Operator : MA/JU
Sample : 05424-03
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YCGB7

Quant Time: Dec 06 00:07:10 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Dec 04 21:39:40 2023
Response via : Initial Calibration

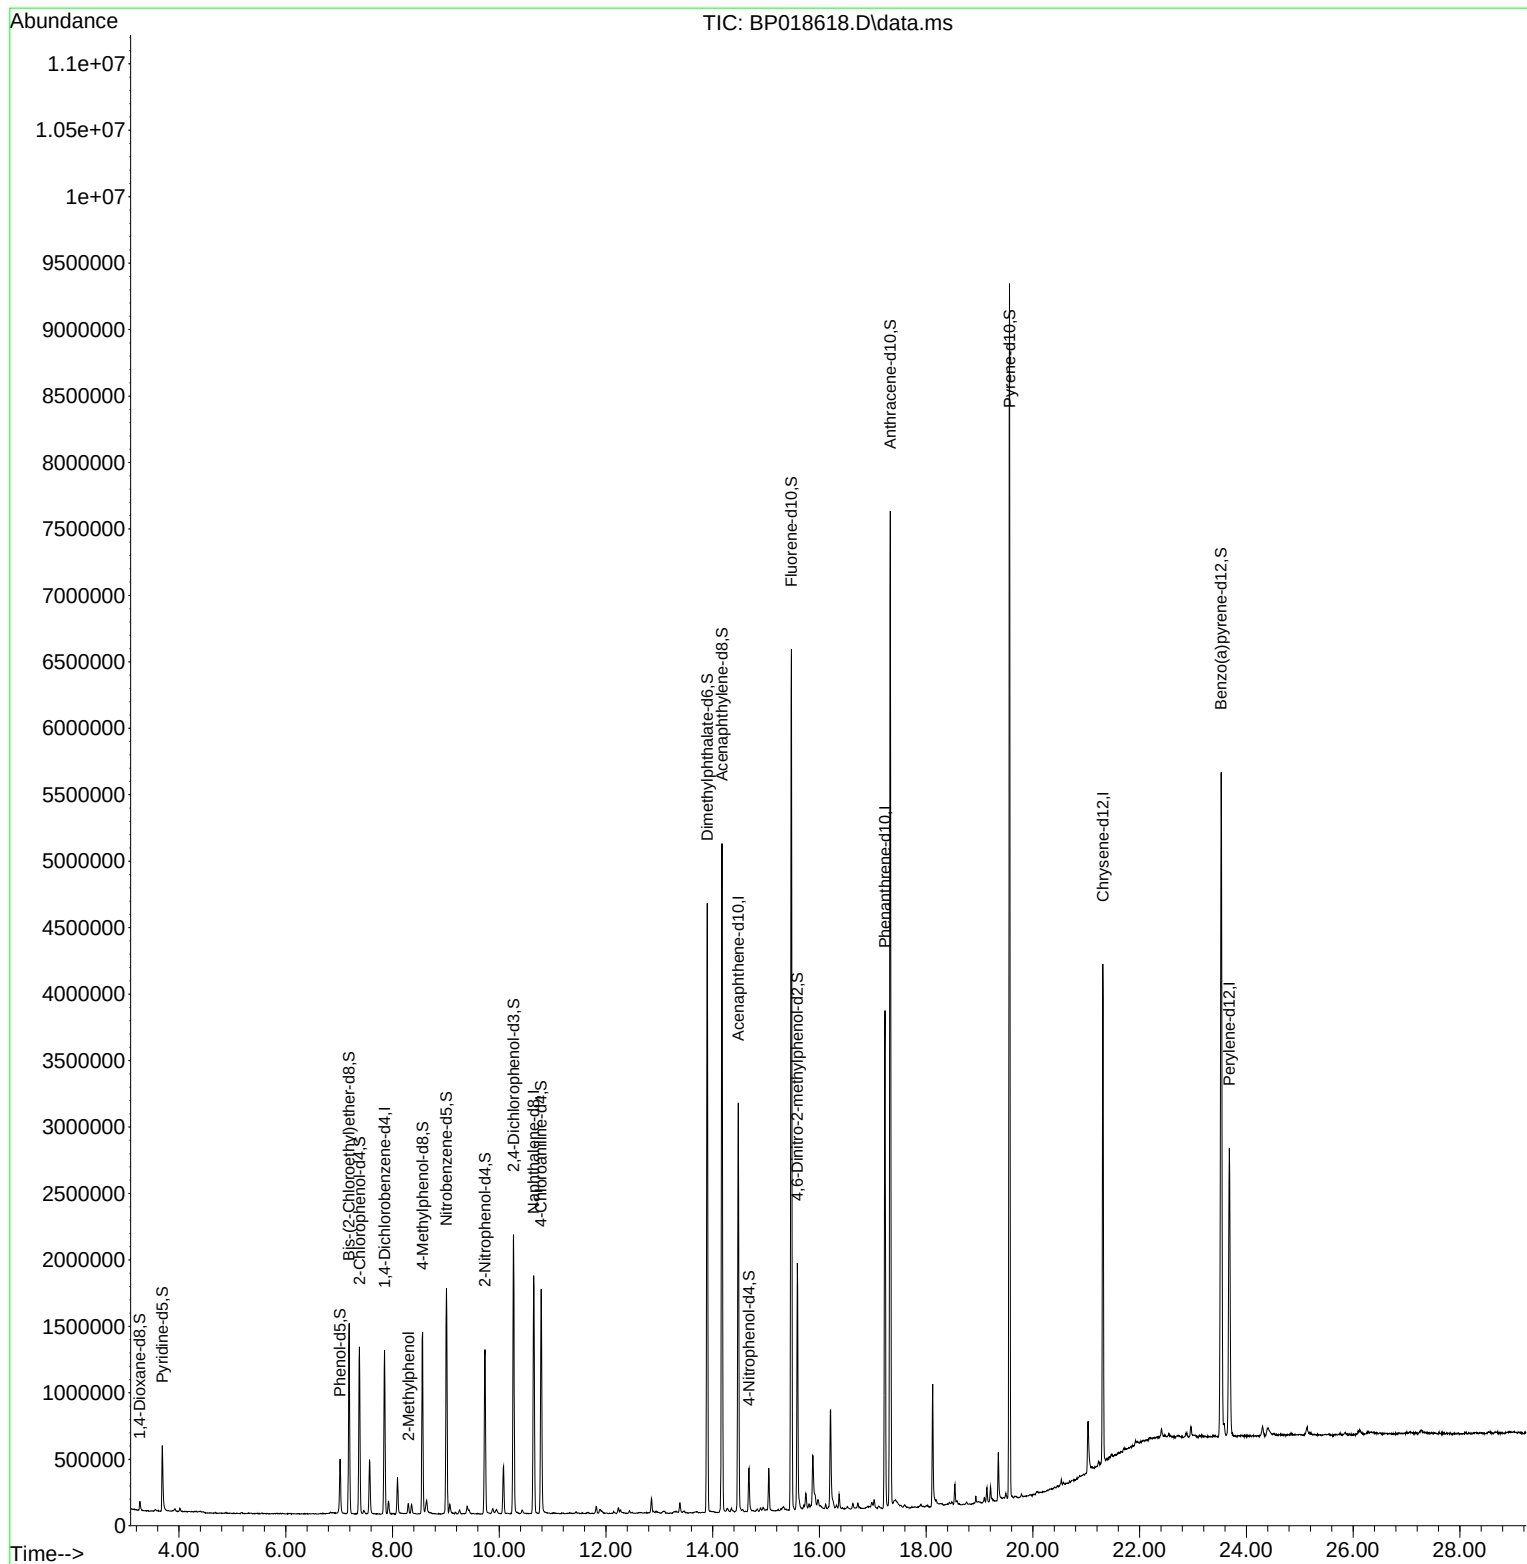

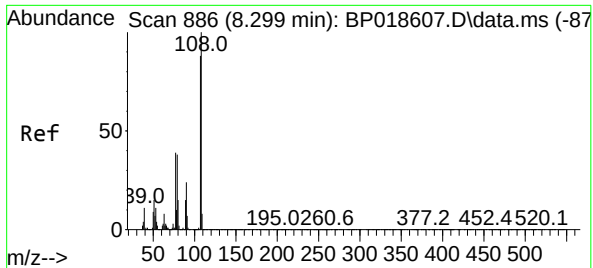

#13
 2-Methylphenol
 Concen: 1.016 ng/ul
 RT: 8.299 min Scan# 886
 Delta R.T. -0.006 min
 Lab File: BP018618.D
 Acq: 05 Dec 2023 23:38

Instrument :
 BNA_P
 ClientSampleId :
 YCGB7

Tgt Ion:108 Resp: 25638
 Ion Ratio Lower Upper
 108 100
 107 90.0 70.6 105.8

