

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018634.D
 Acq On : 06 Dec 2023 13:30
 Operator : MA/JU
 Sample : 05456-07MS
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E05N2MS

Quant Time: Dec 06 21:40:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 04 21:39:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.852	152	296327	20.000	ng/u1	0.00
20) Naphthalene-d8	10.651	136	1170846	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.481	164	565058	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.228	188	1064344	20.000	ng/u1	0.00
79) Chrysene-d12	21.321	240	1135083	20.000	ng/u1	0.00
88) Perylene-d12	23.692	264	1388549	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.264	96	53926	6.201	ng/uL	0.00
4) Pyridine-d5	3.687	84	729580	31.323	ng/u1	0.00
7) Phenol-d5	7.022	99	964359	32.429	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.187	67	598036	33.931	ng/u1	0.00
11) 2-Chlorophenol-d4	7.387	132	783634	33.771	ng/u1	0.00
15) 4-Methylphenol-d8	8.569	113	728413	30.267	ng/u1	0.00
21) Nitrobenzene-d5	9.016	128	364759	35.003	ng/u1	0.00
24) 2-Nitrophenol-d4	9.734	143	387900	35.903	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.275	165	713543	32.299	ng/u1	0.00
31) 4-Chloroaniline-d4	10.793	131	839806	29.088	ng/u1	0.00
46) Dimethylphthalate-d6	13.898	166	1644499	32.608	ng/u1	0.00
49) Acenaphthylene-d8	14.175	160	1944704	35.019	ng/u1	0.00
54) 4-Nitrophenol-d4	14.687	143	258781	31.260	ng/u1	0.00
60) Fluorene-d10	15.475	176	1274830	30.115	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.598	200	162532	25.468	ng/u1	0.00
73) Anthracene-d10	17.328	188	1952260	34.890	ng/u1	0.00
81) Pyrene-d10	19.569	212	2428805	27.489	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.539	264	2808652	34.691	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.299	88	116381	12.205	ng/uL	98
5) Pyridine	3.705	79	798944	33.967	ng/u1	96
6) Benzaldehyde	6.993	77	479387	31.223	ng/u1	98
8) Phenol	7.052	94	1006650	34.518	ng/u1	100
10) Bis(2-Chloroethyl)ether	7.281	93	829760	34.645	ng/u1	99
12) 2-Chlorophenol	7.416	128	795582	33.877	ng/u1	98
13) 2-Methylphenol	8.299	108	728481	32.629	ng/u1	97
14) 2,2'-oxybis(1-Chloropr...	8.381	45	977490	32.166	ng/u1	98
16) Acetophenone	8.681	105	1144757	31.918	ng/u1	98
17) N-Nitroso-di-n-propyla...	8.669	70	555155	28.136	ng/u1	99
18) 4-Methylphenol	8.634	108	762178	31.263	ng/u1	96
19) Hexachloroethane	8.928	117	341002	35.419	ng/u1	96
22) Nitrobenzene	9.057	77	861359	33.997	ng/u1	99
23) Isophorone	9.587	82	1551340	30.030	ng/u1	99
25) 2-Nitrophenol	9.769	139	409308	35.383	ng/u1	99
26) 2,4-Dimethylphenol	9.834	107	618703	27.347	ng/u1	100
27) Bis(2-Chloroethoxy)met...	10.069	93	1013605	31.079	ng/u1	100
29) 2,4-Dichlorophenol	10.299	162	687724	32.319	ng/u1	98
30) Naphthalene	10.699	128	2314820	32.590	ng/u1	99
32) 4-Chloroaniline	10.816	127	760307	27.630	ng/u1	99
33) Hexachlorobutadiene	10.987	225	543571	38.142	ng/u1	99
34) Caprolactam	11.593	113	176159	26.998	ng/u1	94
35) 4-Chloro-3-methylphenol	11.940	107	621148	26.057	ng/u1	99
36) 2-Methylnaphthalene	12.310	142	1455262	28.921	ng/u1	100


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018634.D
 Acq On : 06 Dec 2023 13:30
 Operator : MA/JU
 Sample : 05456-07MS
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E05N2MS

Quant Time: Dec 06 21:40:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Dec 04 21:39:40 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.528	142	1411771	27.782	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.675	216	841717	41.057	ng/ul	99
40) Hexachlorocyclopentadiene	12.657	237	450151	37.045	ng/ul	99
41) 2,4,6-Trichlorophenol	12.916	196	486454	36.885	ng/ul	99
42) 2,4,5-Trichlorophenol	12.987	196	502865	35.171	ng/ul	100
43) 1,1'-Biphenyl	13.322	154	1802891	36.892	ng/ul	99
44) 2-Chloronaphthalene	13.363	162	1436162	37.209	ng/ul	99
45) 2-Nitroaniline	13.569	65	345876	33.055	ng/ul	96
47) Dimethylphthalate	13.945	163	1617374	32.580	ng/ul	99
48) 2,6-Dinitrotoluene	14.063	165	317814	33.885	ng/ul	96
50) Acenaphthylene	14.204	152	2154530	34.508	ng/ul	100
51) 3-Nitroaniline	14.392	138	310730	33.189	ng/ul	98
52) Acenaphthene	14.545	153	1405064	34.036	ng/ul	99
53) 2,4-Dinitrophenol	14.598	184	102082	20.536	ng/ul	97
55) 4-Nitrophenol	14.698	109	202039	32.304	ng/ul	96
56) Dibenzofuran	14.881	168	1885931	32.870	ng/ul	98
57) 2,4-Dinitrotoluene	14.851	165	425001	32.214	ng/ul	95
58) 2,3,4,6-Tetrachlorophenol	15.104	232	351672	29.323	ng/ul	97
59) Diethylphthalate	15.310	149	1364731	28.094	ng/ul	100
61) Fluorene	15.534	166	1464729	32.263	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.528	204	786241	33.021	ng/ul	96
63) 4-Nitroaniline	15.551	138	313326	35.129	ng/ul	99
66) 4,6-Dinitro-2-methylph...	15.610	198	183514	26.896	ng/ul	98
67) N-Nitrosodiphenylamine	15.745	169	1226791	34.784	ng/ul	100
68) 4-Bromophenyl-phenylether	16.422	248	477117	35.508	ng/ul	95
69) Hexachlorobenzene	16.534	284	536753	35.778	ng/ul	99
70) Atrazine	16.698	200	341290	32.548	ng/ul	98
71) Pentachlorophenol	16.881	266	319261	35.782	ng/ul	97
72) Phenanthrene	17.275	178	2224454	34.605	ng/ul	100
74) Anthracene	17.363	178	2232225	34.644	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.281	216	799867	43.463	ng/ul	98
76) Pentachlorobenzene	14.798	250	707519	39.138	ng/ul	99
77) Carbazole	17.639	167	2011337	39.167	ng/ul	99
78) Di-n-butylphthalate	18.192	149	2436155	35.627	ng/ul	100
80) Fluoranthene	19.239	202	2760208	26.428	ng/ul	99
82) Pyrene	19.592	202	2871223	27.251	ng/ul	98
83) Butylbenzylphthalate	20.474	149	1168115	30.284	ng/ul	95
84) 3,3'-Dichlorobenzidine	21.239	252	872365	31.626	ng/ul	98
85) Benzo(a)anthracene	21.304	228	3135435	34.032	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.233	149	1580847	29.818	ng/ul#	98
87) Chrysene	21.357	228	2906220	34.254	ng/ul	100
89) Di-n-octyl phthalate	22.145	149	3175196	31.319	ng/ul	100
90) Benzo(b)fluoranthene	22.968	252	3348861	32.710	ng/ul	99
91) Benzo(k)fluoranthene	23.016	252	3233205	32.640	ng/ul	99
93) Benzo(a)pyrene	23.586	252	3172841	33.917	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	26.162	276	4030273	36.059	ng/ul	97
95) Dibenzo(a,h)anthracene	26.186	278	3358389	36.121	ng/ul	98
96) Benzo(g,h,i)perylene	26.921	276	3264418	36.292	ng/ul	96





(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2
 1,4-Dioxane
 Concen: 12.205 ng/uL
 RT: 3.299 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: BP018634.D
 Acq: 06 Dec 2023 13:30




Instrument :
 BNA_P
 ClientSampleId :
 E05N2MS


Tgt Ion:	88	Resp:	116381
Ion	Ratio	Lower	Upper
88	100		
43	25.7	21.8	32.6
58	71.7	56.5	84.7

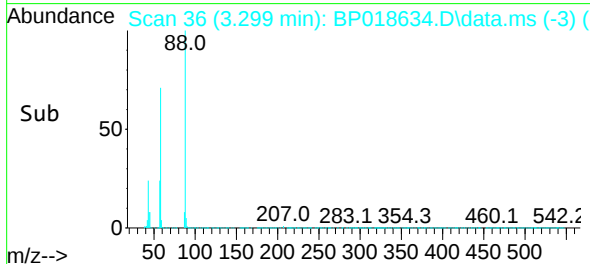

#5
 Pyridine
 Concen: 33.967 ng/uL
 RT: 3.705 min Scan# 105
 Delta R.T. 0.000 min
 Lab File: BP018634.D
 Acq: 06 Dec 2023 13:30

Tgt Ion:	79	Resp:	798944
Ion	Ratio	Lower	Upper
79	100		
52	66.8	57.4	86.0
51	32.0	26.2	39.4


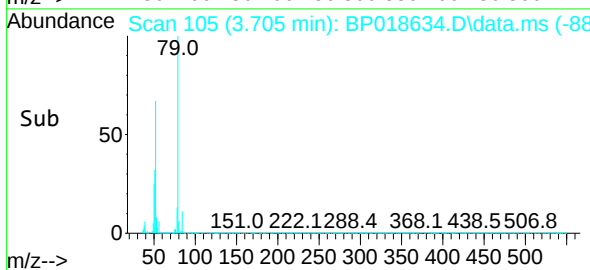

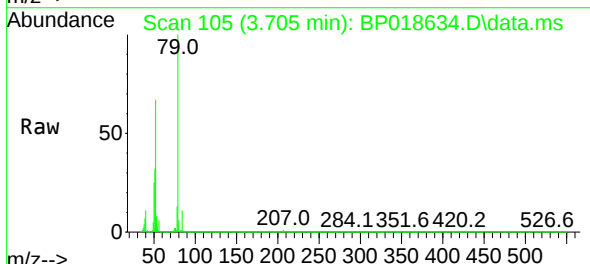




#6
Benzaldehyde
Concen: 31.223 ng/ul
RT: 6.993 min Scan# 60
Delta R.T. -0.006 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30




Instrument :
BNA_P
ClientSampleId :
E05N2MS


Tgt Ion: 77 Resp: 479387
Ion Ratio Lower Upper
77 100
105 99.9 77.9 116.9
106 94.2 74.6 111.8



#8
Phenol
Concen: 34.518 ng/ul
RT: 7.052 min Scan# 674
Delta R.T. 0.000 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30

Tgt Ion: 94 Resp: 1006650
Ion Ratio Lower Upper
94 100
65 26.3 21.0 31.6
66 35.7 28.6 43.0









#10
Bis(2-Chloroethyl)ether
Concen: 34.645 ng/ul
RT: 7.281 min Scan# 713
Delta R.T. -0.006 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30




Instrument :
BNA_P
ClientSampleId :
E05N2MS


Tgt Ion: 93 Resp: 829760
Ion Ratio Lower Upper
93 100
63 73.5 58.3 87.5
95 32.6 25.9 38.9



#12
2-Chlorophenol
Concen: 33.877 ng/ul
RT: 7.416 min Scan# 736
Delta R.T. 0.000 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30

Tgt Ion:128 Resp: 795582
Ion Ratio Lower Upper
128 100
64 45.4 37.0 55.4
130 32.3 26.8 40.2









#13
2-Methylphenol
Concen: 32.629 ng/ul
RT: 8.299 min Scan# 81
Delta R.T. -0.006 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30




Instrument :
BNA_P
ClientSampleId :
E05N2MS


Tgt Ion:108 Resp: 728481
Ion Ratio Lower Upper
108 100
107 90.6 70.6 105.8



#14
2,2'-oxybis(1-Chloropropane)
Concen: 32.166 ng/ul
RT: 8.381 min Scan# 900
Delta R.T. -0.006 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30

Tgt Ion: 45 Resp: 977490
Ion Ratio Lower Upper
45 100
77 16.8 12.7 19.1
79 12.7 10.5 15.7









#16
Acetophenone
Concen: 31.918 ng/ul
RT: 8.681 min Scan# 91
Delta R.T. 0.000 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30




Instrument :
BNA_P
ClientSampleId :
E05N2MS


Tgt Ion:105 Resp: 1144757
Ion Ratio Lower Upper
105 100
77 76.2 59.4 89.0
51 23.8 19.4 29.0



#17
N-Nitroso-di-n-propylamine
Concen: 28.136 ng/ul
RT: 8.669 min Scan# 949
Delta R.T. -0.006 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30

Tgt Ion: 70 Resp: 555155
Ion Ratio Lower Upper
70 100
42 50.5 41.0 61.4
101 10.6 7.8 11.8
130 21.5 16.9 25.3









#18
4-Methylphenol
Concen: 31.263 ng/ul
RT: 8.634 min Scan# 942
Delta R.T. 0.000 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30




Instrument :
BNA_P
ClientSampleId :
E05N2MS


Tgt Ion:108 Resp: 762178
Ion Ratio Lower Upper
108 100
107 109.5 90.6 136.0



#19
Hexachloroethane
Concen: 35.419 ng/ul
RT: 8.928 min Scan# 993
Delta R.T. -0.006 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30

Tgt Ion:117 Resp: 341002
Ion Ratio Lower Upper
117 100
201 109.1 83.7 125.5
199 68.8 52.3 78.5









#22
Nitrobenzene
Concen: 33.997 ng/ul
RT: 9.057 min Scan# 1105
Delta R.T. 0.000 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30




Instrument :
BNA_P
ClientSampleId :
E05N2MS


Tgt Ion: 77 Resp: 861359
Ion Ratio Lower Upper
77 100
123 44.2 35.8 53.8
65 12.8 10.5 15.7



#23
Isophorone
Concen: 30.030 ng/ul
RT: 9.587 min Scan# 1105
Delta R.T. 0.000 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30

Tgt Ion: 82 Resp: 1551340
Ion Ratio Lower Upper
82 100
95 7.0 5.5 8.3
138 17.3 13.5 20.3









#25
2-Nitrophenol
Concen: 35.383 ng/ul
RT: 9.769 min Scan# 1135
Delta R.T. 0.000 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30




Instrument :
BNA_P
ClientSampleId :
E05N2MS


Tgt Ion:139 Resp: 409308
Ion Ratio Lower Upper
139 100
65 48.6 39.1 58.7
109 30.7 23.8 35.6



#26
2,4-Dimethylphenol
Concen: 27.347 ng/ul
RT: 9.834 min Scan# 1147
Delta R.T. 0.000 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30

Tgt Ion:107 Resp: 618703
Ion Ratio Lower Upper
107 100
121 50.4 40.0 60.0
122 86.4 69.1 103.7









#27
 Bis(2-Chloroethoxy)methane
 Concen: 31.079 ng/ul
 RT: 10.069 min Scan# 1187
 Delta R.T. -0.006 min
 Lab File: BP018634.D
 Acq: 06 Dec 2023 13:30

Instrument :
 BNA_P
 ClientSampleId :
 E05N2MS

Tgt Ion: 93 Resp: 1013605




Ion	Ratio	Lower	Upper
93	100		
95	32.4	26.1	39.1
123	10.9	8.9	13.3

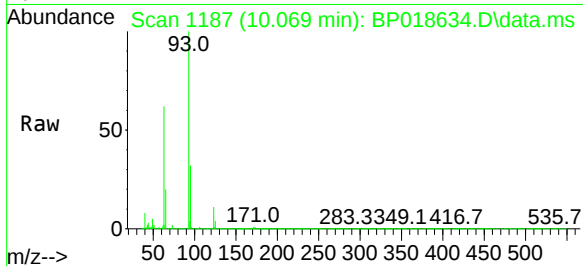


#29
 2,4-Dichlorophenol
 Concen: 32.319 ng/ul
 RT: 10.299 min Scan# 1226
 Delta R.T. 0.000 min
 Lab File: BP018634.D
 Acq: 06 Dec 2023 13:30

Tgt Ion:162 Resp: 687724

Ion	Ratio	Lower	Upper
162	100		
164	64.5	51.7	77.5
98	34.0	29.2	43.8




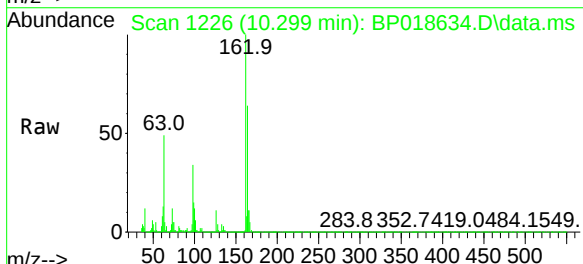




#30
Naphthalene
Concen: 32.590 ng/ul
RT: 10.699 min Scan# 1294
Delta R.T. -0.006 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30




Instrument :
BNA_P
ClientSampleId :
E05N2MS


Tgt Ion:128 Resp: 2314820
Ion Ratio Lower Upper
128 100
129 10.8 8.9 13.3
127 12.9 10.5 15.7

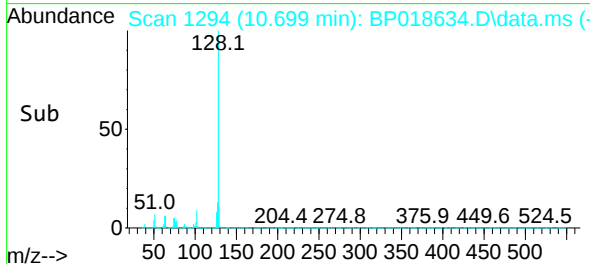

#32
4-Chloroaniline
Concen: 27.630 ng/ul
RT: 10.816 min Scan# 1314
Delta R.T. 0.000 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30

Tgt Ion:127 Resp: 760307
Ion Ratio Lower Upper
127 100
129 32.4 25.6 38.4


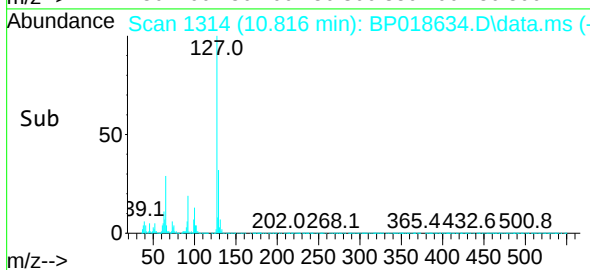

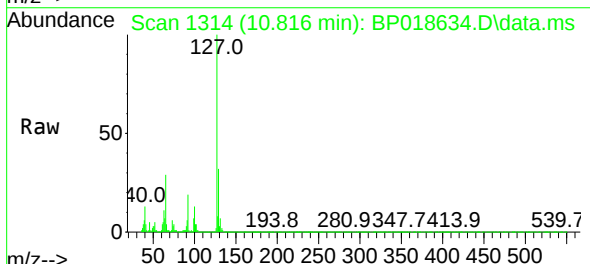




#33
Hexachlorobutadiene
Concen: 38.142 ng/ul
RT: 10.987 min Scan# 1343
Delta R.T. 0.000 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30




Instrument :
BNA_P
ClientSampleId :
E05N2MS


Tgt Ion:225 Resp: 543571
Ion Ratio Lower Upper
225 100
223 63.3 49.5 74.3
227 64.2 50.9 76.3

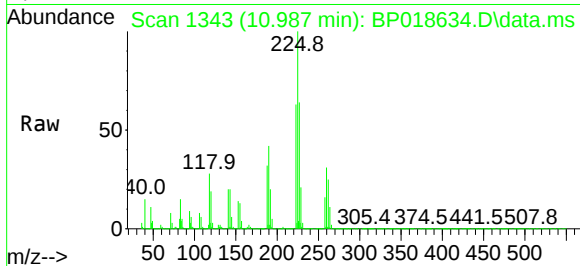

#34
Caprolactam
Concen: 26.998 ng/ul
RT: 11.593 min Scan# 1446
Delta R.T. 0.000 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30

Tgt Ion:113 Resp: 176159
Ion Ratio Lower Upper
113 100
55 159.5 133.7 200.5
56 115.4 97.4 146.2




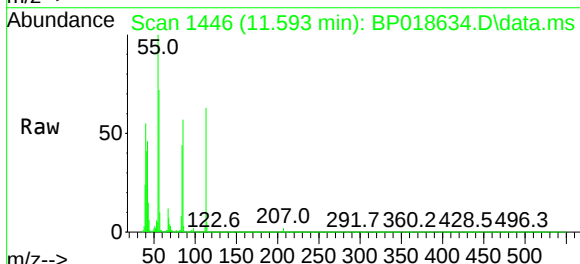




#35
4-Chloro-3-methylphenol
Concen: 26.057 ng/ul
RT: 11.940 min Scan# 1505
Delta R.T. 0.000 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30




Instrument :
BNA_P
ClientSampleId :
E05N2MS


Tgt Ion:107 Resp: 621148
Ion Ratio Lower Upper
107 100
144 26.3 21.0 31.6
142 80.4 63.6 95.4



#36
2-Methylnaphthalene
Concen: 28.921 ng/ul
RT: 12.310 min Scan# 1568
Delta R.T. 0.000 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30

Tgt Ion:142 Resp: 1455262
Ion Ratio Lower Upper
142 100
141 88.9 71.4 107.0









#37
1-Methylnaphthalene
Concen: 27.782 ng/ul
RT: 12.528 min Scan# 1605
Delta R.T. 0.000 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30




Instrument :
BNA_P
ClientSampleId :
E05N2MS


Tgt Ion:142 Resp: 1411771
Ion Ratio Lower Upper
142 100
141 93.1 73.5 110.3
116 3.7 2.8 4.2

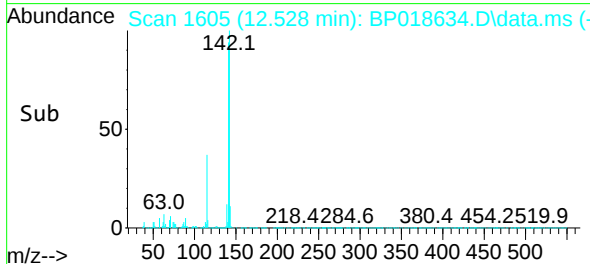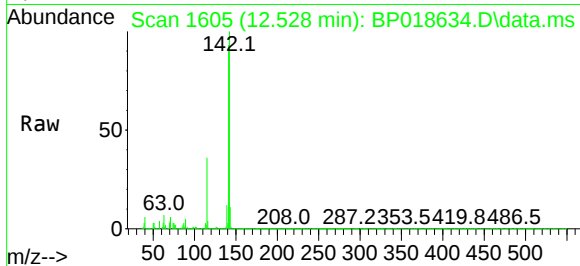

#39
1,2,4,5-Tetrachlorobenzene
Concen: 41.057 ng/ul
RT: 12.675 min Scan# 1630
Delta R.T. -0.006 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30

Tgt Ion:216 Resp: 841717
Ion Ratio Lower Upper
216 100
214 78.3 63.9 95.9
179 20.5 16.3 24.5
108 15.1 12.6 19.0


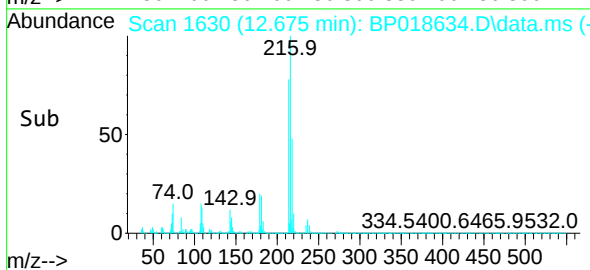

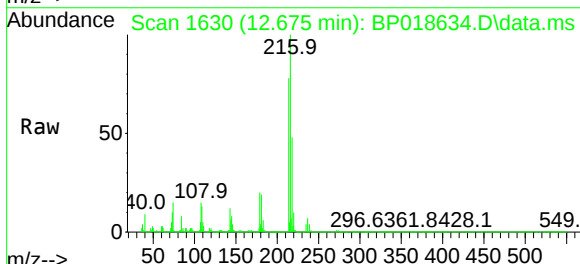




#40
Hexachlorocyclopentadiene
Concen: 37.045 ng/ul
RT: 12.657 min Scan# 1626
Delta R.T. 0.000 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30




Instrument :
BNA_P
ClientSampleId :
E05N2MS


Tgt Ion:237 Resp: 450151
Ion Ratio Lower Upper
237 100
235 61.3 49.4 74.0
272 12.9 9.8 14.8



#41
2,4,6-Trichlorophenol
Concen: 36.885 ng/ul
RT: 12.916 min Scan# 1671
Delta R.T. -0.006 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30

Tgt Ion:196 Resp: 486454
Ion Ratio Lower Upper
196 100
198 95.3 76.9 115.3
200 30.1 25.0 37.6





#42

2,4,5-Trichlorophenol

Concen: 35.171 ng/ul

RT: 12.987 min Scan# 1

Delta R.T. 0.000 min

Lab File: BP018634.D

Acq: 06 Dec 2023 13:30

Instrument :

BNA_P

ClientSampleId :

E05N2MS





Tgt Ion:196 Resp: 502865

Ion Ratio Lower Upper

196 100

198 97.1 77.9 116.9

200 31.4 25.2 37.8

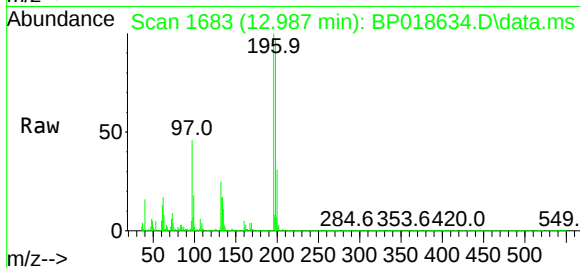

#43

1,1'-Biphenyl

Concen: 36.892 ng/ul

RT: 13.322 min Scan# 1740

Delta R.T. 0.000 min

Lab File: BP018634.D

Acq: 06 Dec 2023 13:30




Tgt Ion:154 Resp: 1802891


Ion Ratio Lower Upper

154 100

153 41.1 32.8 49.2

76 12.5 10.7 16.1




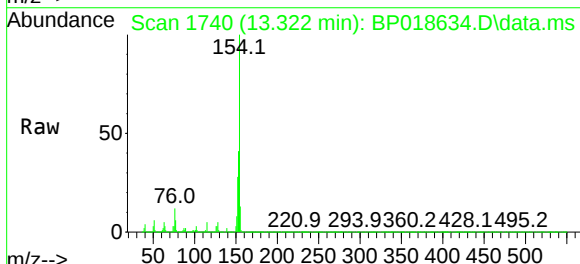




#44
2-Chloronaphthalene
Concen: 37.209 ng/ul
RT: 13.363 min Scan# 1747
Delta R.T. 0.000 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30




Instrument :
BNA_P
ClientSampleId :
E05N2MS


Tgt Ion:162 Resp: 1436162
Ion Ratio Lower Upper
162 100
164 32.4 25.7 38.5
127 36.7 30.3 45.5

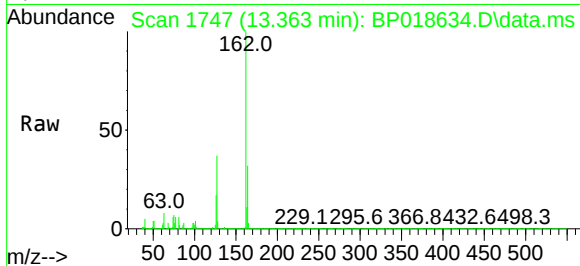

#45
2-Nitroaniline
Concen: 33.055 ng/ul
RT: 13.569 min Scan# 1782
Delta R.T. 0.000 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30

Tgt Ion: 65 Resp: 345876
Ion Ratio Lower Upper
65 100
92 74.2 56.9 85.3
138 114.6 88.2 132.2




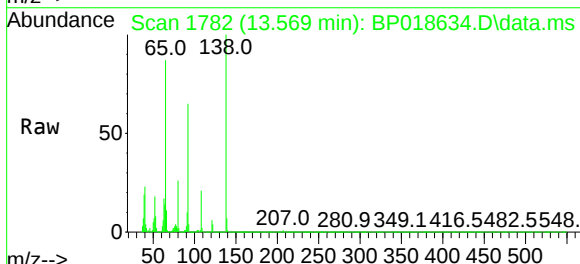




#47
Dimethylphthalate
Concen: 32.580 ng/ul
RT: 13.945 min Scan# 1846
Delta R.T. -0.006 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30




Instrument :
BNA_P
ClientSampleId :
E05N2MS


Tgt Ion:163 Resp: 1617374
Ion Ratio Lower Upper
163 100
194 4.2 3.2 4.8
164 10.2 8.0 12.0

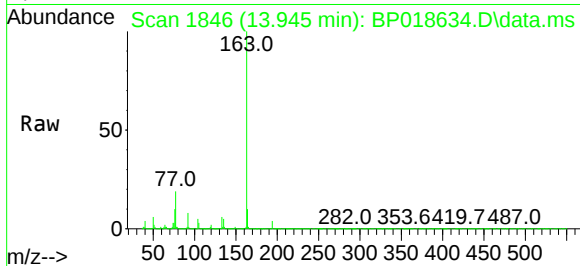

#48
2,6-Dinitrotoluene
Concen: 33.885 ng/ul
RT: 14.063 min Scan# 1866
Delta R.T. -0.006 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30

Tgt Ion:165 Resp: 317814
Ion Ratio Lower Upper
165 100
89 55.1 46.6 70.0
121 20.2 17.3 25.9




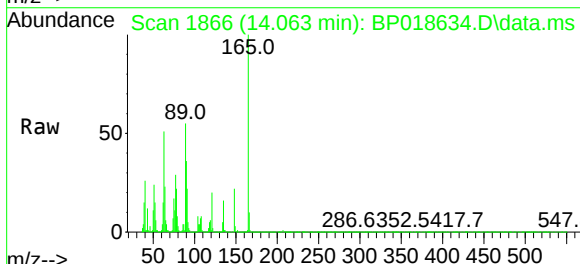




#50
Acenaphthylene
Concen: 34.508 ng/ul
RT: 14.204 min Scan# 1890
Delta R.T. 0.000 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30




Instrument :
BNA_P
ClientSampleId :
E05N2MS


Tgt Ion:152 Resp: 2154530
Ion Ratio Lower Upper
152 100
151 20.0 15.9 23.9
153 13.6 10.6 16.0

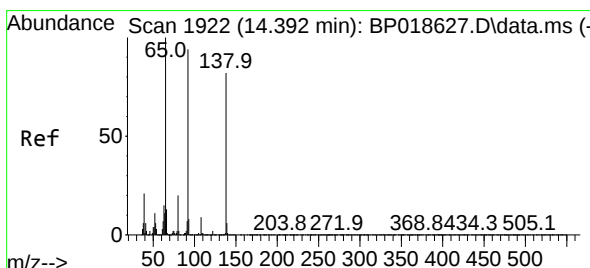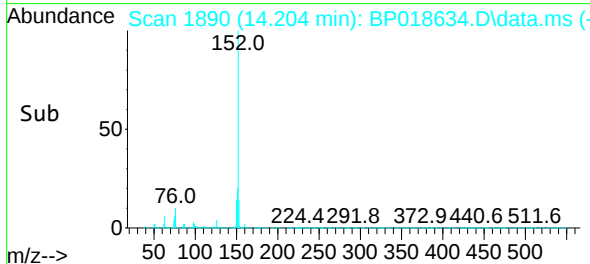

#51
3-Nitroaniline
Concen: 33.189 ng/ul
RT: 14.392 min Scan# 1922
Delta R.T. 0.000 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30

Tgt Ion:138 Resp: 310730
Ion Ratio Lower Upper
138 100
108 11.6 9.5 14.3
92 114.6 93.1 139.7

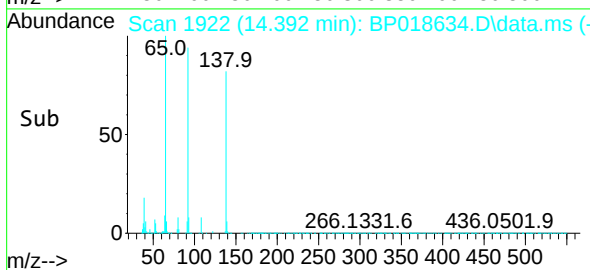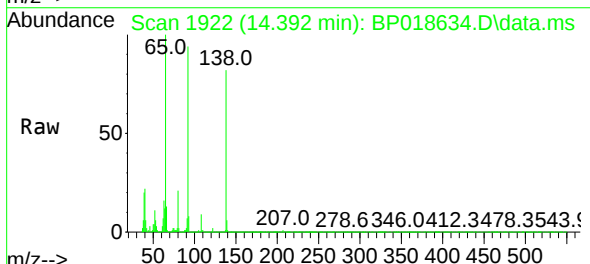



#52

Acenaphthene

Concen: 34.036 ng/ul

RT: 14.545 min Scan# 1948

Delta R.T. -0.006 min

Lab File: BP018634.D

Acq: 06 Dec 2023 13:30

Instrument :

BNA_P

ClientSampleId :

E05N2MS





Tgt Ion:153 Resp: 1405064

Ion Ratio Lower Upper

153 100

152 47.3 38.1 57.1

154 88.3 71.7 107.5

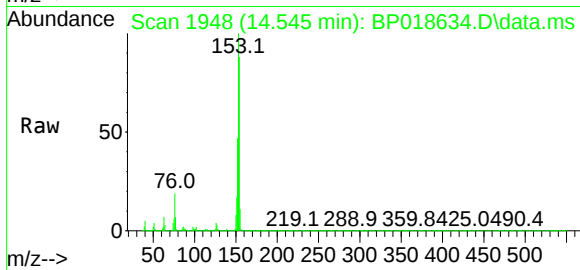

#53

2,4-Dinitrophenol

Concen: 20.536 ng/ul

RT: 14.598 min Scan# 1957

Delta R.T. 0.000 min

Lab File: BP018634.D

Acq: 06 Dec 2023 13:30




Tgt Ion:184 Resp: 102082


Ion Ratio Lower Upper

184 100

63 56.5 48.2 72.4

154 61.0 49.1 73.7



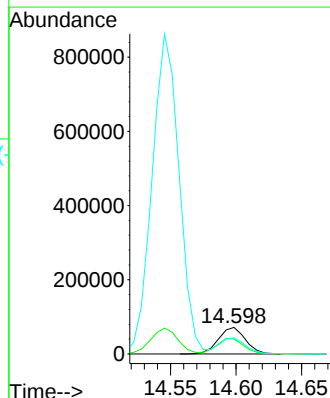
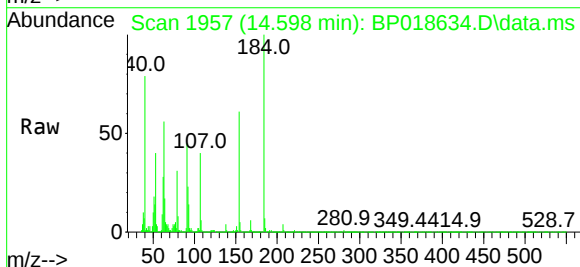




#55
4-Nitrophenol
Concen: 32.304 ng/ul
RT: 14.698 min Scan# 1974
Delta R.T. 0.000 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30




Instrument :
BNA_P
ClientSampleId :
E05N2MS


Tgt Ion:109 Resp: 202039
Ion Ratio Lower Upper
109 100
139 132.7 109.0 163.4
65 126.9 106.2 159.4

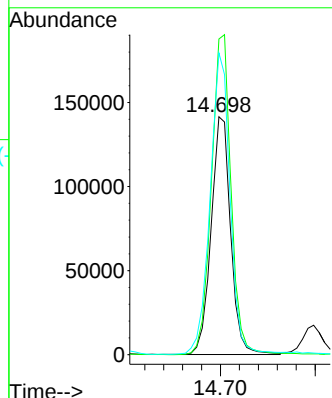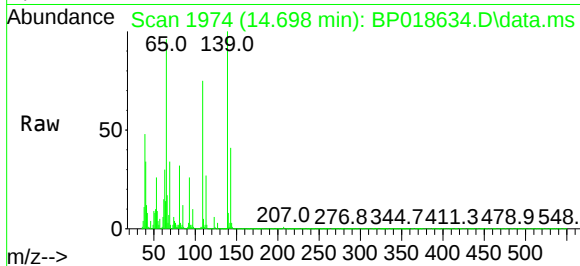

#56
Dibenzofuran
Concen: 32.870 ng/ul
RT: 14.881 min Scan# 2005
Delta R.T. 0.000 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30

Tgt Ion:168 Resp: 1885931
Ion Ratio Lower Upper
168 100
139 35.2 29.1 43.7



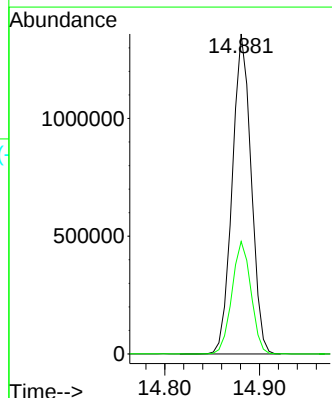
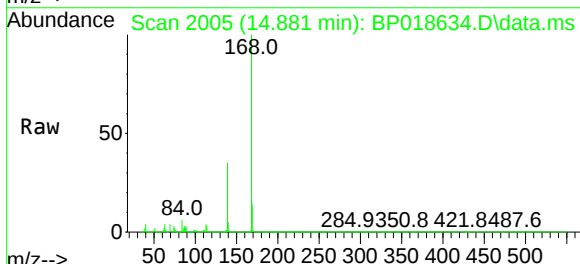




#57
2,4-Dinitrotoluene
Concen: 32.214 ng/ul
RT: 14.851 min Scan# 2000
Delta R.T. 0.000 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30




Instrument :
BNA_P
ClientSampleId :
E05N2MS


Tgt Ion:165 Resp: 425001
Ion Ratio Lower Upper
165 100
63 37.7 32.7 49.1
182 2.8 2.1 3.1



#58
2,3,4,6-Tetrachlorophenol
Concen: 29.323 ng/ul
RT: 15.104 min Scan# 2043
Delta R.T. -0.006 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30

Tgt Ion:232 Resp: 351672
Ion Ratio Lower Upper
232 100
131 39.9 33.8 50.8
130 2.2 1.8 2.8
166 29.8 24.7 37.1



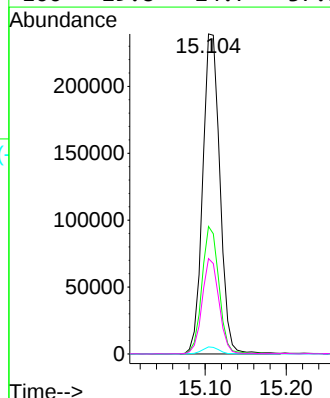





#59
Diethylphthalate
Concen: 28.094 ng/ul
RT: 15.310 min Scan# 2078
Delta R.T. -0.006 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30




Instrument :
BNA_P
ClientSampleId :
E05N2MS


Tgt Ion:149 Resp: 1364731
Ion Ratio Lower Upper
149 100
177 23.1 18.2 27.4
150 12.5 9.9 14.9

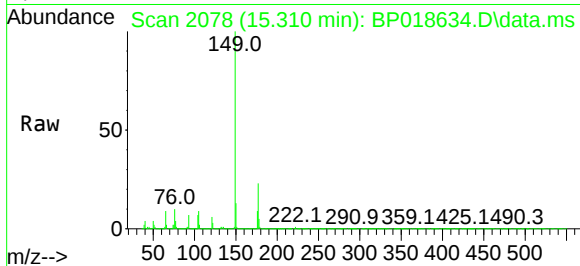

#61
Fluorene
Concen: 32.263 ng/ul
RT: 15.534 min Scan# 2116
Delta R.T. 0.000 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30

Tgt Ion:166 Resp: 1464729
Ion Ratio Lower Upper
166 100
165 97.0 78.0 117.0
167 13.3 10.8 16.2




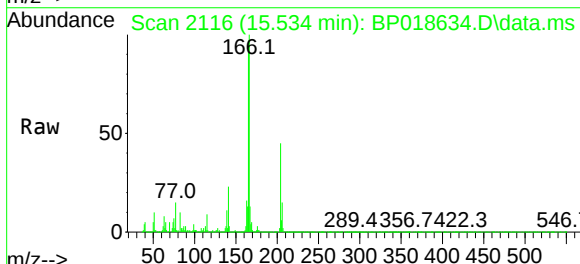




#62
4-Chlorophenyl-phenylether
Concen: 33.021 ng/ul
RT: 15.528 min Scan# 2115
Delta R.T. 0.000 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30




Instrument :
BNA_P
ClientSampleId :
E05N2MS


Tgt Ion:204 Resp: 786241
Ion Ratio Lower Upper
204 100
206 33.7 27.1 40.7
141 53.3 45.8 68.8

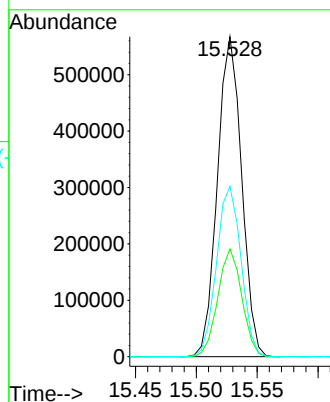

#63
4-Nitroaniline
Concen: 35.129 ng/ul
RT: 15.551 min Scan# 2119
Delta R.T. -0.006 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30

Tgt Ion:138 Resp: 313326
Ion Ratio Lower Upper
138 100
92 52.2 42.3 63.5
108 78.4 62.0 93.0


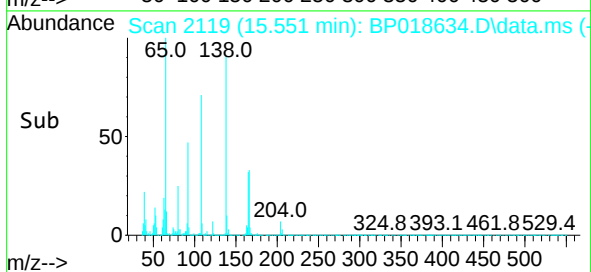
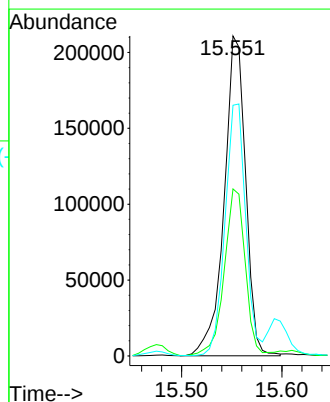
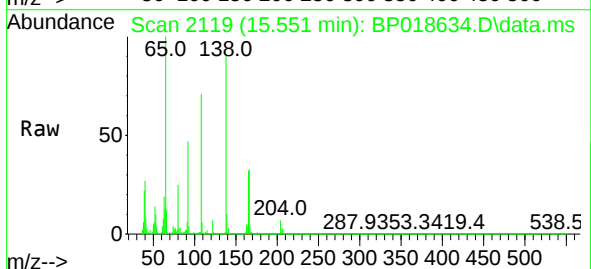




#66
 4,6-Dinitro-2-methylphenol
 Concen: 26.896 ng/ul
 RT: 15.610 min Scan# 2129
 Delta R.T. 0.000 min
 Lab File: BP018634.D
 Acq: 06 Dec 2023 13:30




Instrument :
 BNA_P
 ClientSampleId :
 E05N2MS


Tgt Ion:198 Resp: 183514
 Ion Ratio Lower Upper
 198 100
 182 4.1 3.4 5.2
 77 24.6 20.6 30.8

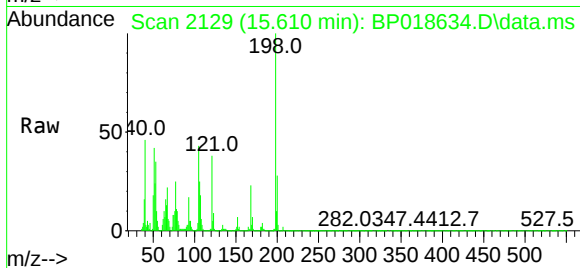

#67
 N-Nitrosodiphenylamine
 Concen: 34.784 ng/ul
 RT: 15.745 min Scan# 2152
 Delta R.T. 0.000 min
 Lab File: BP018634.D
 Acq: 06 Dec 2023 13:30

Tgt Ion:169 Resp: 1226791
 Ion Ratio Lower Upper
 169 100
 168 66.6 53.1 79.7
 167 36.3 29.1 43.7









#68
4-Bromophenyl-phenylether
Concen: 35.508 ng/ul
RT: 16.422 min Scan# 21
Delta R.T. 0.000 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30




Instrument :
BNA_P
ClientSampleId :
E05N2MS


Tgt Ion:248 Resp: 477117
Ion Ratio Lower Upper
248 100
250 95.6 79.3 118.9
141 65.3 57.2 85.8

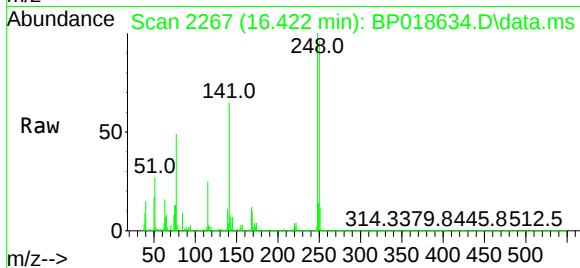

#69
Hexachlorobenzene
Concen: 35.778 ng/ul
RT: 16.534 min Scan# 2286
Delta R.T. 0.000 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30

Tgt Ion:284 Resp: 536753
Ion Ratio Lower Upper
284 100
142 30.9 25.8 38.6
249 31.2 24.9 37.3


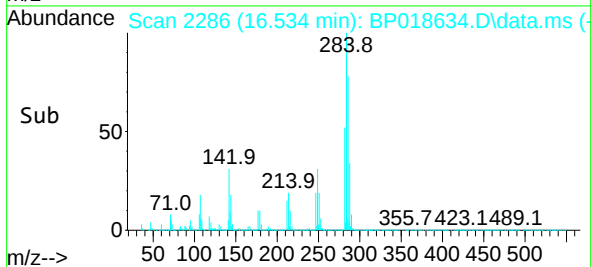

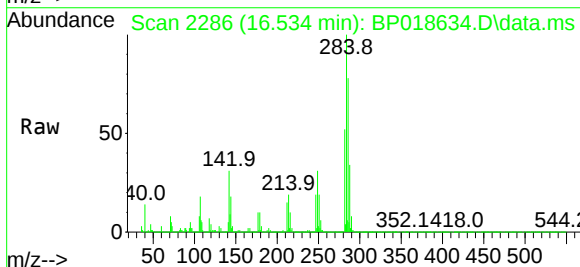




#70
Atrazine
Concen: 32.548 ng/ul
RT: 16.698 min Scan# 21
Delta R.T. 0.000 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30




Instrument :
BNA_P
ClientSampleId :
E05N2MS


Tgt Ion:200 Resp: 341290
Ion Ratio Lower Upper
200 100
173 25.3 21.0 31.4
215 48.9 38.2 57.2

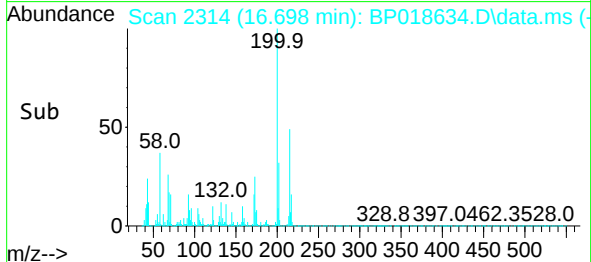

#71
Pentachlorophenol
Concen: 35.782 ng/ul
RT: 16.881 min Scan# 2345
Delta R.T. 0.000 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30

Tgt Ion:266 Resp: 319261
Ion Ratio Lower Upper
266 100
264 60.1 50.2 75.2
268 64.5 50.5 75.7





#72

Phenanthrene

Concen: 34.605 ng/u1

RT: 17.275 min Scan# 2411

Delta R.T. 0.000 min

Lab File: BP018634.D

Acq: 06 Dec 2023 13:30

Instrument :

BNA_P

ClientSampleId :

E05N2MS





Tgt Ion:178 Resp: 2224454

Ion Ratio Lower Upper

178 100

179 15.3 12.3 18.5

176 19.1 15.4 23.2



#74

Anthracene

Concen: 34.644 ng/u1

RT: 17.363 min Scan# 2427

Delta R.T. 0.000 min

Lab File: BP018634.D

Acq: 06 Dec 2023 13:30




Tgt Ion:178 Resp: 2232225


Ion Ratio Lower Upper

178 100

179 15.3 12.5 18.7

176 18.6 15.0 22.6


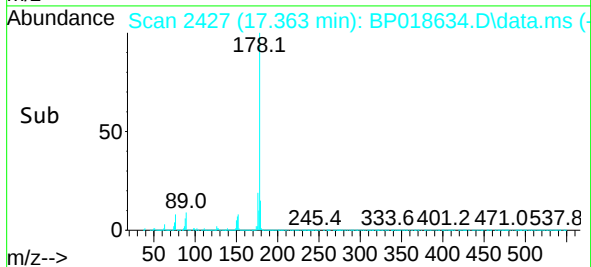

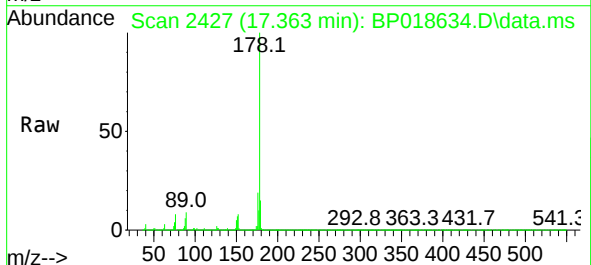




#75
1,2,3,4-Tetrachlorobenzene
Concen: 43.463 ng/uL
RT: 13.281 min Scan# 1733
Delta R.T. -0.006 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30




Instrument :
BNA_P
ClientSampleId :
E05N2MS


Tgt Ion:216 Resp: 799867
Ion Ratio Lower Upper
216 100
214 79.0 61.4 92.2
218 47.5 39.2 58.8

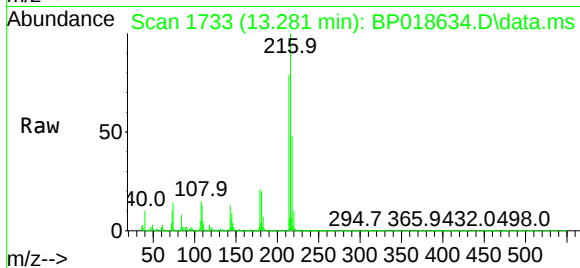

#76
Pentachlorobenzene
Concen: 39.138 ng/uL
RT: 14.798 min Scan# 1991
Delta R.T. 0.000 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30

Tgt Ion:250 Resp: 707519
Ion Ratio Lower Upper
250 100
248 63.3 50.6 75.8
252 62.7 51.3 76.9


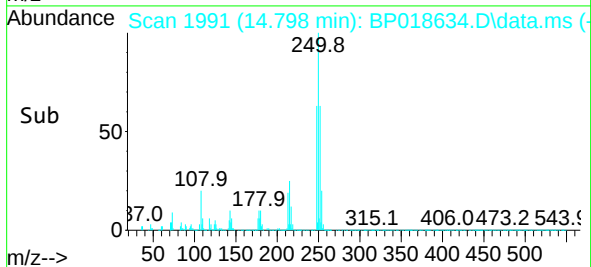

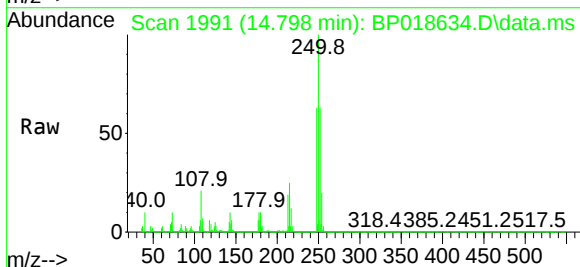




#77
Carbazole
Concen: 39.167 ng/ul
RT: 17.639 min Scan# 2474
Delta R.T. 0.000 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30




Instrument :
BNA_P
ClientSampleId :
E05N2MS


Tgt Ion:167 Resp: 2011337
Ion Ratio Lower Upper
167 100
166 21.1 17.1 25.7
139 12.0 10.2 15.4

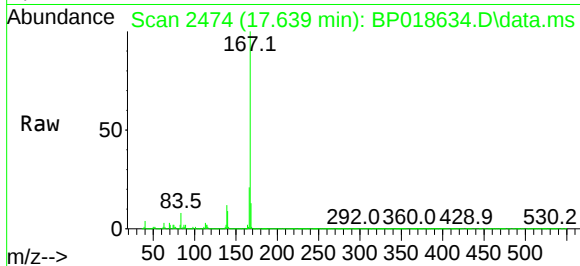

#78
Di-n-butylphthalate
Concen: 35.627 ng/ul
RT: 18.192 min Scan# 2568
Delta R.T. 0.000 min
Lab File: BP018634.D
Acq: 06 Dec 2023 13:30

Tgt Ion:149 Resp: 2436155
Ion Ratio Lower Upper
149 100
150 9.3 7.4 11.2
104 5.0 3.9 5.9

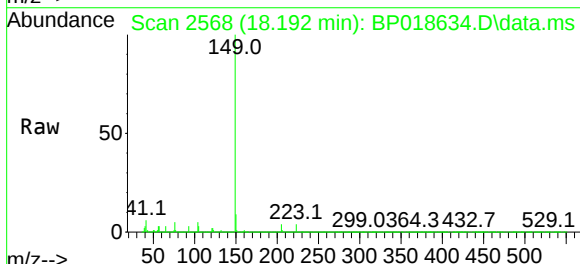



#80

Fluoranthene

Concen: 26.428 ng/ul

RT: 19.239 min Scan# 21

Delta R.T. 0.000 min

Lab File: BP018634.D

Acq: 06 Dec 2023 13:30

Instrument :

BNA_P

ClientSampleId :

E05N2MS





Tgt Ion:202 Resp: 2760208

Ion Ratio Lower Upper

202 100

101 10.8 9.1 13.7

100 8.4 7.1 10.7

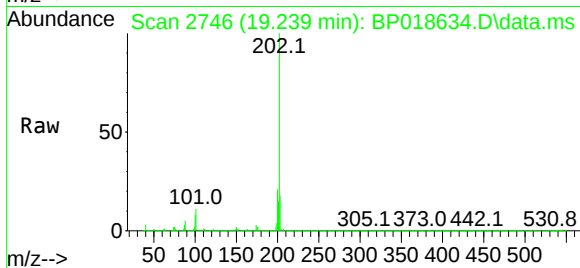

#82

Pyrene

Concen: 27.251 ng/ul

RT: 19.592 min Scan# 2806

Delta R.T. 0.000 min

Lab File: BP018634.D

Acq: 06 Dec 2023 13:30




Tgt Ion:202 Resp: 2871223


Ion Ratio Lower Upper

202 100

101 12.8 11.0 16.4

100 10.4 9.1 13.7

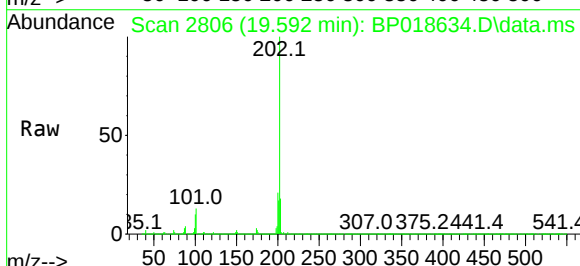



#83

Butylbenzylphthalate

Concen: 30.284 ng/ul

RT: 20.474 min Scan# 2955

Delta R.T. 0.000 min

Lab File: BP018634.D

Acq: 06 Dec 2023 13:30

Instrument :

BNA_P

ClientSampleId :

E05N2MS





Tgt Ion:149 Resp: 1168115

Ion Ratio Lower Upper

149 100

91 65.9 56.6 85.0

206 22.4 17.4 26.0



#84

3,3'-Dichlorobenzidine

Concen: 31.626 ng/ul

RT: 21.239 min Scan# 3086

Delta R.T. 0.000 min

Lab File: BP018634.D

Acq: 06 Dec 2023 13:30




Tgt Ion:252 Resp: 872365


Ion Ratio Lower Upper

252 100

254 65.1 51.0 76.4

126 10.0 7.8 11.6





#85

Benzo(a)anthracene

Concen: 34.032 ng/ul

RT: 21.304 min Scan# 3097

Delta R.T. 0.000 min

Lab File: BP018634.D

Acq: 06 Dec 2023 13:30

Instrument :

BNA_P

ClientSampleId :

E05N2MS





Tgt Ion:228 Resp: 3135435

Ion Ratio Lower Upper

228 100

229 19.8 15.7 23.5

226 27.7 21.9 32.9



#86

Bis(2-ethylhexyl)phthalate

Concen: 29.818 ng/ul

RT: 21.233 min Scan# 3085

Delta R.T. 0.000 min

Lab File: BP018634.D

Acq: 06 Dec 2023 13:30




Tgt Ion:149 Resp: 1580847


Ion Ratio Lower Upper

149 100

167 28.4 22.2 33.2

279 5.1 3.3 4.9#





#87

Chrysene

Concen: 34.254 ng/ul

RT: 21.357 min Scan# 3105

Delta R.T. 0.006 min

Lab File: BP018634.D

Acq: 06 Dec 2023 13:30

Instrument :

BNA_P

ClientSampleId :

E05N2MS





Tgt Ion:228 Resp: 2906220

Ion Ratio Lower Upper

228 100

226 29.8 23.9 35.9

229 19.8 15.6 23.4



#89

Di-n-octyl phthalate

Concen: 31.319 ng/ul




RT: 22.145 min Scan# 3240


Delta R.T. -0.006 min

Lab File: BP018634.D

Acq: 06 Dec 2023 13:30

Tgt Ion:149 Resp: 3175196

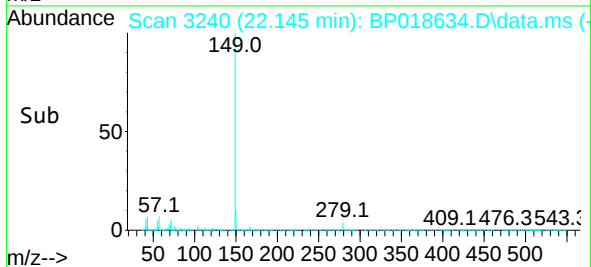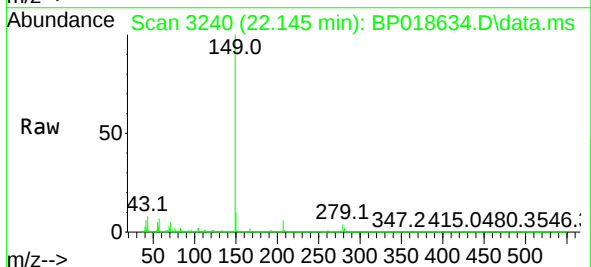



#90

Benzo(b)fluoranthene

Concen: 32.710 ng/ul

RT: 22.968 min Scan# 3380

Delta R.T. 0.006 min

Lab File: BP018634.D

Acq: 06 Dec 2023 13:30

Instrument :

BNA_P

ClientSampleId :

E05N2MS





Tgt Ion:252 Resp: 3348861

Ion Ratio Lower Upper

252 100

253 21.8 17.3 25.9

125 9.2 7.8 11.6



#91

Benzo(k)fluoranthene

Concen: 32.640 ng/ul

RT: 23.016 min Scan# 3388

Delta R.T. 0.000 min

Lab File: BP018634.D

Acq: 06 Dec 2023 13:30




Tgt Ion:252 Resp: 3233205


Ion Ratio Lower Upper

252 100

253 21.6 17.7 26.5

125 9.3 8.0 12.0



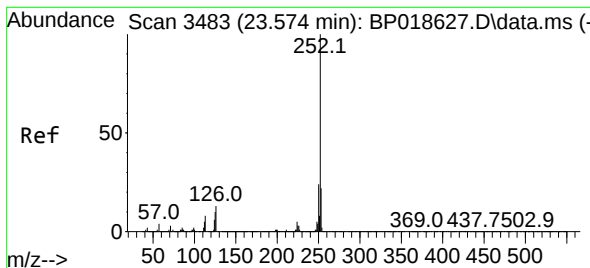

#93

Benzo(a)pyrene

Concen: 33.917 ng/ul

RT: 23.586 min Scan# 34

Delta R.T. 0.000 min

Lab File: BP018634.D

Acq: 06 Dec 2023 13:30

Instrument :

BNA_P

ClientSampleId :

E05N2MS





Tgt Ion:252 Resp: 3172841

Ion Ratio Lower Upper

252 100

253 21.7 17.8 26.8

125 10.6 9.2 13.8

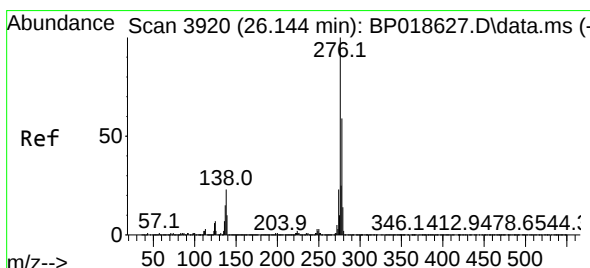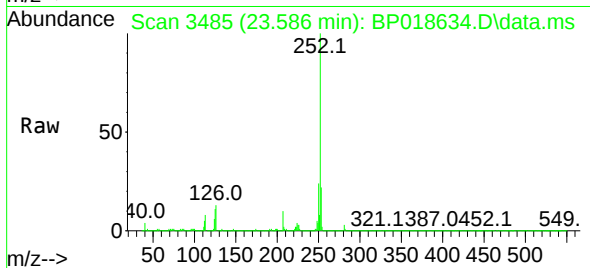

#94

Indeno(1,2,3-cd)pyrene

Concen: 36.059 ng/ul

RT: 26.162 min Scan# 3923

Delta R.T. 0.006 min

Lab File: BP018634.D

Acq: 06 Dec 2023 13:30




Tgt Ion:276 Resp: 4030273


Ion Ratio Lower Upper

276 100

138 22.1 19.4 29.2

277 25.0 19.8 29.6

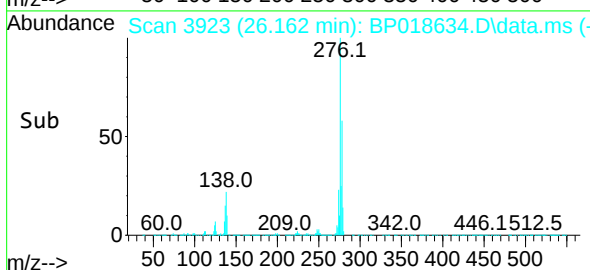

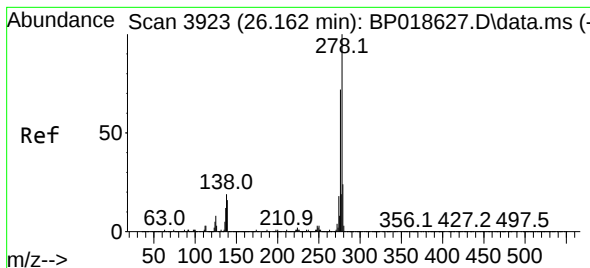

#95

Dibenzo(a,h)anthracene

Concen: 36.121 ng/ul

RT: 26.186 min Scan# 3923

Delta R.T. 0.006 min

Lab File: BP018634.D

Acq: 06 Dec 2023 13:30

Instrument :

BNA_P

ClientSampleId :

E05N2MS





Tgt Ion:278 Resp: 3358389

Ion Ratio Lower Upper

278 100

139 14.3 13.0 19.6

279 23.7 18.7 28.1

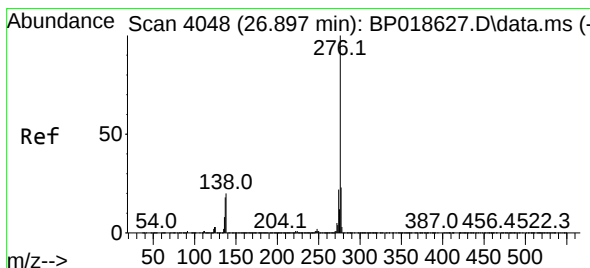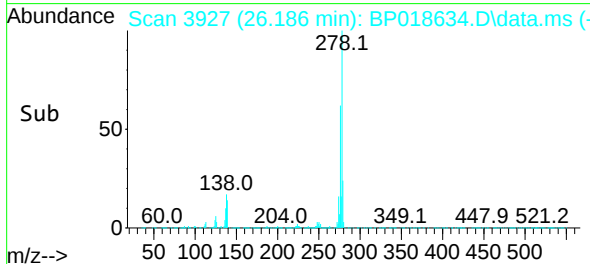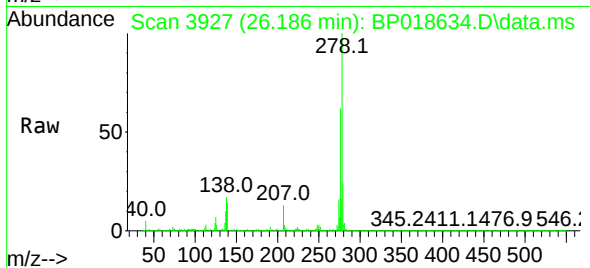

#96

Benzo(g,h,i)perylene

Concen: 36.292 ng/ul

RT: 26.921 min Scan# 4052

Delta R.T. 0.006 min

Lab File: BP018634.D

Acq: 06 Dec 2023 13:30

Tgt Ion:276 Resp: 3264418

Ion Ratio Lower Upper

276 100

138 19.4 18.1 27.1

277 23.7 19.4 29.0

