

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018555.D
 Acq On : 04 Dec 2023 09:48
 Operator : MA/JU
 Sample : PB157364BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK364

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018555.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	39	rVB	123385	153278	2.17%	0.184%
2	3.687	98	102	119	rBV	1350937	1878690	26.60%	2.250%
3	4.022	155	159	165	rBV2	23037	33181	0.47%	0.040%
4	7.022	662	669	679	rVB	1568401	2380146	33.70%	2.851%
5	7.193	690	698	707	rBV	1350863	2052681	29.06%	2.459%
6	7.387	721	731	739	rBV	1550803	2405730	34.06%	2.882%
7	7.858	803	811	820	rBV	1332012	2067099	29.27%	2.476%
8	8.563	922	931	941	rBV	1910906	3040274	43.05%	3.642%
9	8.746	960	962	965	rBV	5213	7505	0.11%	0.009%
10	9.016	1000	1008	1016	rBV	1497636	2344529	33.20%	2.808%
11	9.440	1076	1080	1083	rVB4	5964	7353	0.10%	0.009%
12	9.740	1120	1131	1140	rBV	1071025	1746704	24.73%	2.092%
13	10.275	1212	1222	1233	rBV	1870601	3056306	43.27%	3.661%
14	10.652	1277	1286	1294	rVB	1791885	3036022	42.99%	3.637%
15	10.793	1303	1310	1323	rBV	1513616	2517052	35.64%	3.015%
16	11.928	1496	1503	1504	rBV6	5684	7808	0.11%	0.009%
17	12.240	1550	1556	1562	rVB2	37618	60952	0.86%	0.073%
18	13.387	1747	1751	1757	rBV5	18413	28904	0.41%	0.035%
19	13.457	1759	1763	1767	rBV7	5457	8967	0.13%	0.011%
20	13.904	1831	1839	1847	rBV	3506185	4805854	68.05%	5.756%
21	14.181	1878	1886	1900	rBV	3970434	5707331	80.81%	6.836%
22	14.487	1931	1938	1946	rBV	2935566	4189544	59.32%	5.018%
23	14.681	1963	1971	1982	rBV	1260557	1798946	25.47%	2.155%
24	14.898	2004	2008	2010	rBV4	5670	7064	0.10%	0.008%
25	15.475	2100	2106	2113	rBV	4794608	7062581	100.00%	8.460%
26	15.592	2119	2126	2139	rBV	1029983	1394535	19.75%	1.670%
27	15.716	2144	2147	2154	rVV2	27145	46871	0.66%	0.056%
28	16.039	2198	2202	2204	rBV4	6141	7725	0.11%	0.009%
29	16.910	2347	2350	2354	rVB2	8896	12460	0.18%	0.015%
30	17.016	2366	2368	2373	rVB4	7108	9479	0.13%	0.011%
31	17.234	2398	2405	2413	rBV	3205612	4430601	62.73%	5.307%
32	17.334	2415	2422	2436	rVV	4762828	6866545	97.22%	8.225%
33	19.145	2726	2730	2735	rBV3	52458	71808	1.02%	0.086%
34	19.210	2737	2741	2745	rBV2	52886	71222	1.01%	0.085%
35	19.563	2796	2801	2812	rBV	4975630	6730506	95.30%	8.062%
36	21.316	3094	3099	3107	rBV	2906935	3570643	50.56%	4.277%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018555.D
Acq On : 04 Dec 2023 09:48
Operator : MA/JU
Sample : PB157364BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK364

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Title : SVOA CALIBRATION

37	23.539	3470	3477	3485	rBV	3263868	6048617	85.64%	7.245%
38	23.686	3496	3502	3512	rVB	1963232	3820598	54.10%	4.576%




Sum of corrected areas: 83486111

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018555.D
Acq On : 04 Dec 2023 09:48
Operator : MA/JU
Sample : PB157364BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK364

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

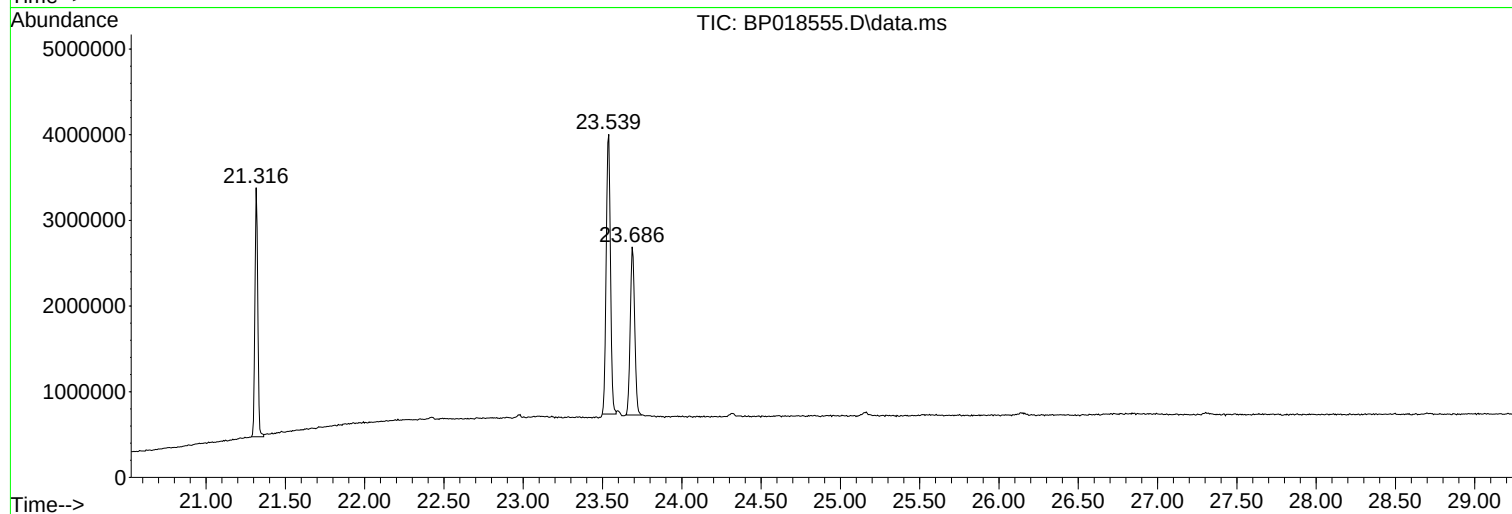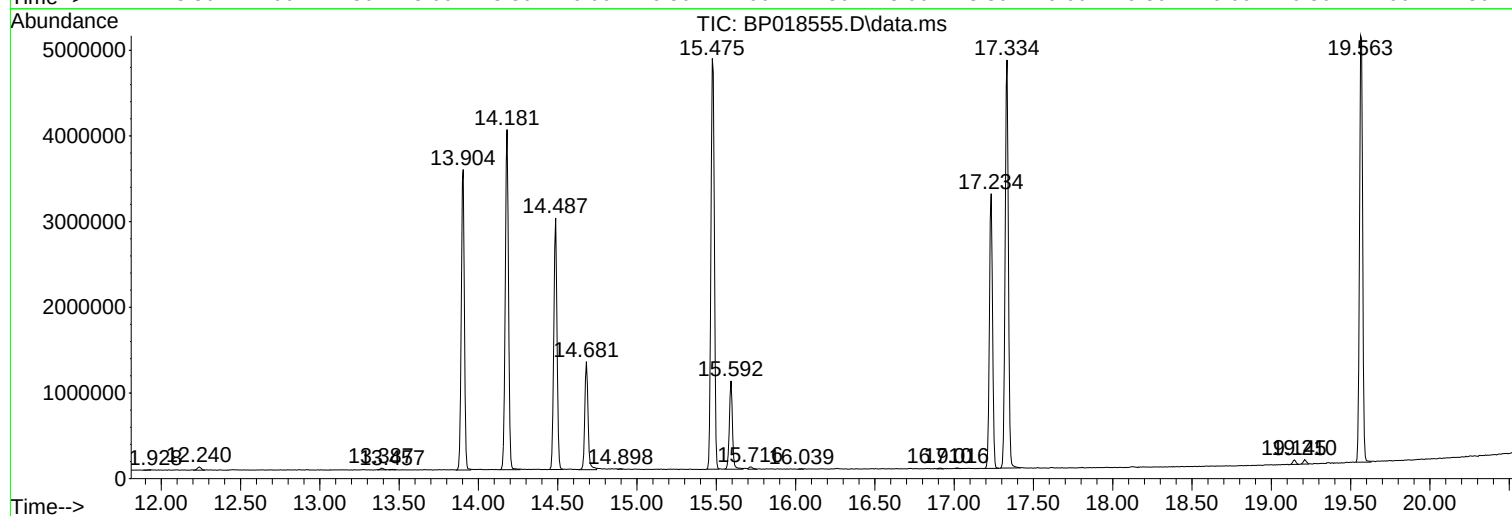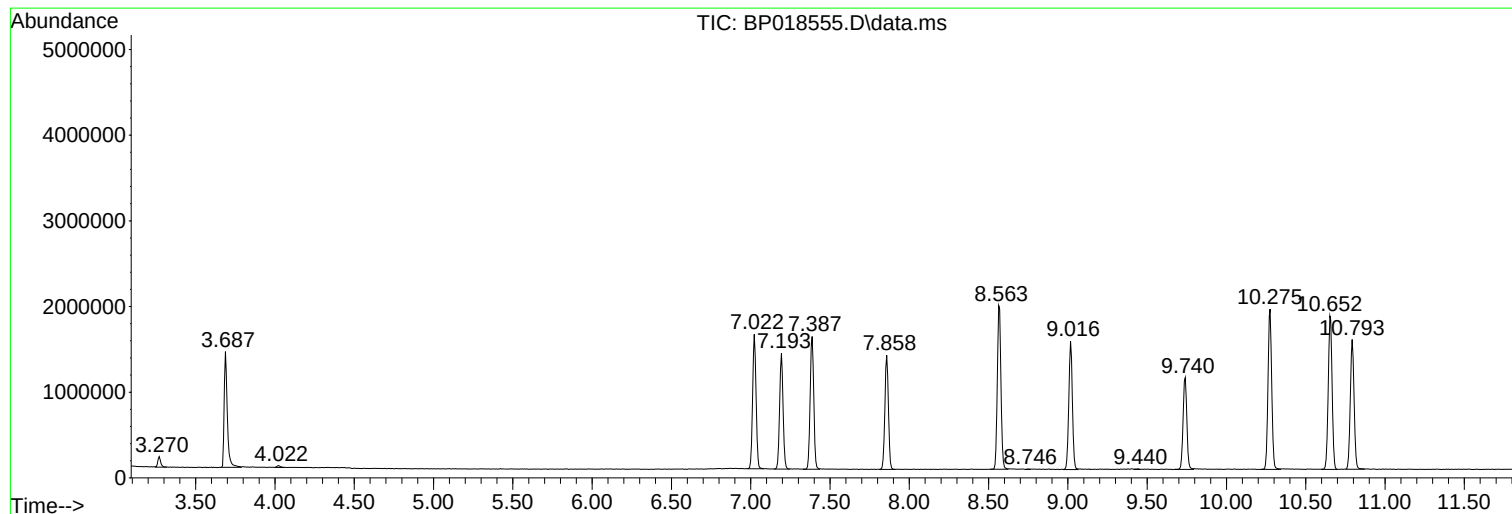

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018555.D
Acq On : 04 Dec 2023 09:48
Operator : MA/JU
Sample : PB157364BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK364

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018555.D
Acq On : 04 Dec 2023 09:48
Operator : MA/JU
Sample : PB157364BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK364

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------