

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018557.D
 Acq On : 04 Dec 2023 10:56
 Operator : MA/JU
 Sample : 05439-19
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018557.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	27	31	36	rVB	78582	92684	0.89%	0.099%
2	3.687	99	102	114	rBV	478660	710313	6.80%	0.758%
3	3.928	139	143	147	rVB	19632	27901	0.27%	0.030%
4	4.023	155	159	164	rVB2	26638	36233	0.35%	0.039%
5	4.458	231	233	238	rVB4	12542	18494	0.18%	0.020%
6	7.022	663	669	677	rVB	349933	525231	5.03%	0.561%
7	7.193	689	698	707	rBV	1308273	2016060	19.30%	2.152%
8	7.387	723	731	742	rBV	1211637	1894004	18.13%	2.022%
9	7.469	742	745	756	rVB3	22338	44181	0.42%	0.047%
10	7.858	803	811	818	rBV	1341857	2130488	20.39%	2.275%
11	7.922	818	822	827	rBV4	7121	14334	0.14%	0.015%
12	8.293	879	885	887	rBV3	6756	11040	0.11%	0.012%
13	8.563	922	931	939	rBV	1066513	1649612	15.79%	1.761%
14	8.752	957	963	967	rBV3	12201	27142	0.26%	0.029%
15	9.016	1001	1008	1017	rBV	1510892	2396973	22.94%	2.559%
16	9.446	1074	1081	1082	rBV4	11905	18135	0.17%	0.019%
17	9.734	1123	1130	1140	rBV	1114197	1813422	17.36%	1.936%
18	10.269	1214	1221	1229	rBV	1876893	3075539	29.44%	3.284%
19	10.522	1259	1264	1269	rBV2	51240	79732	0.76%	0.085%
20	10.652	1277	1286	1293	rBV	1984845	3310767	31.69%	3.535%
21	10.710	1293	1296	1300	rVB5	10797	14848	0.14%	0.016%
22	10.793	1300	1310	1319	rBV	1835644	3036880	29.07%	3.242%
23	11.057	1350	1355	1361	rVB6	9853	20745	0.20%	0.022%
24	11.122	1361	1366	1374	rBV6	6024	12736	0.12%	0.014%
25	11.410	1410	1415	1418	rBV2	9283	14794	0.14%	0.016%
26	11.469	1418	1425	1429	rBV3	8502	21469	0.21%	0.023%
27	12.240	1549	1556	1563	rBV2	41079	75715	0.72%	0.081%
28	13.393	1747	1752	1758	rVB2	28453	47062	0.45%	0.050%
29	13.451	1760	1762	1765	rVV2	8546	11316	0.11%	0.012%
30	13.899	1832	1838	1849	rBV	3734304	5220116	49.96%	5.573%
31	14.181	1878	1886	1894	rBV	4392124	6362241	60.90%	6.793%
32	14.487	1931	1938	1946	rBV	3324676	4876768	46.68%	5.207%
33	14.681	1965	1971	1980	rBV	299683	444539	4.25%	0.475%
34	14.846	1995	1999	2001	rVV4	7932	11130	0.11%	0.012%
35	14.893	2005	2007	2013	rVB3	13969	23781	0.23%	0.025%
36	15.475	2100	2106	2113	rBV	5790302	8368873	80.10%	8.935%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018557.D
 Acq On : 04 Dec 2023 10:56
 Operator : MA/JU
 Sample : 05439-19
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	15.593	2120	2126	2136	rBV	1635674	2120760	20.30%	2.264%
38	15.716	2143	2147	2151	rVB3	23058	30908	0.30%	0.033%
39	16.045	2199	2203	2207	rBV2	11094	19875	0.19%	0.021%
40	16.257	2236	2239	2243	rVB4	10940	16577	0.16%	0.018%
41	16.598	2293	2297	2300	rVB2	6791	10773	0.10%	0.012%
42	17.016	2361	2368	2373	rBV4	13219	33113	0.32%	0.035%
43	17.104	2378	2383	2384	rBV	9172	12901	0.12%	0.014%
44	17.234	2398	2405	2411	rBV	4095915	5783589	55.36%	6.175%
45	17.334	2415	2422	2432	rBV	6418133	9313806	89.15%	9.944%
46	17.910	2516	2520	2526	rVB3	31438	42002	0.40%	0.045%
47	18.122	2552	2556	2563	rBV3	150955	214301	2.05%	0.229%
48	19.045	2709	2713	2718	rVB6	51207	63840	0.61%	0.068%
49	19.145	2726	2730	2734	rBV	89134	114428	1.10%	0.122%
50	19.210	2737	2741	2745	rBV	80913	102490	0.98%	0.109%
51	19.357	2762	2766	2769	rBV3	62329	77604	0.74%	0.083%
52	19.569	2796	2802	2813	rBV	7911020	10447700	100.00%	11.154%
53	21.039	3049	3052	3060	rBV4	121242	187068	1.79%	0.200%
54	21.316	3094	3099	3111	rBV	3975989	5021684	48.06%	5.361%
55	23.539	3470	3477	3485	rBV2	3773216	7300721	69.88%	7.795%
56	23.692	3497	3503	3513	rVB	2147192	4295251	41.11%	4.586%




Sum of corrected areas: 93664689

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018557.D
Acq On : 04 Dec 2023 10:56
Operator : MA/JU
Sample : 05439-19
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AE1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

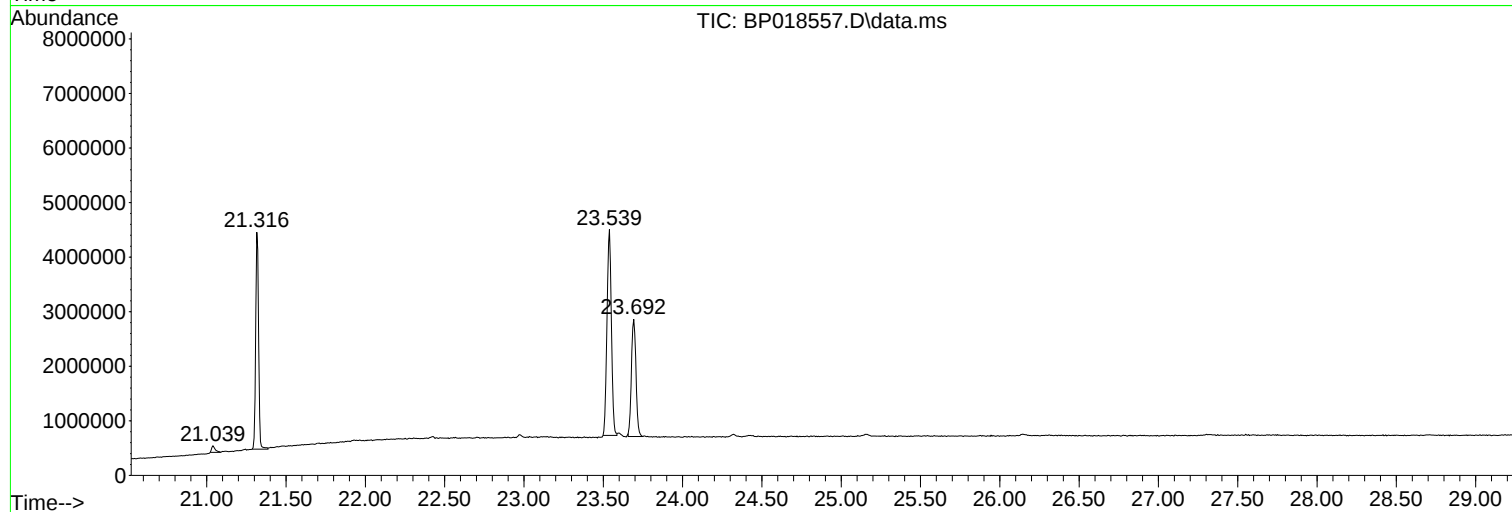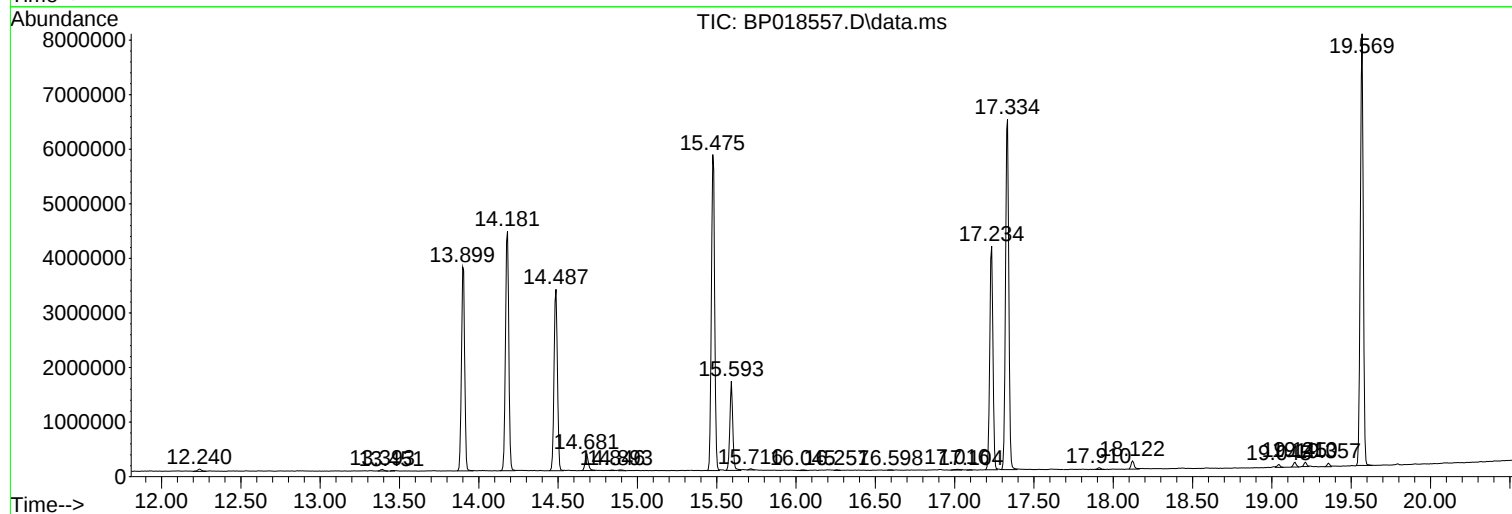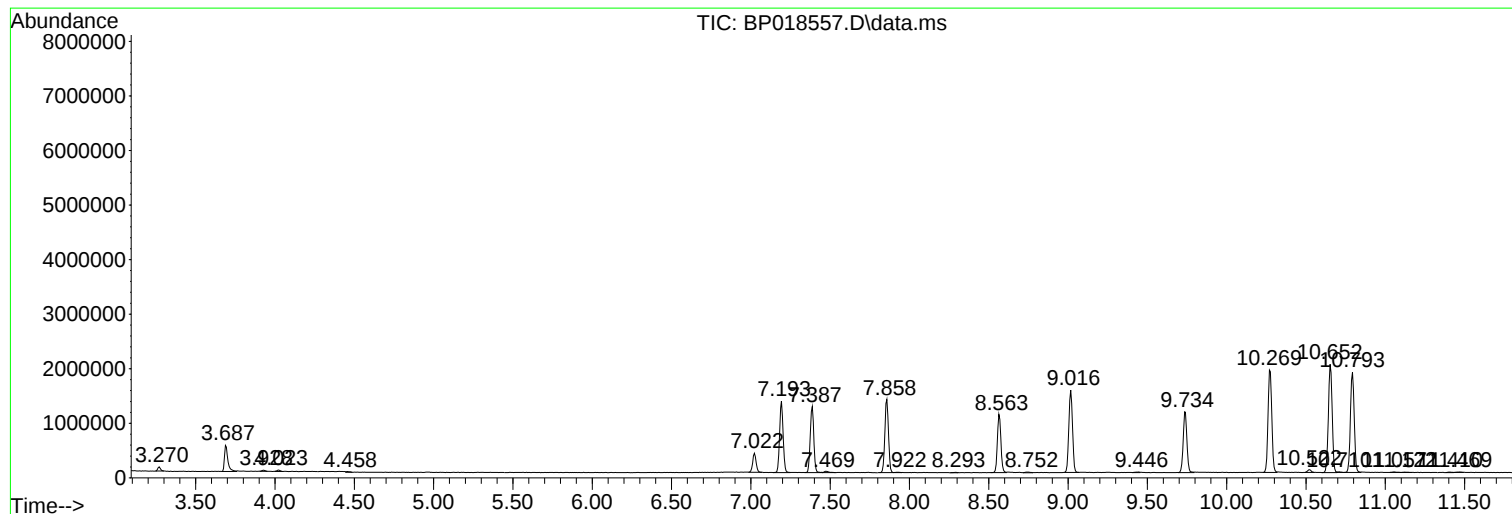

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018557.D
Acq On : 04 Dec 2023 10:56
Operator : MA/JU
Sample : 05439-19
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AE1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018557.D
Acq On : 04 Dec 2023 10:56
Operator : MA/JU
Sample : 05439-19
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AE1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc