

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018558.D
 Acq On : 04 Dec 2023 11:30
 Operator : MA/JU
 Sample : 05439-20
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AK5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP018558.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.270	28	31	39	rVB	74705	95475	1.15%	0.121%
2	3.693	99	103	119	rBV	381728	569006	6.87%	0.721%
3	3.928	140	143	148	rVB3	24434	29637	0.36%	0.038%
4	4.022	155	159	163	rVB	33906	40882	0.49%	0.052%
5	4.399	221	223	227	rVB5	7873	8812	0.11%	0.011%
6	5.787	454	459	463	rBV3	10811	14533	0.18%	0.018%
7	5.863	469	472	477	rVB2	6280	10418	0.13%	0.013%
8	5.911	477	480	486	rVV4	5735	10626	0.13%	0.013%
9	5.958	486	488	494	rVB5	7713	11666	0.14%	0.015%
10	7.022	662	669	675	rVB	301625	460328	5.56%	0.584%
11	7.193	691	698	706	rBV	1222800	1853549	22.37%	2.350%
12	7.387	724	731	739	rBV	1080384	1673470	20.20%	2.122%
13	7.487	743	748	756	rVB5	9893	22825	0.28%	0.029%
14	7.857	801	811	818	rBV	1401415	2195818	26.51%	2.784%
15	7.928	818	823	827	rBV3	15363	24295	0.29%	0.031%
16	8.563	924	931	942	rBV	863899	1352930	16.33%	1.716%
17	9.016	1000	1008	1018	rBV	1330666	2120495	25.60%	2.689%
18	9.175	1032	1035	1041	rBV5	6874	15961	0.19%	0.020%
19	9.446	1079	1081	1086	rVB4	7553	8836	0.11%	0.011%
20	9.740	1121	1131	1142	rBV	886668	1448698	17.49%	1.837%
21	10.275	1214	1222	1232	rBV	1425707	2416571	29.17%	3.064%
22	10.340	1232	1233	1239	rVB2	7756	9774	0.12%	0.012%
23	10.651	1276	1286	1294	rBV	1867445	3149858	38.02%	3.994%
24	10.716	1294	1297	1301	rVB4	10048	14813	0.18%	0.019%
25	10.793	1301	1310	1318	rBV	1568238	2601153	31.40%	3.298%
26	12.240	1550	1556	1563	rBV3	29329	55802	0.67%	0.071%
27	12.675	1628	1630	1635	rVB2	7589	8961	0.11%	0.011%
28	13.228	1719	1724	1727	rVB2	6551	8943	0.11%	0.011%
29	13.393	1748	1752	1757	rVB4	15924	26073	0.31%	0.033%
30	13.898	1832	1838	1846	rBV	2902003	4022893	48.56%	5.101%
31	14.181	1875	1886	1894	rBV	3306432	4866265	58.74%	6.170%
32	14.487	1930	1938	1948	rBV	2857749	4188803	50.56%	5.311%
33	14.569	1948	1952	1957	rVV3	39811	57843	0.70%	0.073%
34	14.681	1965	1971	1982	rBV	177496	298272	3.60%	0.378%
35	14.904	2004	2009	2014	rVB7	13856	22777	0.27%	0.029%
36	15.157	2046	2052	2057	rBV3	18993	39561	0.48%	0.050%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
 Data File : BP018558.D
 Acq On : 04 Dec 2023 11:30
 Operator : MA/JU
 Sample : 05439-20
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AK5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
 Title : SVOA CALIBRATION

37	15.292	2070	2075	2077	rBV4	5872	9393	0.11%	0.012%
38	15.475	2097	2106	2113	rBV	4537931	6337862	76.50%	8.036%
39	15.592	2120	2126	2140	rBV	840001	1160242	14.01%	1.471%
40	15.716	2142	2147	2152	rVB3	20643	33852	0.41%	0.043%
41	16.828	2333	2336	2339	rBV2	8909	9384	0.11%	0.012%
42	16.904	2347	2349	2354	rVB5	7024	9541	0.12%	0.012%
43	17.233	2398	2405	2414	rVB	3008847	4361095	52.64%	5.530%
44	17.328	2415	2421	2435	rVV	4868011	6868525	82.91%	8.709%
45	17.422	2435	2437	2445	rVB6	14809	24281	0.29%	0.031%
46	17.904	2514	2519	2523	rBV2	207747	252070	3.04%	0.320%
47	18.122	2552	2556	2561	rBV5	21464	33223	0.40%	0.042%
48	19.145	2726	2730	2735	rVB2	56043	73040	0.88%	0.093%
49	19.210	2738	2741	2746	rVV2	52848	68246	0.82%	0.087%
50	19.569	2796	2802	2814	rBV	6077533	7776789	93.87%	9.861%
51	21.316	3094	3099	3105	rBV	3586821	4643629	56.05%	5.888%
52	23.539	3470	3477	3485	rBV2	4414682	8284435	100.00%	10.505%
53	23.692	3496	3503	3514	rVB	2627633	5162151	62.31%	6.546%




Sum of corrected areas: 78864380

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018558.D
Acq On : 04 Dec 2023 11:30
Operator : MA/JU
Sample : 05439-20
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AK5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

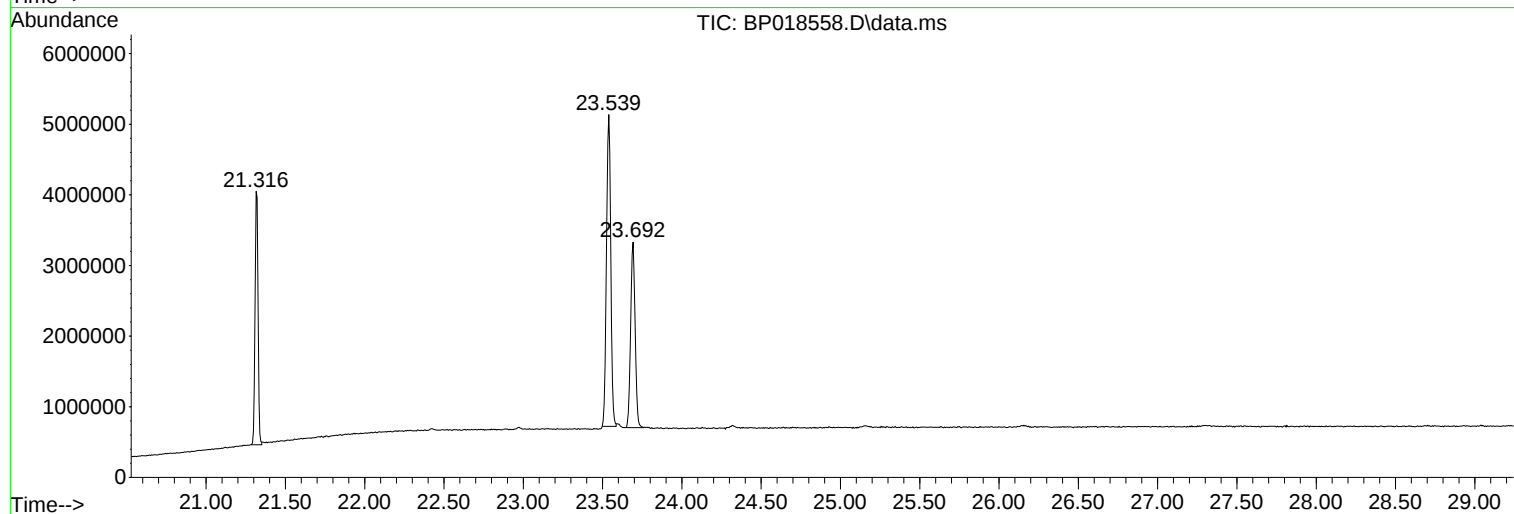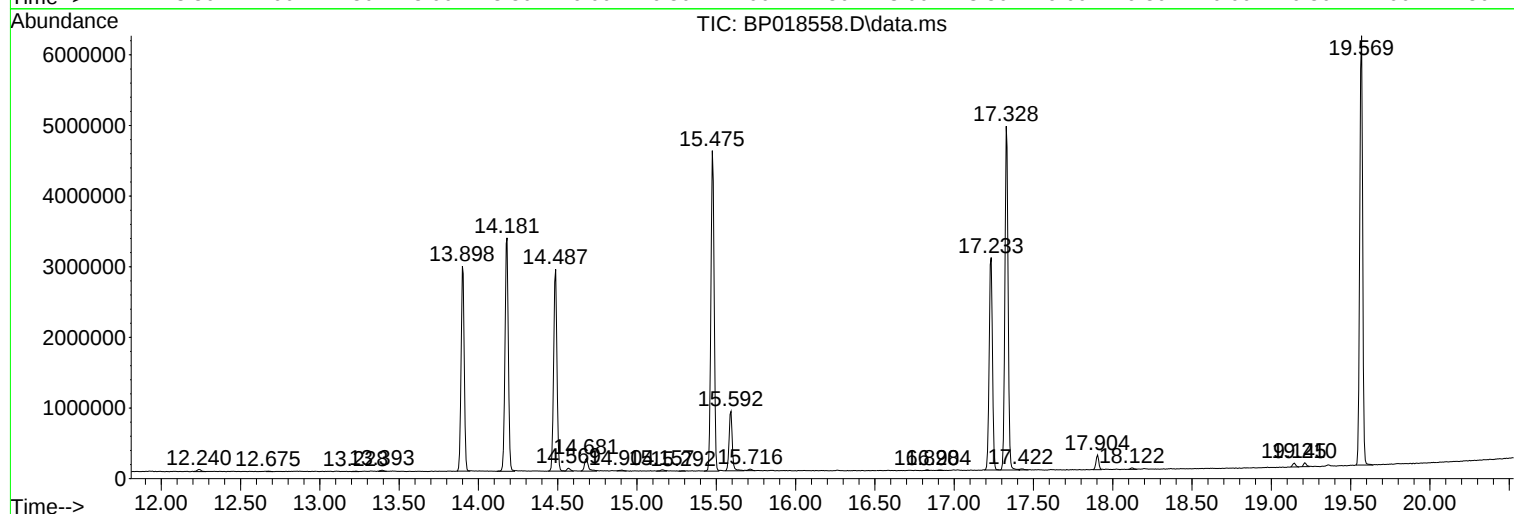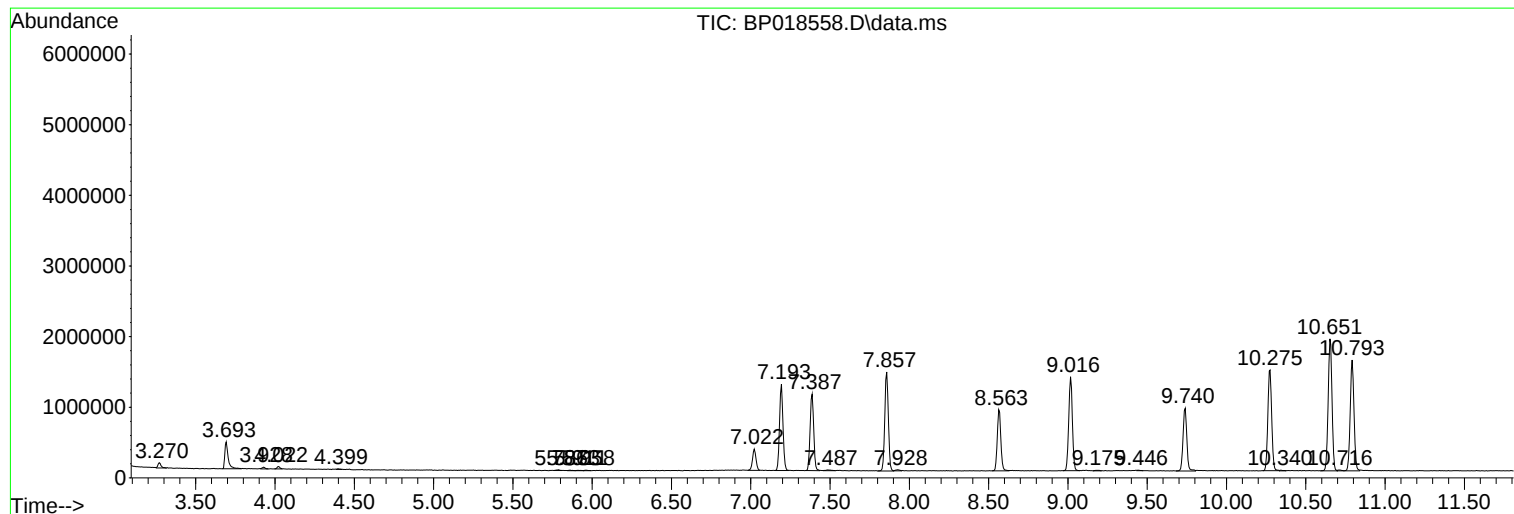

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018558.D
Acq On : 04 Dec 2023 11:30
Operator : MA/JU
Sample : 05439-20
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AK5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP120423\
Data File : BP018558.D
Acq On : 04 Dec 2023 11:30
Operator : MA/JU
Sample : 05439-20
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AK5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP120123.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc